

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092221\
 Data File : PQ054599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 13:54
 Operator : AJ\MA
 Sample : M3816-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MW-14-20210916-1-2-WC

Manual Integrations
 APPROVED

mohammad
 9/23/2021 1:36:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 17:21:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.200	4.207	475.7E6	248.0E6	19.919	18.760
2) SA Decachlor...	11.370	9.535	339.6E6	230.0E6	20.119m	16.974m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092221\
Data File : PQ054599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 13:54
Operator : AJ\MA
Sample : M3816-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
MW-14-20210916-1-2-WC


Manual Integrations
APPROVED

mohammad
9/23/2021 1:36:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 17:21:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

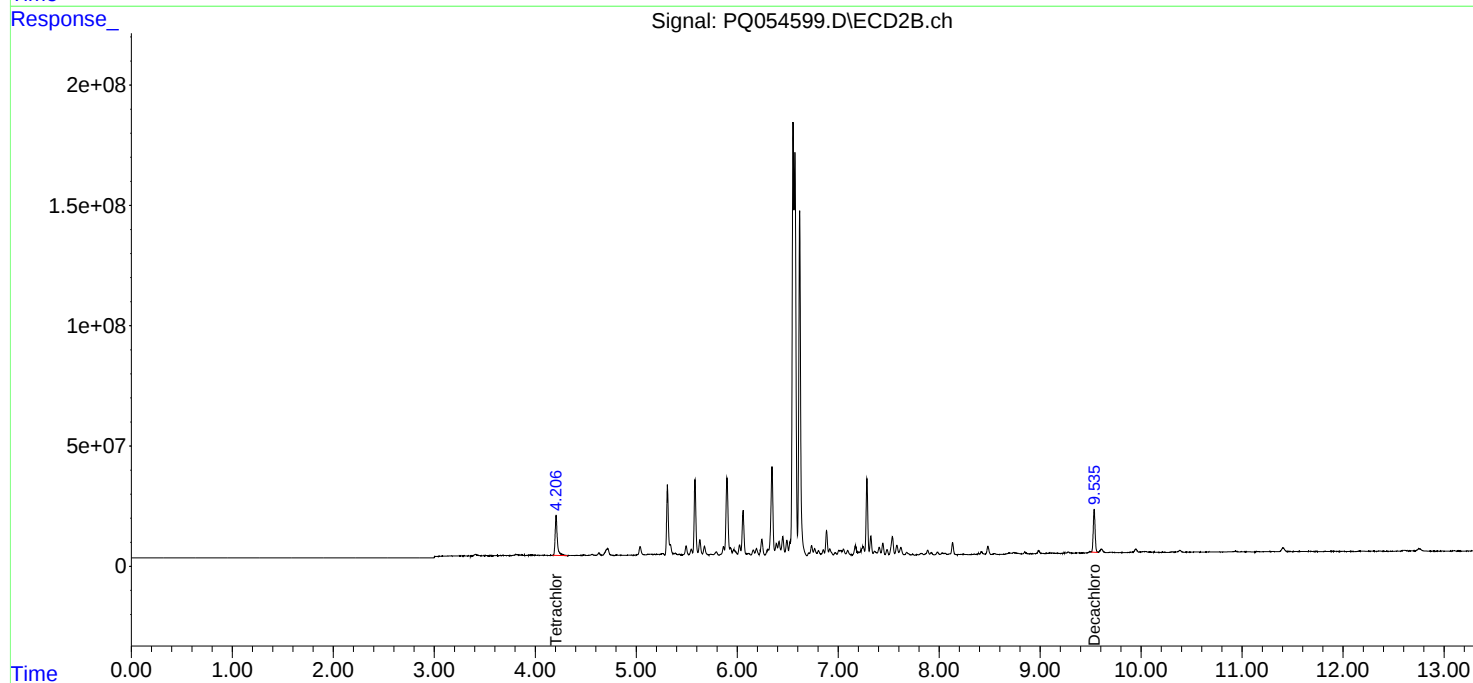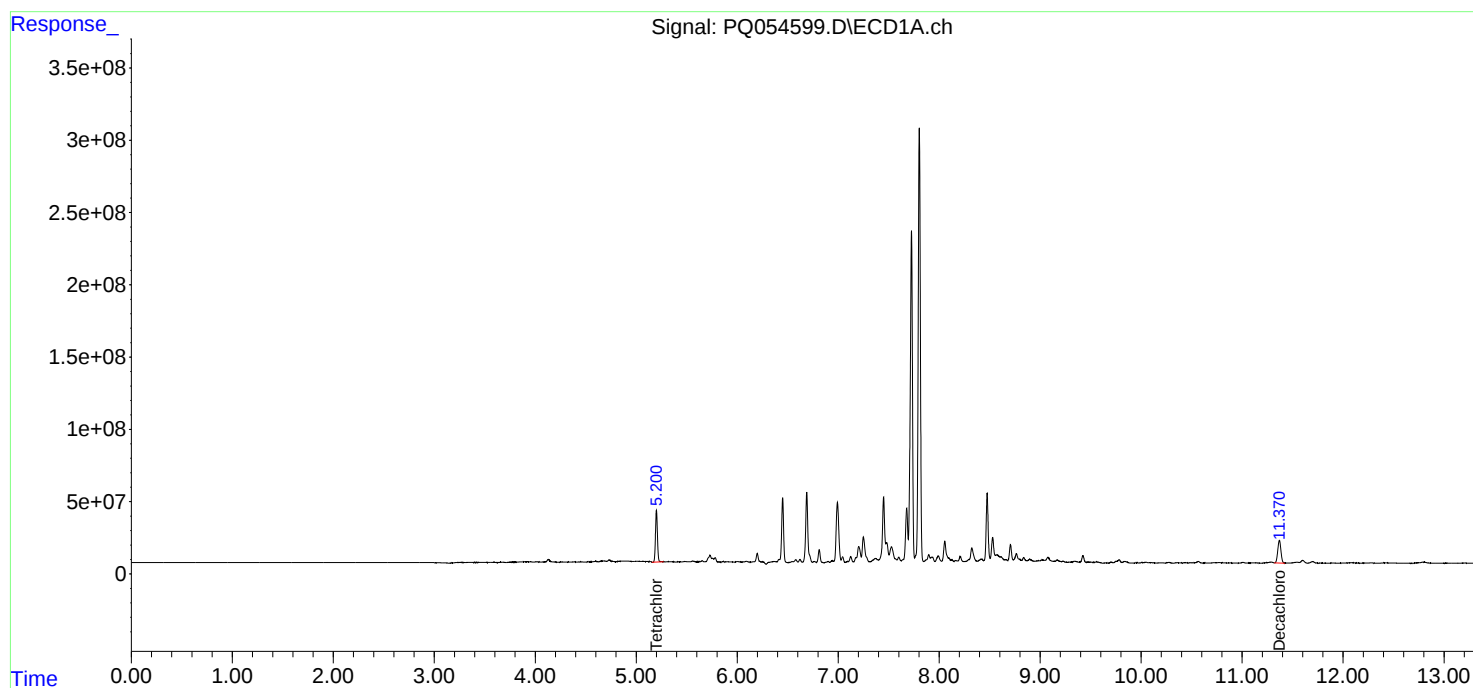

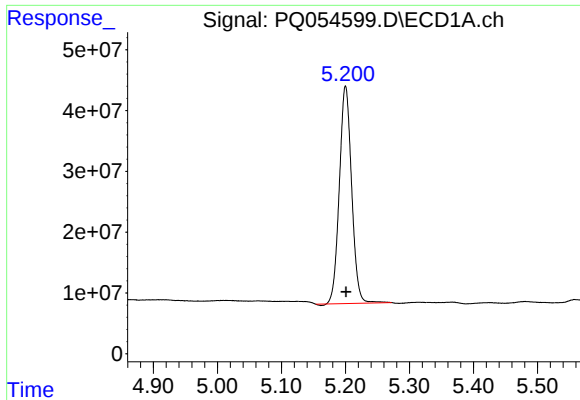


#1 Tetrachloro-m-xylene

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 475700332
Conc: 19.92 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MW-14-20210916-1-2-WC


Manual Integrations
APPROVED

mohammad
9/23/2021 1:36:13 PM

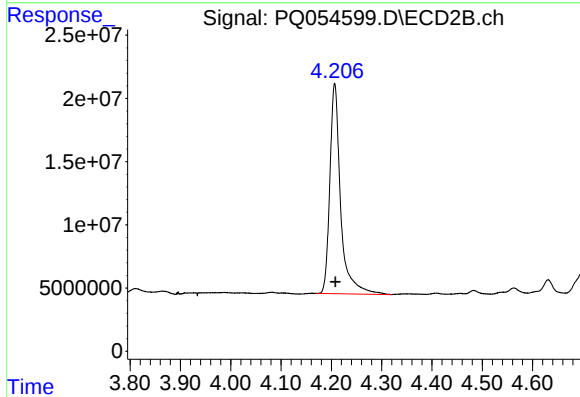


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: -0.001 min
Response: 248006535
Conc: 18.76 ng/ml

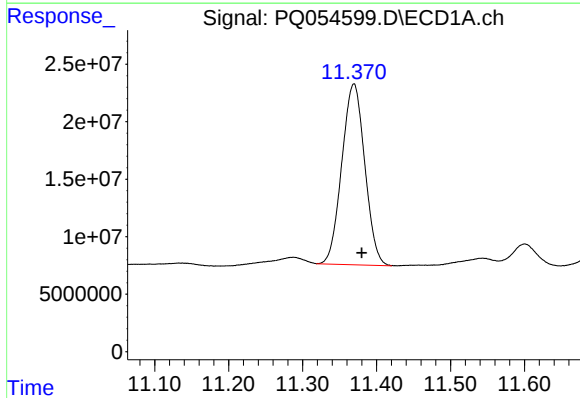

#2 Decachlorobiphenyl

R.T.: 11.370 min
Delta R.T.: -0.010 min
Response: 339563557
Conc: 20.12 ng/ml m

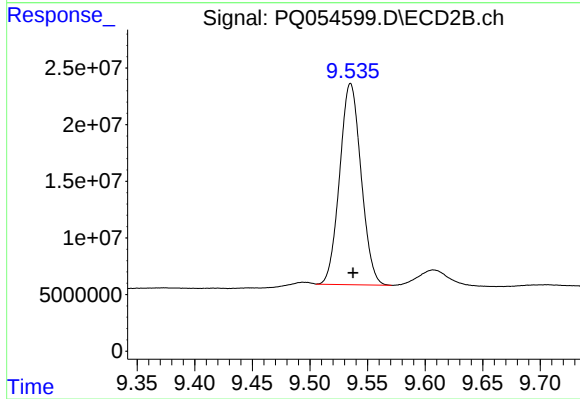

#2 Decachlorobiphenyl

R.T.: 9.535 min
Delta R.T.: -0.003 min
Response: 230034666
Conc: 16.97 ng/ml m