

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092221\
 Data File : PQ054613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 18:01
 Operator : AJ\MA
 Sample : M3826-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AUD-1183

Manual Integrations
 APPROVED

mohammad
 9/23/2021 1:36:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 02:17:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.200	4.209	447.0E6	227.5E6	18.719m	17.212
2) SA Decachlor...	11.366	9.534	165.3E6	129.0E6	9.795	9.520

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092221\
Data File : PQ054613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 18:01
Operator : AJ\MA
Sample : M3826-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
AUD-1183


Manual Integrations
APPROVED

mohammad
9/23/2021 1:36:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 02:17:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

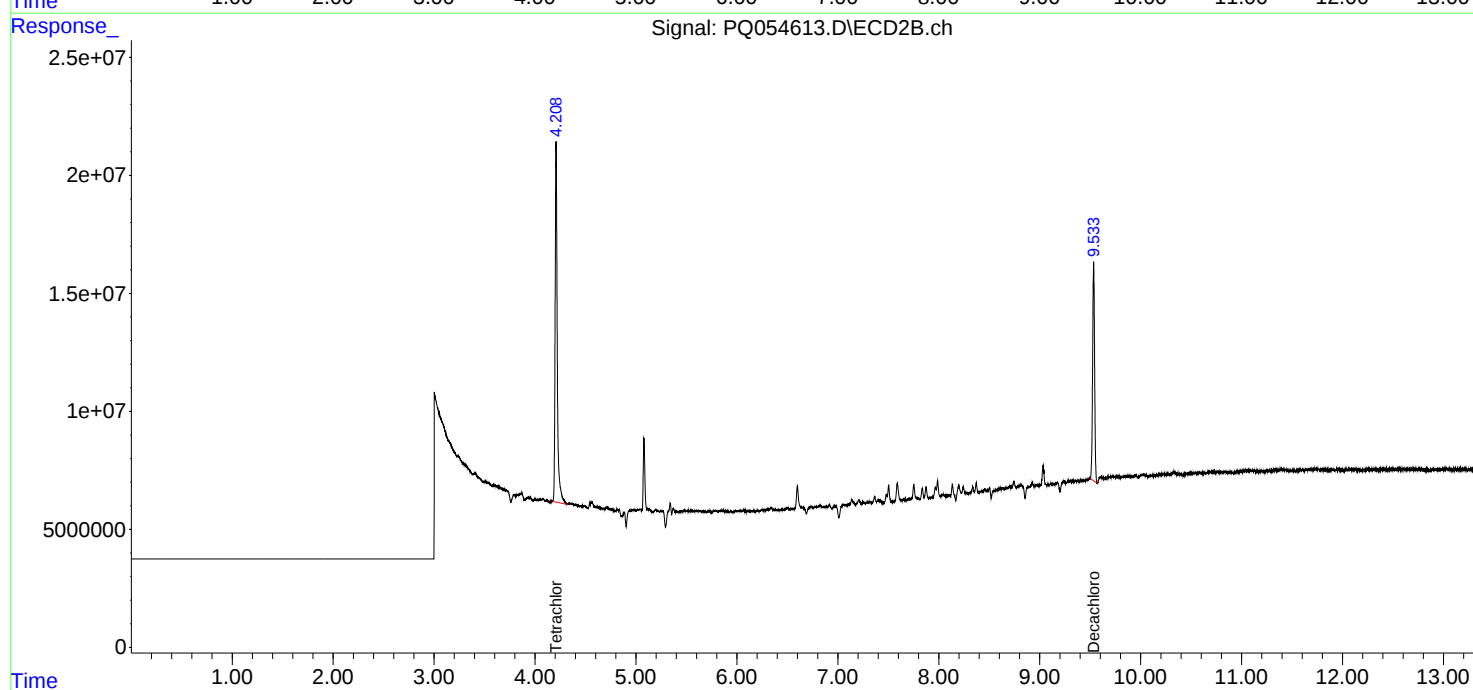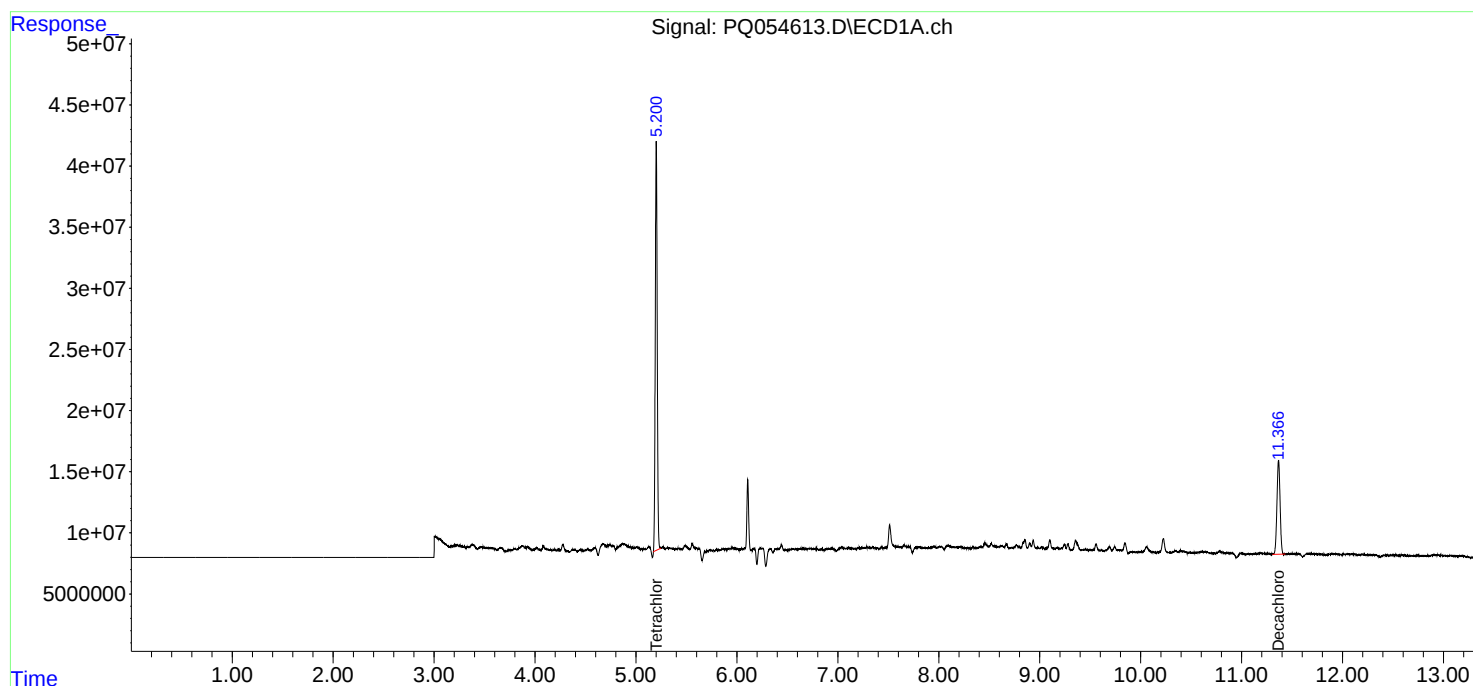

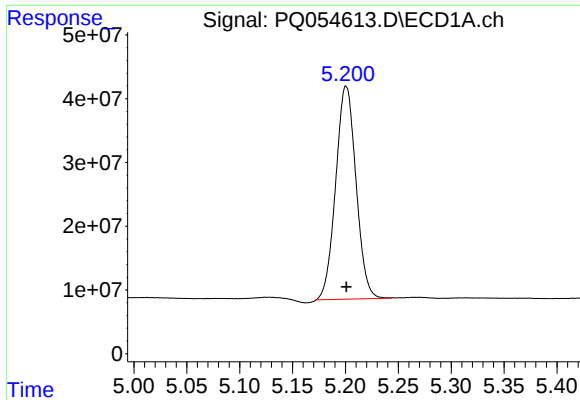


#1 Tetrachloro-m-xylene

R.T.: 5.200 min
Delta R.T.: -0.001 min
Response: 447026632
Conc: 18.72 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
AUD-1183


Manual Integrations
APPROVED

mohammad
9/23/2021 1:36:37 PM

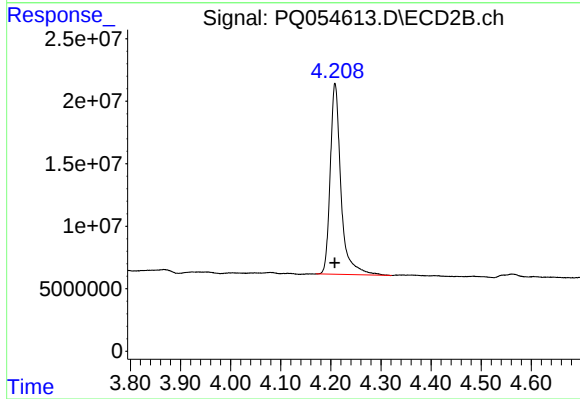


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: 0.000 min
Response: 227544486
Conc: 17.21 ng/ml

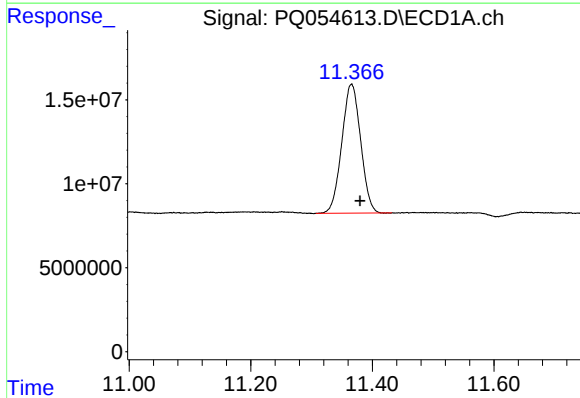

#2 Decachlorobiphenyl

R.T.: 11.366 min
Delta R.T.: -0.014 min
Response: 165318013
Conc: 9.79 ng/ml

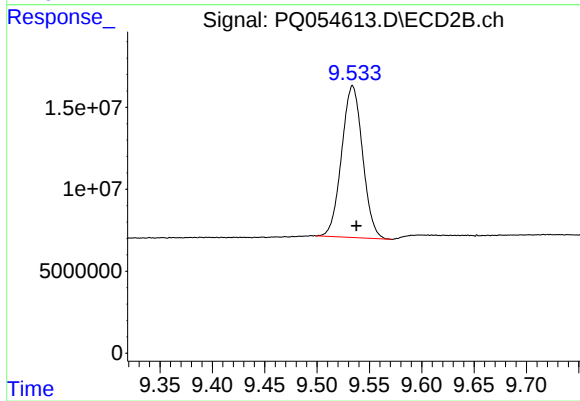

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.004 min
Response: 129011335
Conc: 9.52 ng/ml