

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092221\
 Data File : PQ054614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2021 18:17
 Operator : AJ\MA
 Sample : M3826-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 DRIP-COMP-AUD-1181-1187

Manual Integrations
 APPROVED

mohammad
 9/23/2021 1:36:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 02:19:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.199	4.210	414.7E6	149.6E6	17.367m	11.313m#
2) SA Decachlor...	11.367	9.534	143.7E6	111.0E6	8.514	8.193

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092221\
Data File : PQ054614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2021 18:17
Operator : AJ\MA
Sample : M3826-05
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
DRIP-COMP-AUD-1181-1187


Manual Integrations
APPROVED

mohammad
9/23/2021 1:36:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 02:19:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

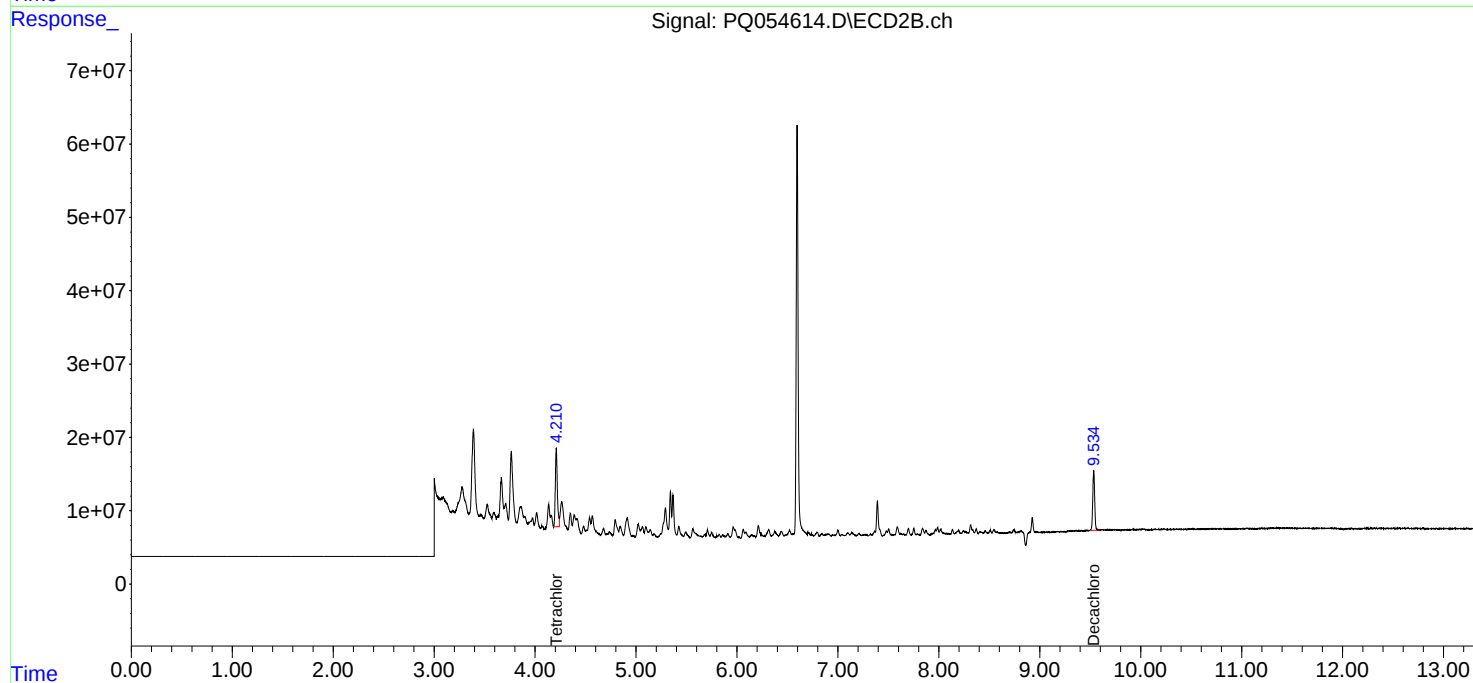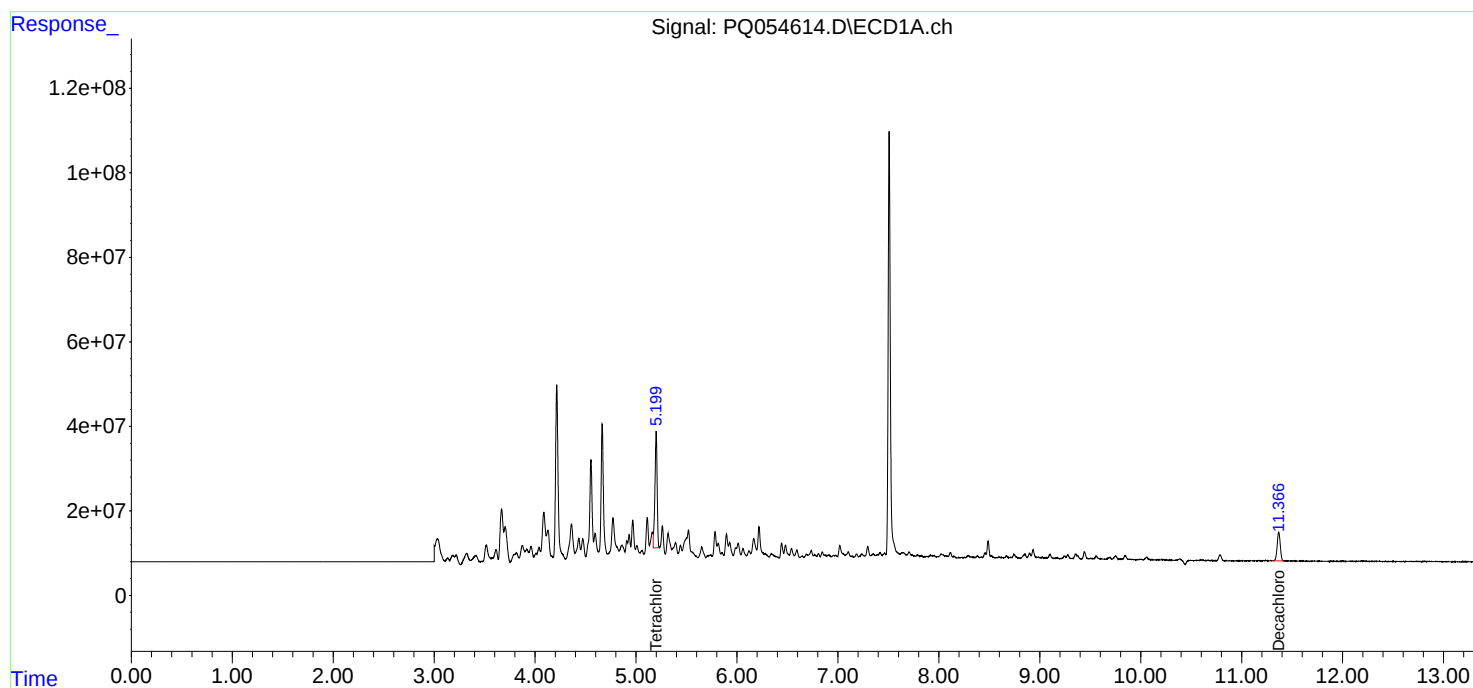

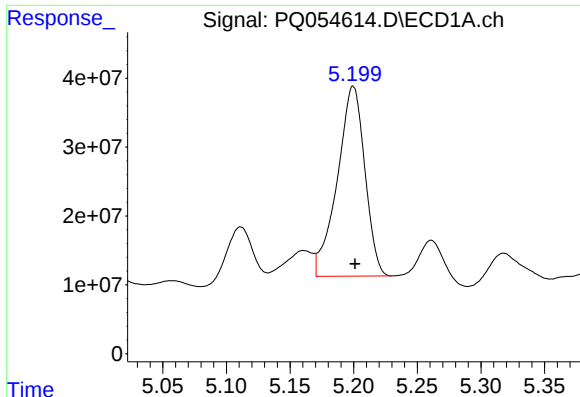


#1 Tetrachloro-m-xylene

R.T.: 5.199 min
Delta R.T.: -0.002 min
Response: 414748046
Conc: 17.37 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
DRIP-COMP-AUD-1181-1187


Manual Integrations
APPROVED

mohammad
9/23/2021 1:36:39 PM

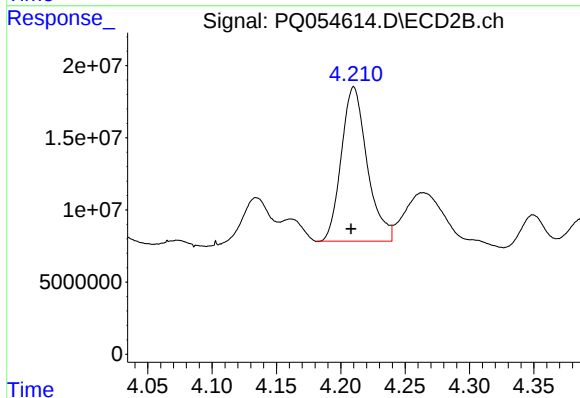


#1 Tetrachloro-m-xylene

R.T.: 4.210 min
Delta R.T.: 0.002 min
Response: 149551306
Conc: 11.31 ng/ml m

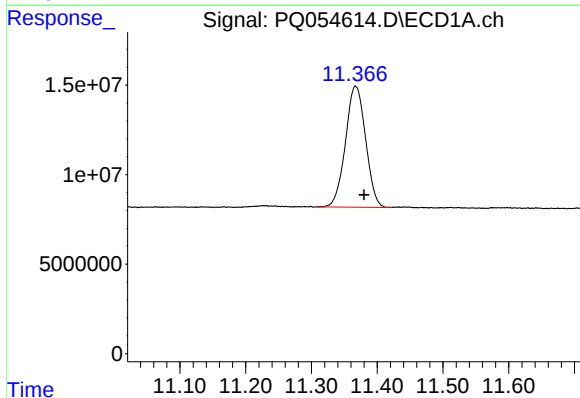

#2 Decachlorobiphenyl

R.T.: 11.367 min
Delta R.T.: -0.013 min
Response: 143705828
Conc: 8.51 ng/ml

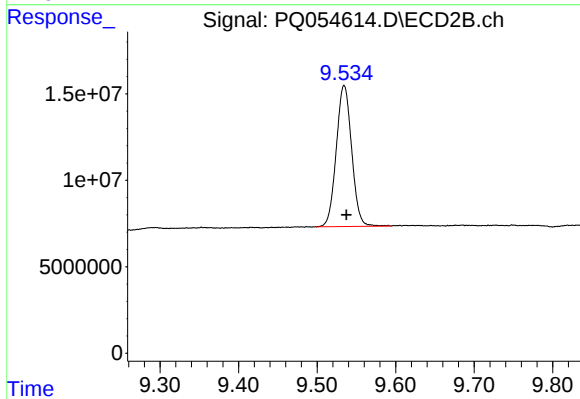

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.003 min
Response: 111029715
Conc: 8.19 ng/ml