

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092321\
 Data File : PQ054699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2021 03:09
 Operator : AJ\MA
 Sample : M3861-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MW-23-20210921-0-1-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 06:56:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.200	4.207	586.5E6	316.3E6	24.557	23.925
2) SA Decachlor...	11.365	9.532	404.3E6	283.4E6	23.955	20.913

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092321\
Data File : PQ054699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2021 03:09
Operator : AJ\MA
Sample : M3861-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MW-23-20210921-0-1-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 06:56:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

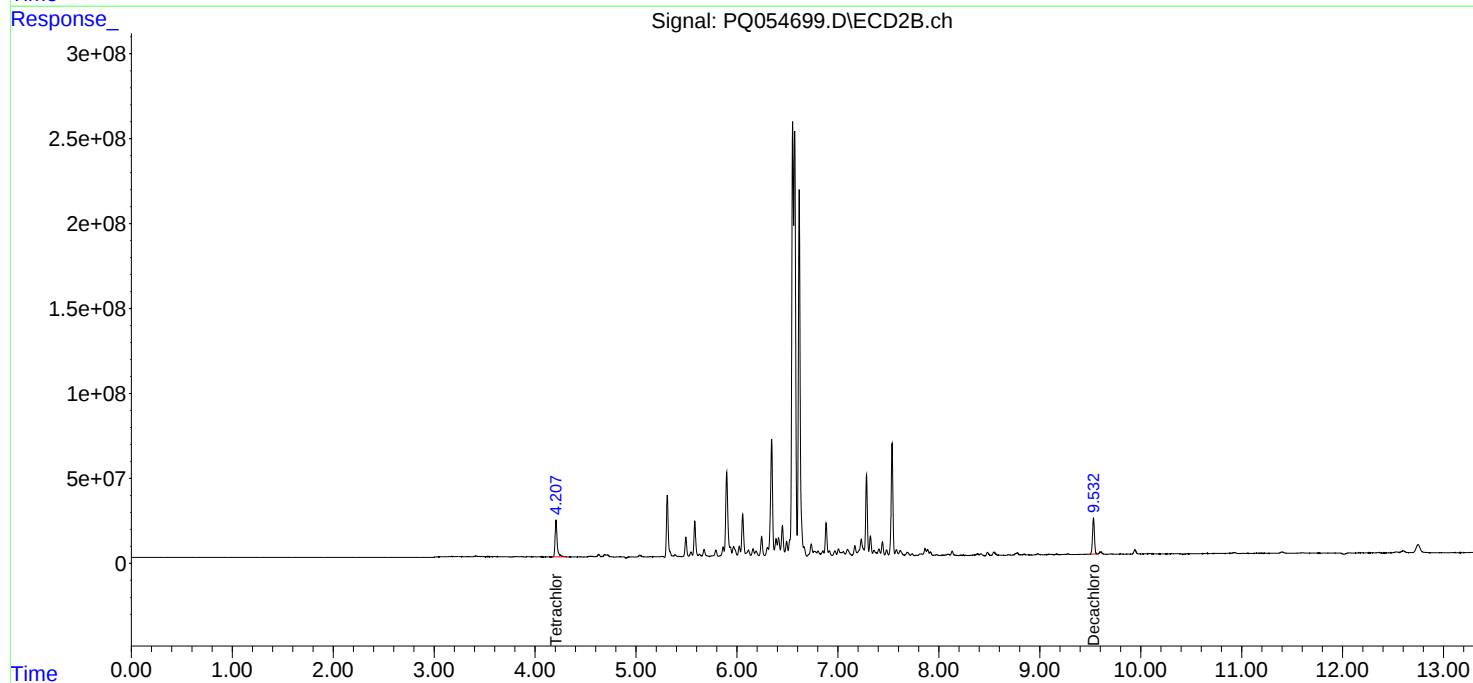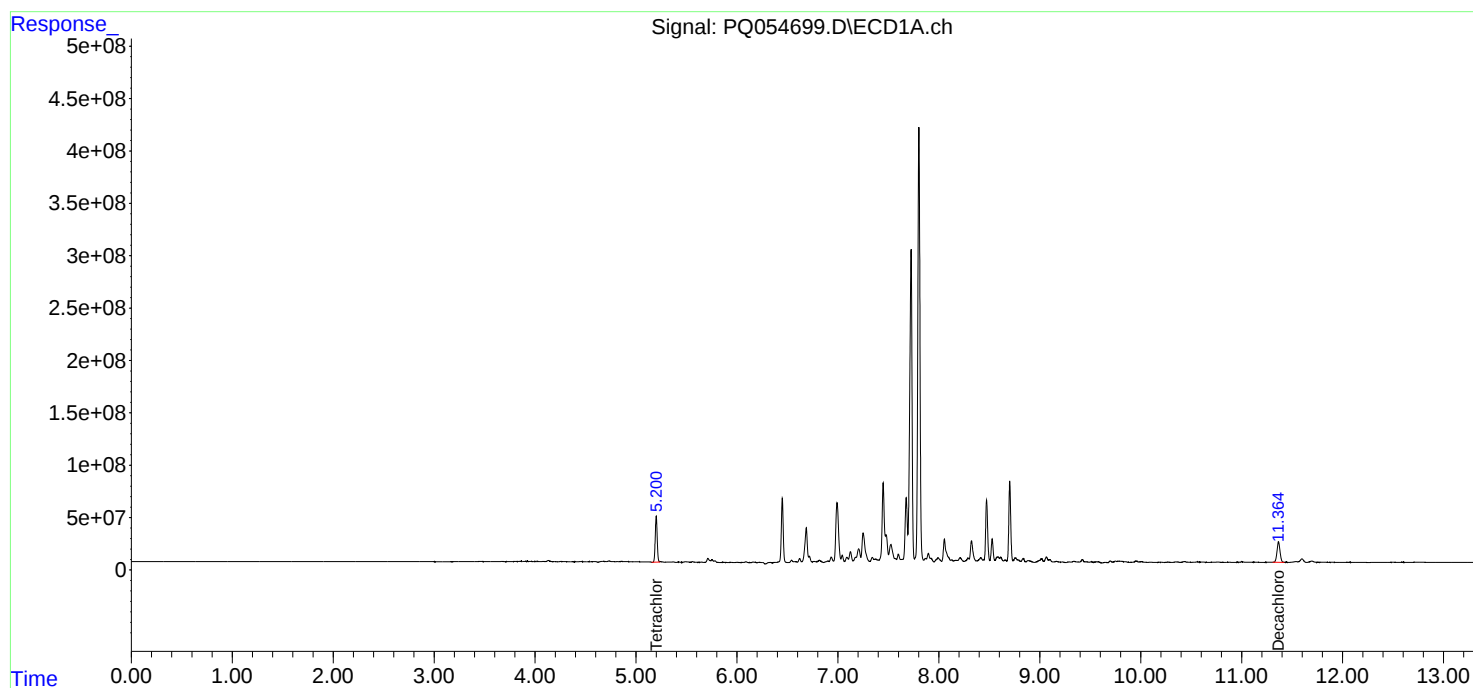


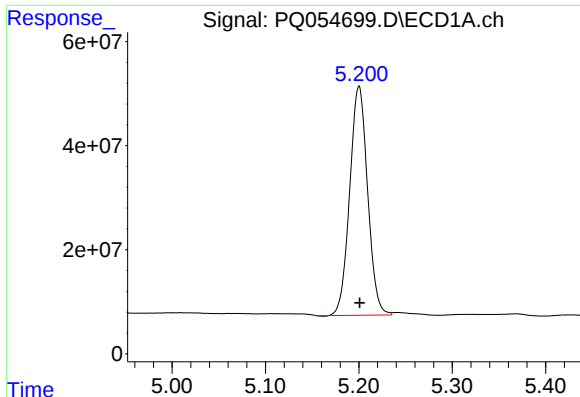

#1 Tetrachloro-m-xylene


R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 586459956
Conc: 24.56 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MW-23-20210921-0-1-WC

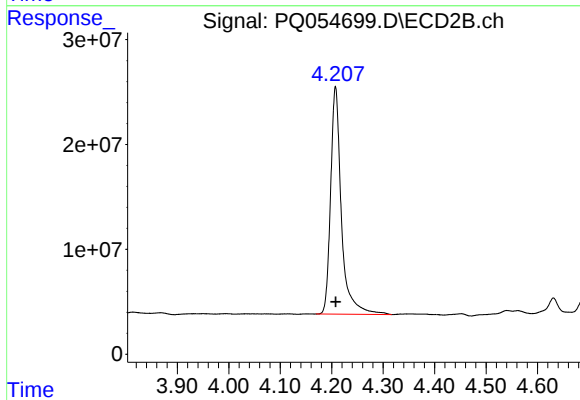


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: 0.000 min
Response: 316278040
Conc: 23.92 ng/ml

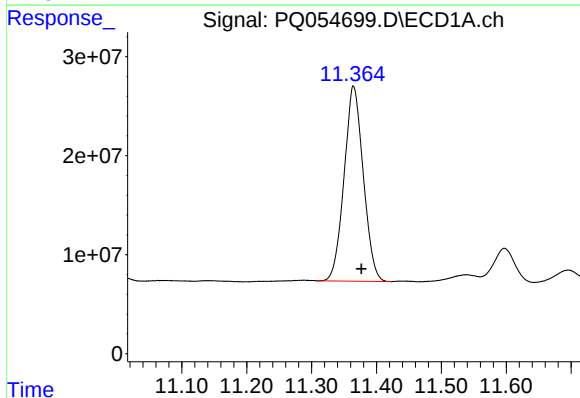

#2 Decachlorobiphenyl

R.T.: 11.365 min
Delta R.T.: -0.013 min
Response: 404314775
Conc: 23.95 ng/ml

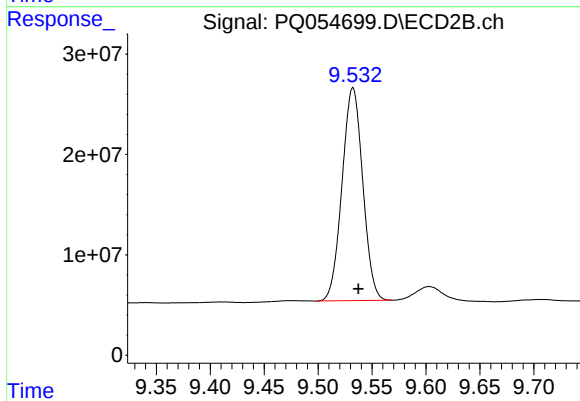

#2 Decachlorobiphenyl

R.T.: 9.532 min
Delta R.T.: -0.005 min
Response: 283409804
Conc: 20.91 ng/ml