

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092321\
 Data File : PQ054711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2021 06:25
 Operator : AJ\MA
 Sample : M3862-01 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 01-A-01-B-01-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:33:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.200	4.208	46398755	22152598	1.943m	1.676
2) SA Decachlor...	11.364	9.533	34541414	22455067	2.047	1.657

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092321\
Data File : PQ054711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2021 06:25
Operator : AJ\MA
Sample : M3862-01 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
01-A-01-B-01-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:33:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

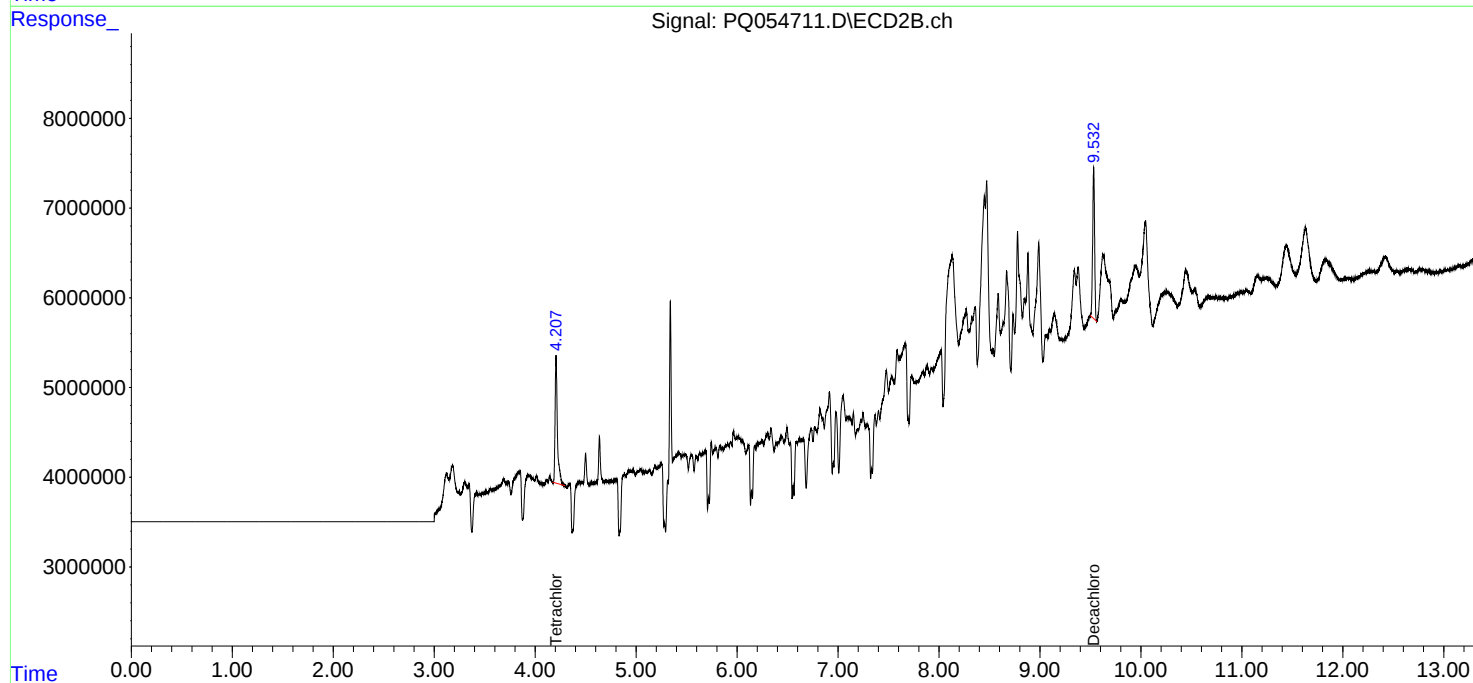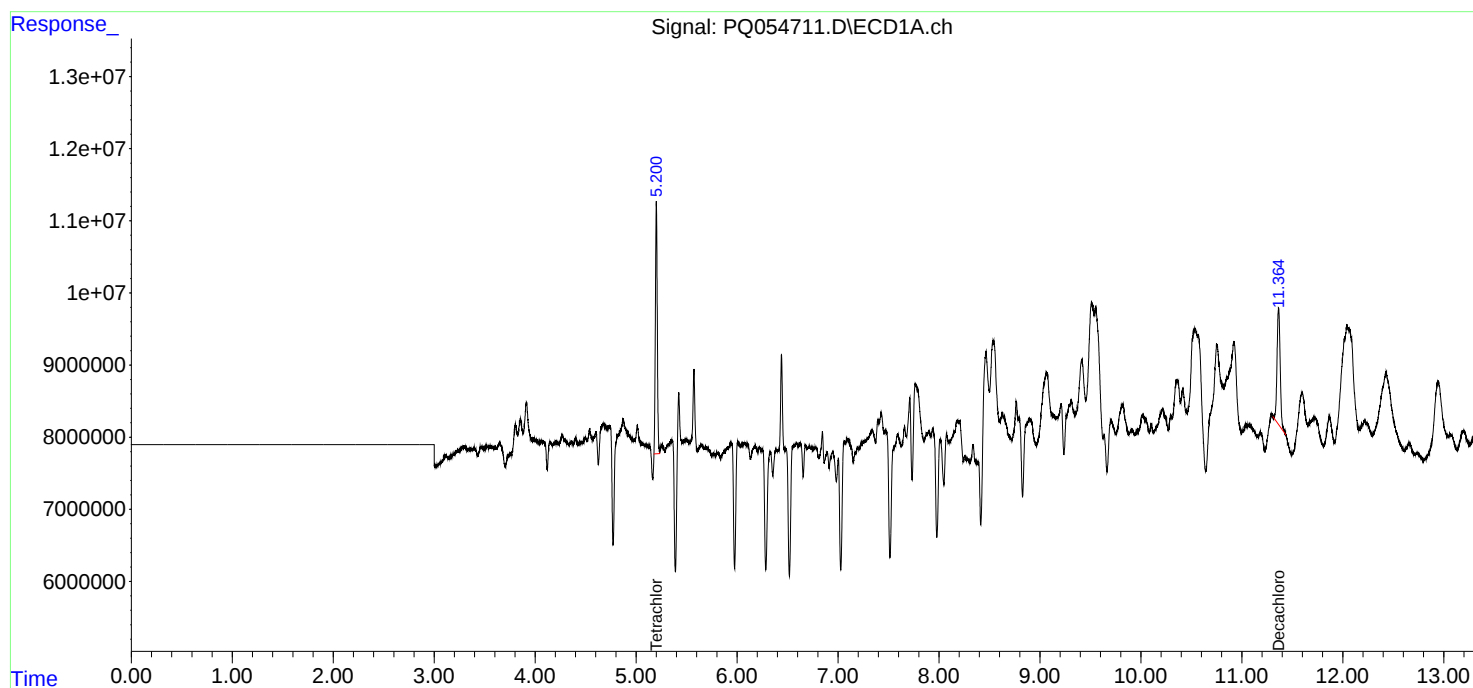


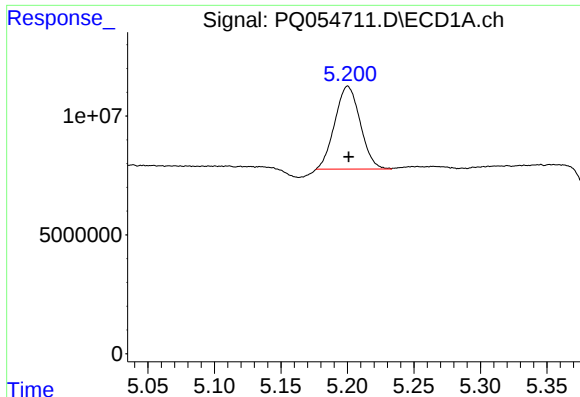

#1 Tetrachloro-m-xylene


R.T.: 5.200 min
Delta R.T.: -0.001 min
Response: 46398755
Conc: 1.94 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
01-A-01-B-01-C

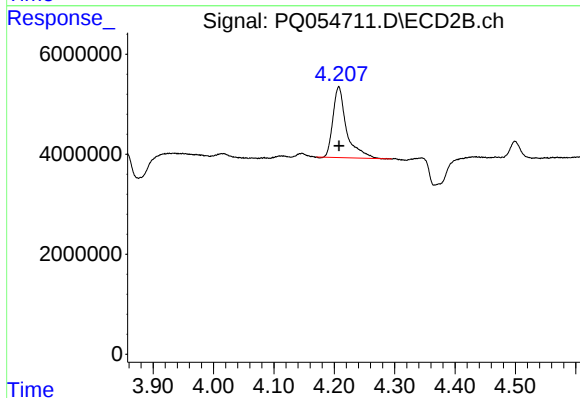


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 22152598
Conc: 1.68 ng/ml

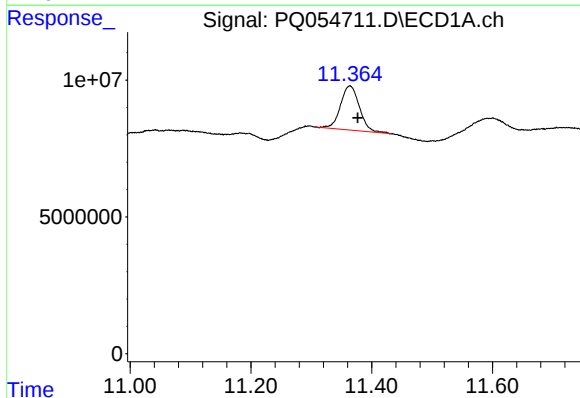

#2 Decachlorobiphenyl

R.T.: 11.364 min
Delta R.T.: -0.013 min
Response: 34541414
Conc: 2.05 ng/ml

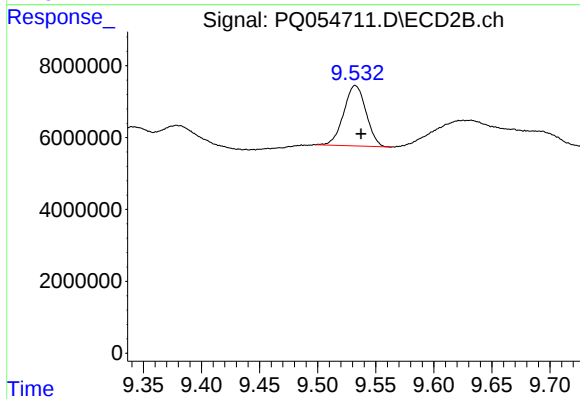

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.005 min
Response: 22455067
Conc: 1.66 ng/ml