

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092424\
 Data File : PQ068764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 03:05
 Operator : YP\AJ
 Sample : PB163647BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB163647BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 04:54:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ090624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:06:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.437	2.819	124.4E6	128.3E6	17.425	18.007
2) SA Decachlor...	8.609	7.592	73009630	118.6E6	16.752	17.953m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092424\
Data File : PQ068764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 03:05
Operator : YP\AJ
Sample : PB163647BL
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PB163647BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 04:54:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ090624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:06:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

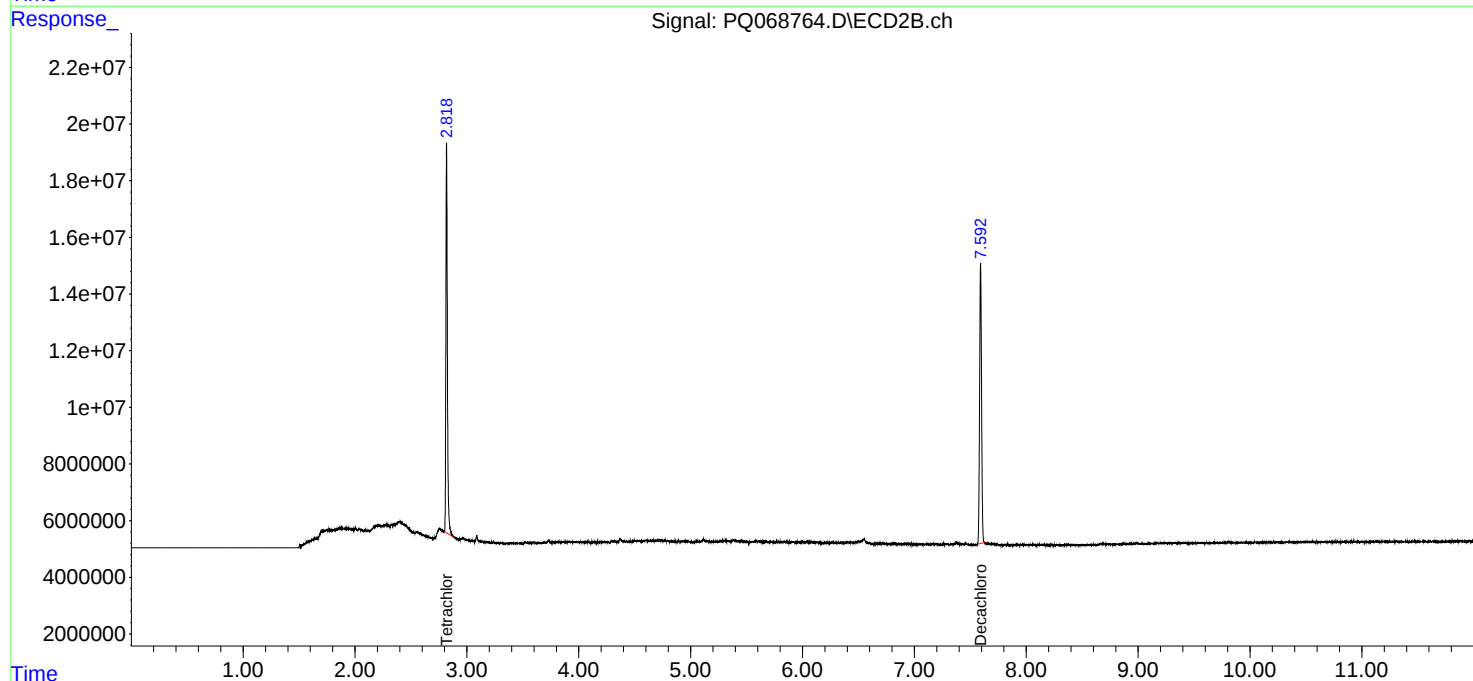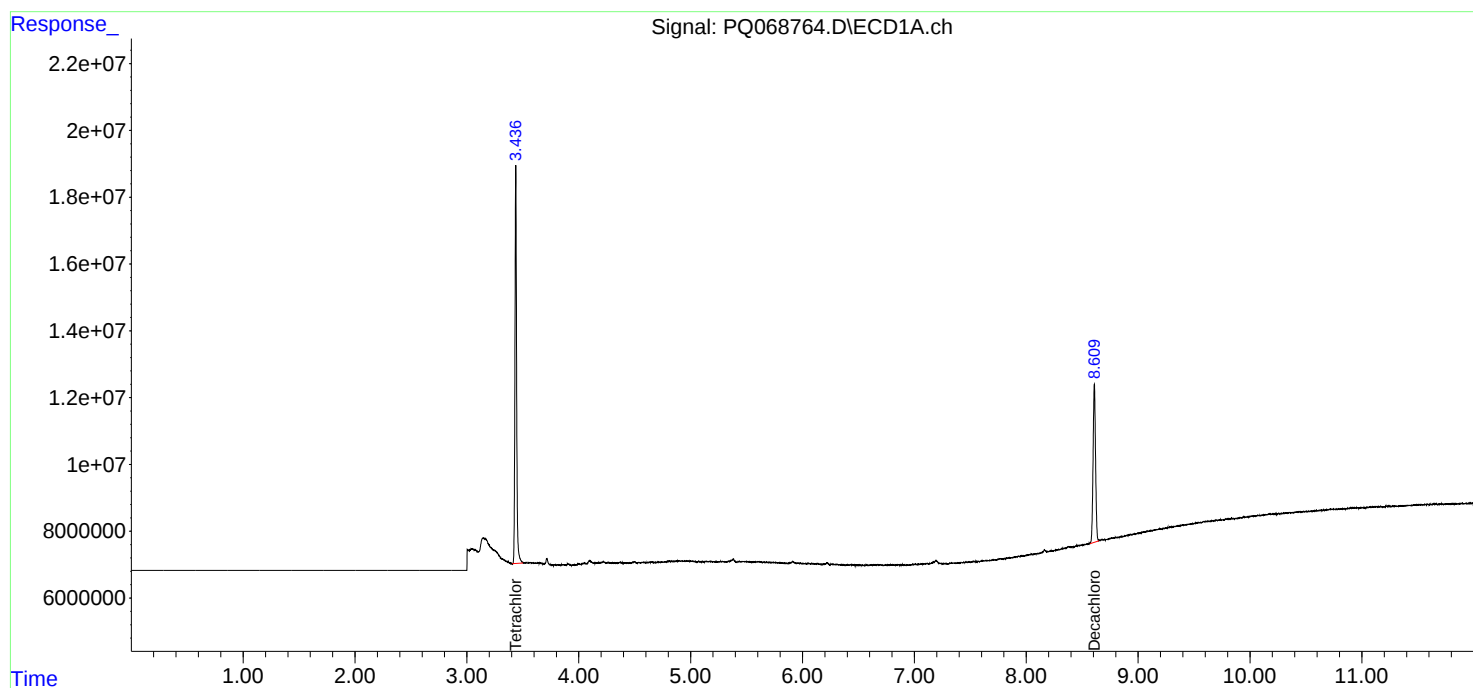

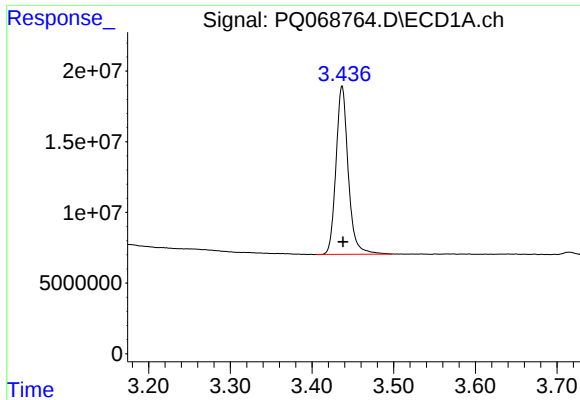


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: -0.001 min
Response: 124428905
Conc: 17.43 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB163647BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :Ankita Jodhani 09/25/2024

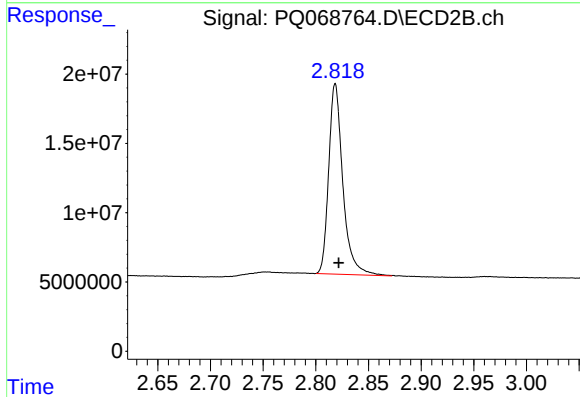


#1 Tetrachloro-m-xylene

R.T.: 2.819 min
Delta R.T.: -0.003 min
Response: 128254525
Conc: 18.01 ng/ml

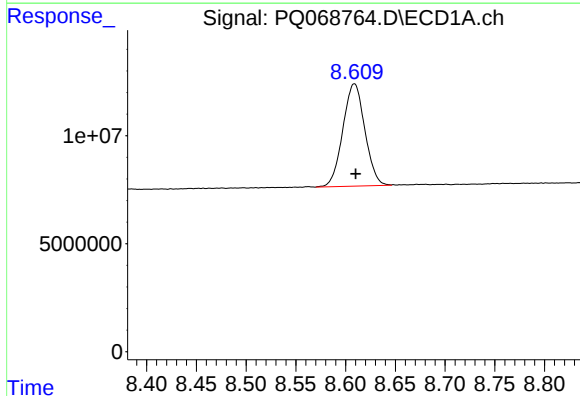

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: -0.001 min
Response: 73009630
Conc: 16.75 ng/ml

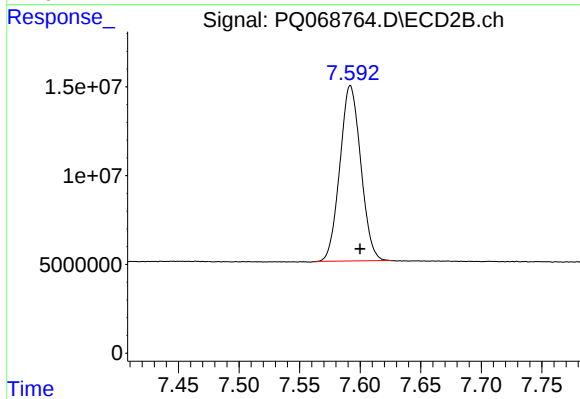

#2 Decachlorobiphenyl

R.T.: 7.592 min
Delta R.T.: -0.008 min
Response: 118557596
Conc: 17.95 ng/ml m