

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092624\
 Data File : PQ068873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2024 14:40
 Operator : YP\AJ
 Sample : P4192-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ETGI-355

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/27/2024
 Supervised By :Ankita Jodhani 09/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 04:47:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ090624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:06:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.435	2.817	135.8E6	149.5E6	19.014	20.985
2) SA Decachlor...	8.609	7.591	69777389	132.8E6	16.010m	20.109 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092624\
Data File : PQ068873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2024 14:40
Operator : YP\AJ
Sample : P4192-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ETGI-355


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 04:47:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ090624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:06:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

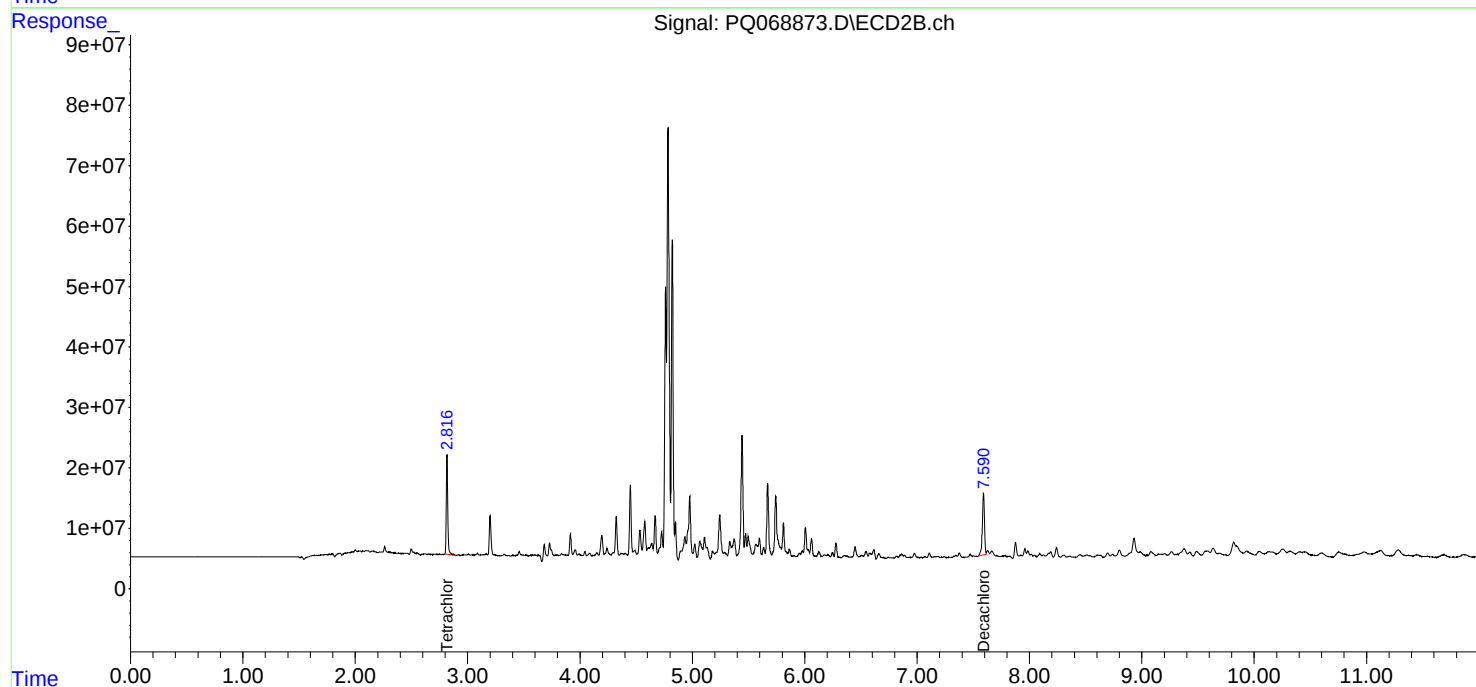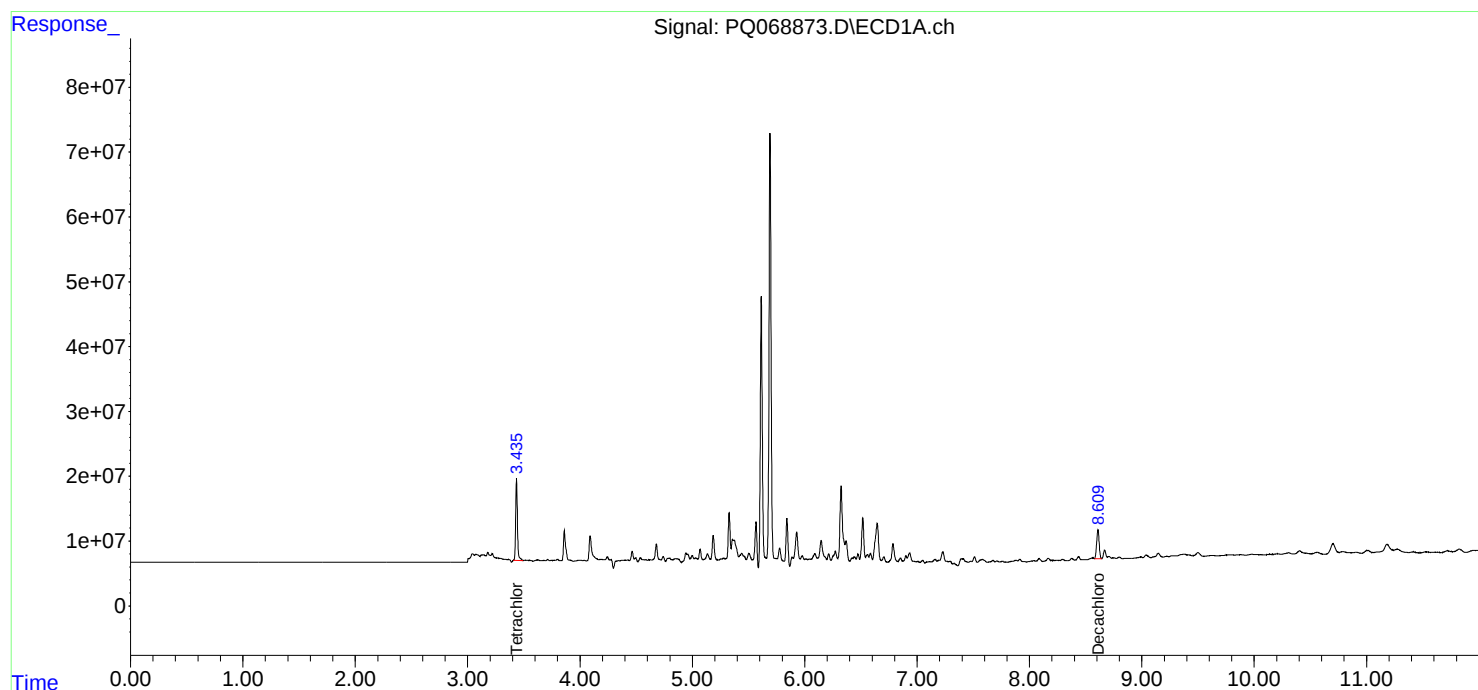

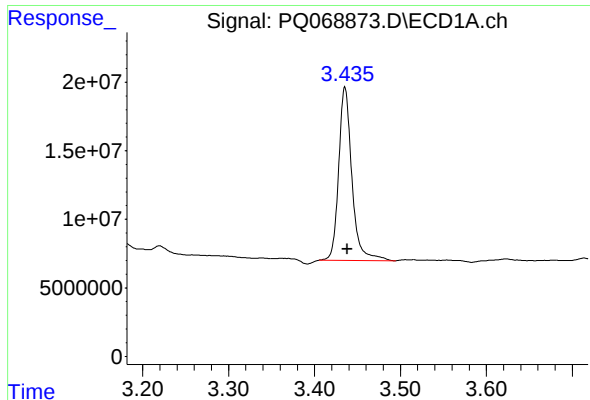


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.003 min
Response: 135768479
Conc: 19.01 ng/ml

Instrument :
ECD_Q
ClientSampleId :
ETGI-355


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :Ankita Jodhani 09/27/2024

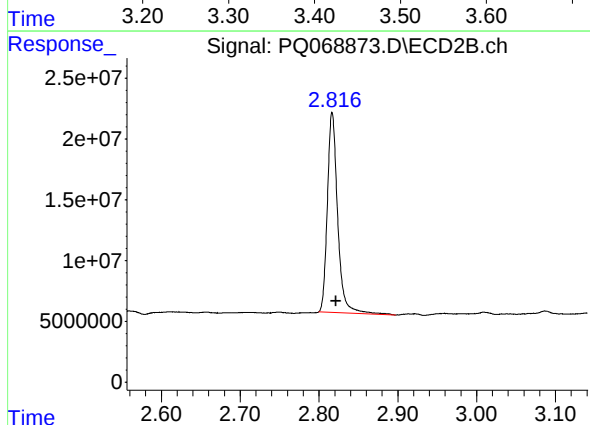


#1 Tetrachloro-m-xylene

R.T.: 2.817 min
Delta R.T.: -0.005 min
Response: 149460658
Conc: 20.98 ng/ml

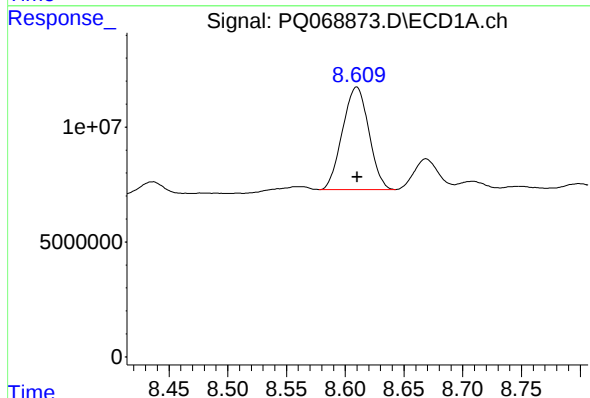

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: 0.000 min
Response: 69777389
Conc: 16.01 ng/ml m

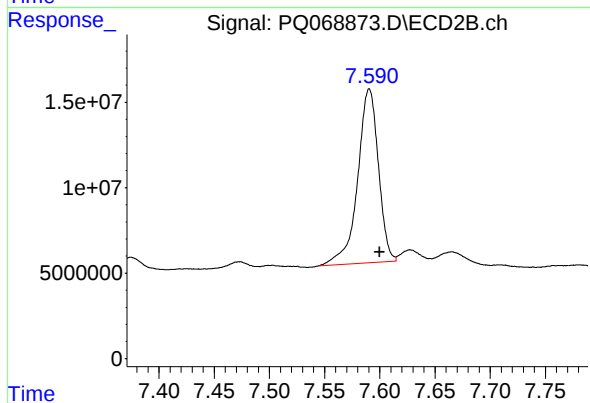

#2 Decachlorobiphenyl

R.T.: 7.591 min
Delta R.T.: -0.009 min
Response: 132798232
Conc: 20.11 ng/ml