

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092721\
 Data File : PQ054766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2021 11:19
 Operator : AJ\MA
 Sample : M3920-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 S-839-R-SO-6-6.5-092321

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:56:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.201	4.207	557.9E6	289.4E6	23.362	21.892
2)	SA Decachlor...	11.368	9.534	342.7E6	279.2E6	20.303	20.603

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092721\
Data File : PQ054766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2021 11:19
Operator : AJ\MA
Sample : M3920-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
S-839-R-SO-6-6.5-092321

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:56:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

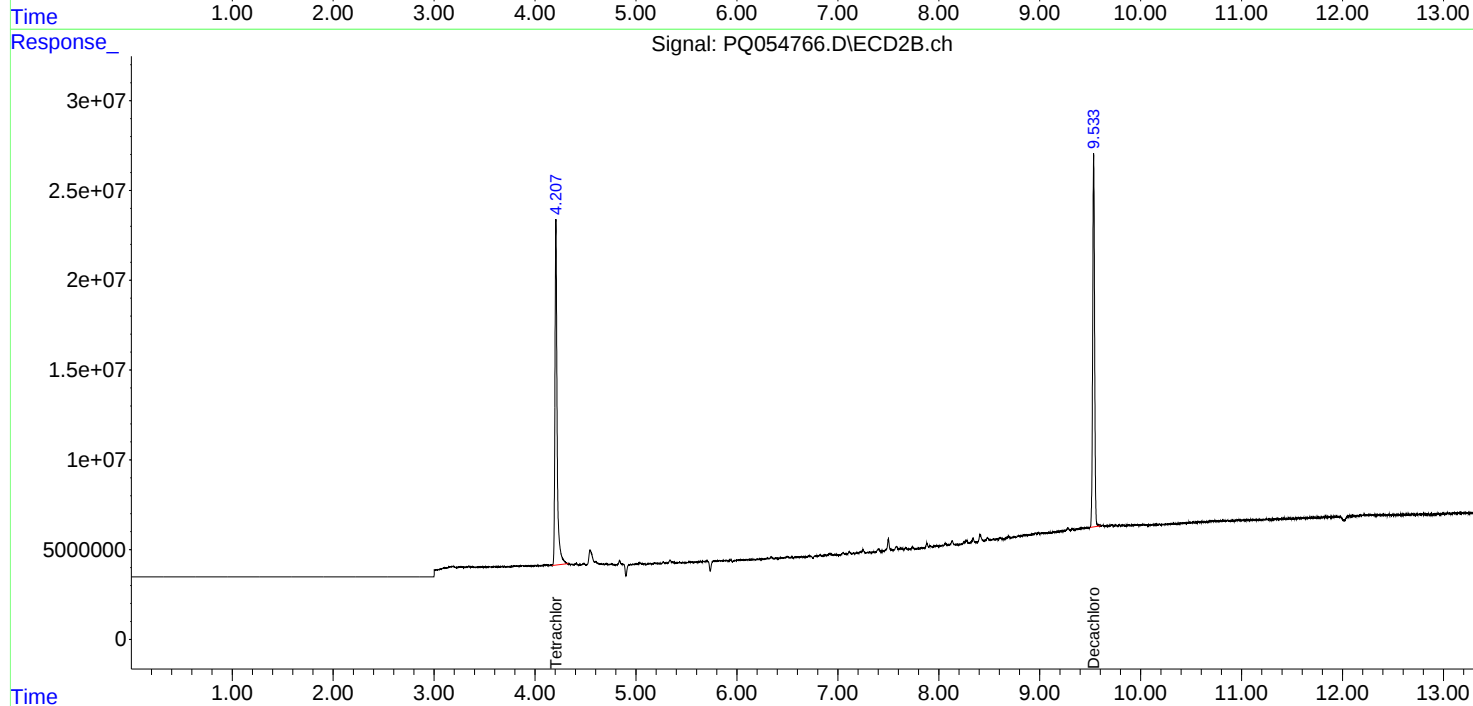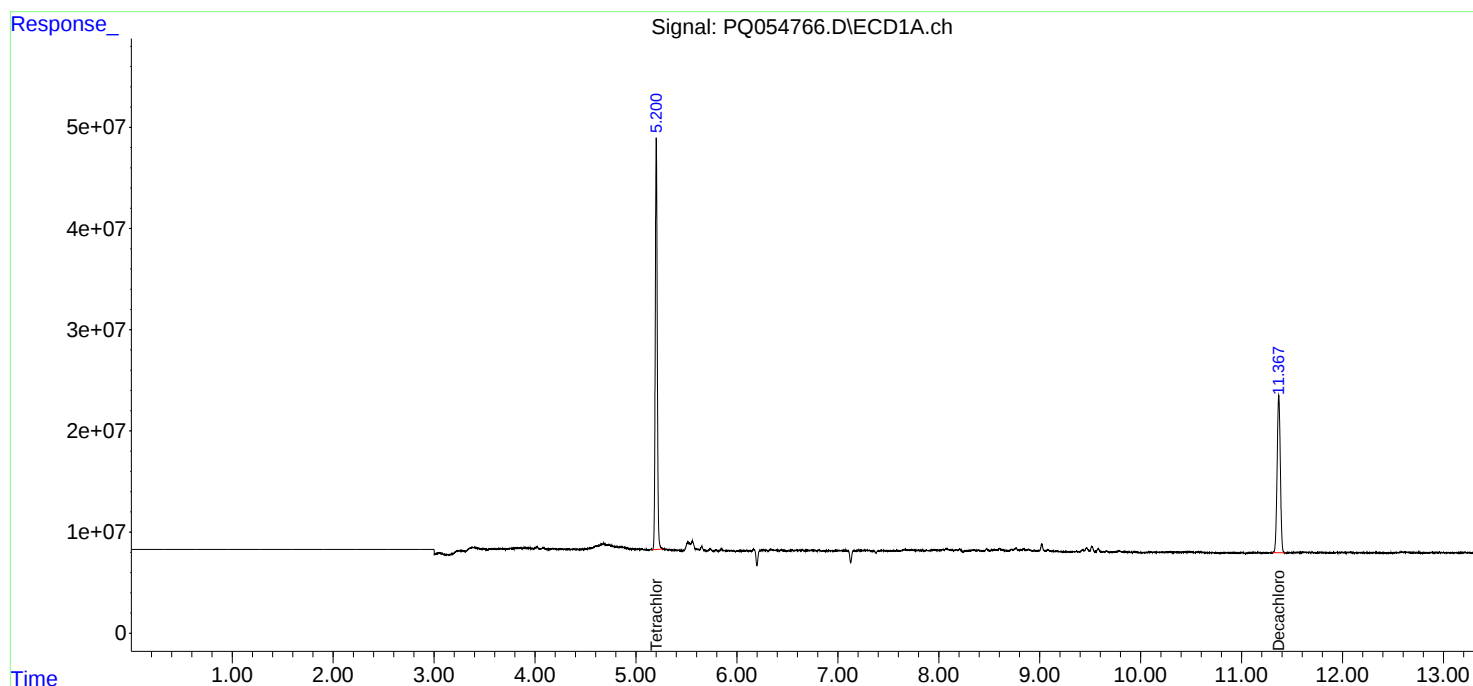


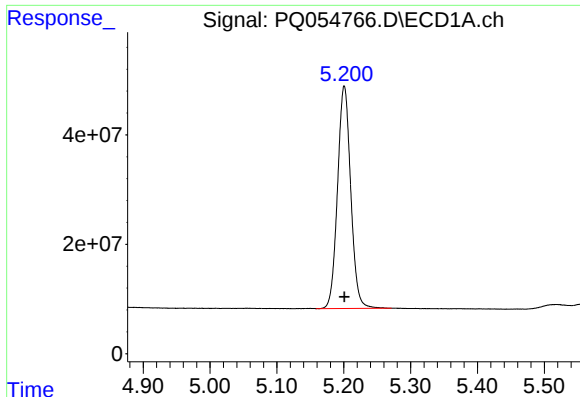

#1 Tetrachloro-m-xylene


R.T.: 5.201 min
Delta R.T.: 0.000 min
Response: 557905894
Conc: 23.36 ng/ml

Instrument :
ECD_Q
ClientSampleId :
S-839-R-SO-6-6.5-092321

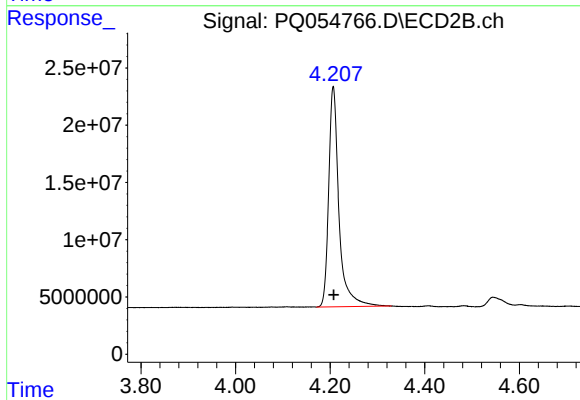


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: -0.001 min
Response: 289404375
Conc: 21.89 ng/ml

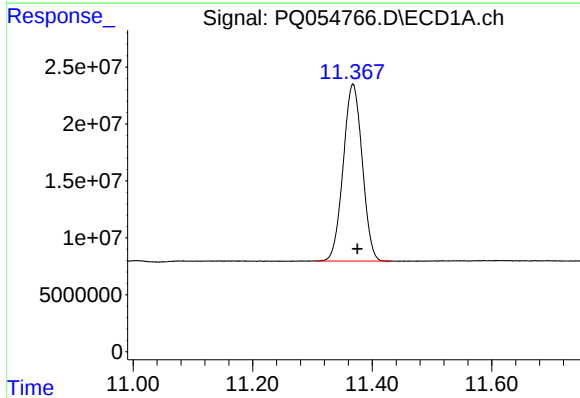

#2 Decachlorobiphenyl

R.T.: 11.368 min
Delta R.T.: -0.007 min
Response: 342676527
Conc: 20.30 ng/ml

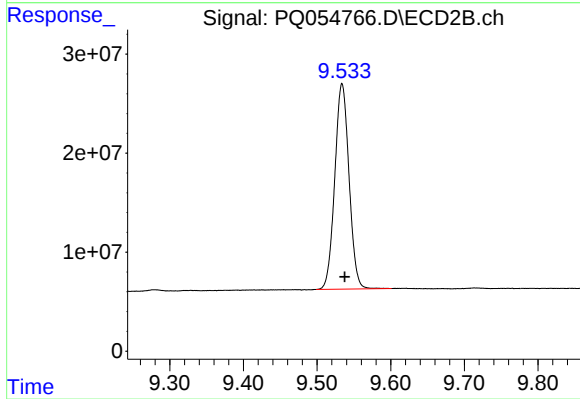

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.004 min
Response: 279213826
Conc: 20.60 ng/ml