

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092723\
 Data File : PQ063423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 18:11
 Operator : YP\AJ
 Sample : 04621-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ETGI-287

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/28/2023
 Supervised By :Ankita Jodhani 09/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:24:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 20 05:26:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.462	2.780	85370549	69079885	18.228m	19.989m
2) SA Decachlor...	8.697	7.581	58597346	68725355	16.768m	19.118m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ092723\
Data File : PQ063423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 18:11
Operator : YP\AJ
Sample : 04621-02
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ETGI-287


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:24:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 20 05:26:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

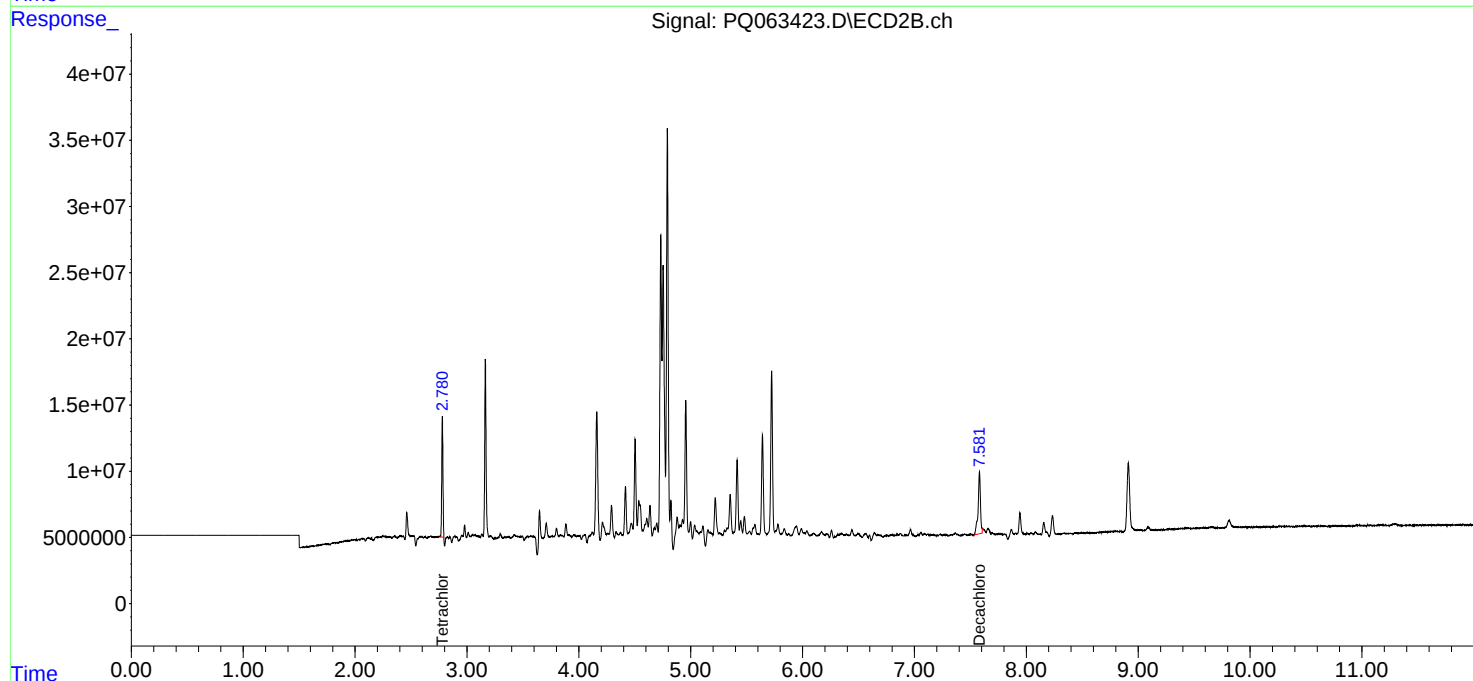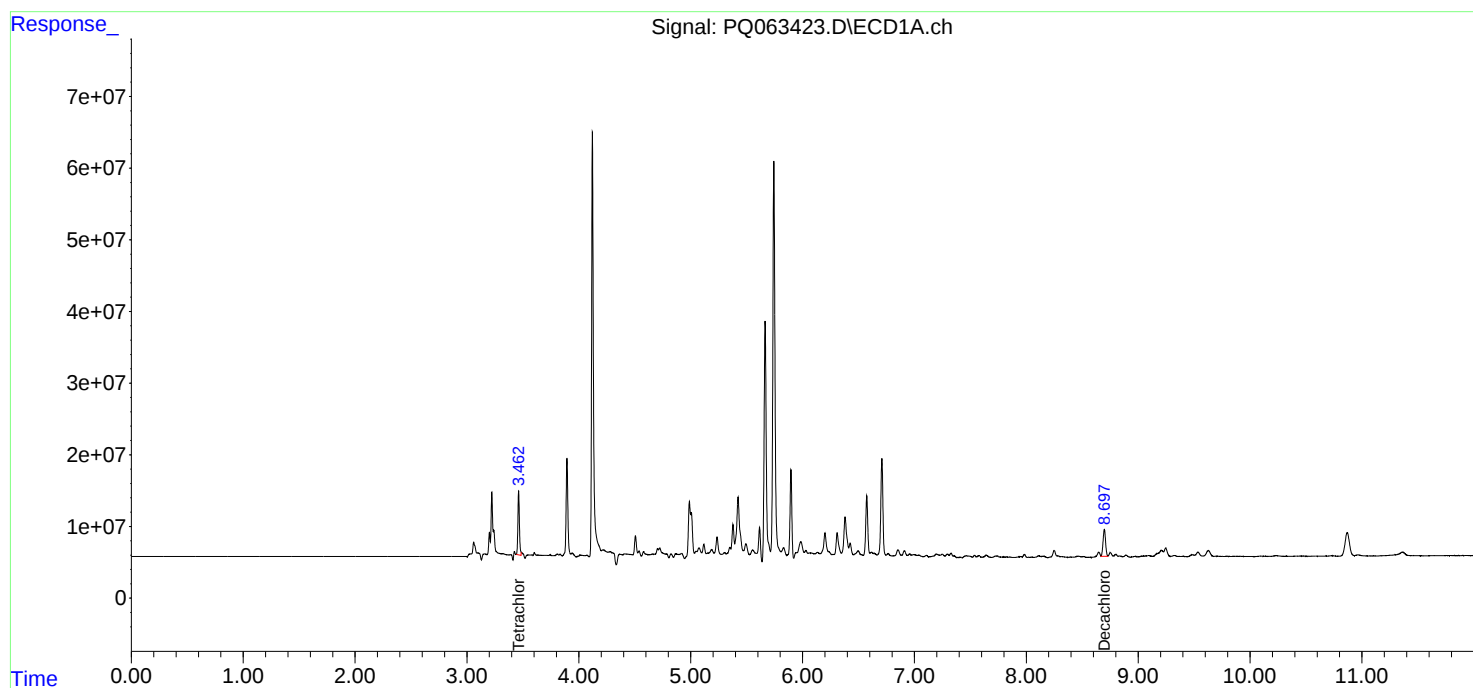

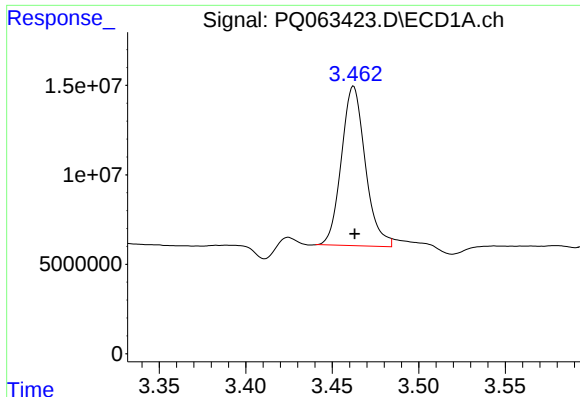


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: -0.001 min
Response: 85370549
Conc: 18.23 ng/ml

Instrument :
ECD_Q
ClientSampleId :
ETGI-287


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

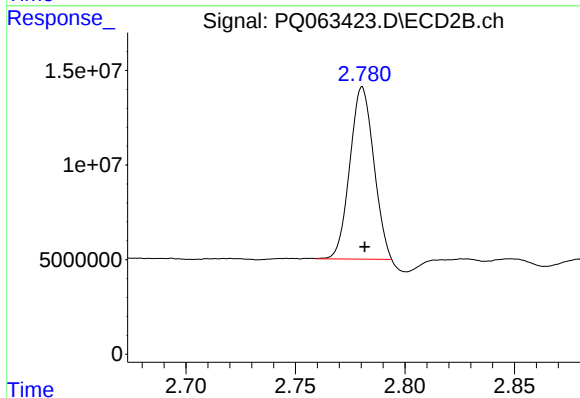


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.001 min
Response: 69079885
Conc: 19.99 ng/ml m

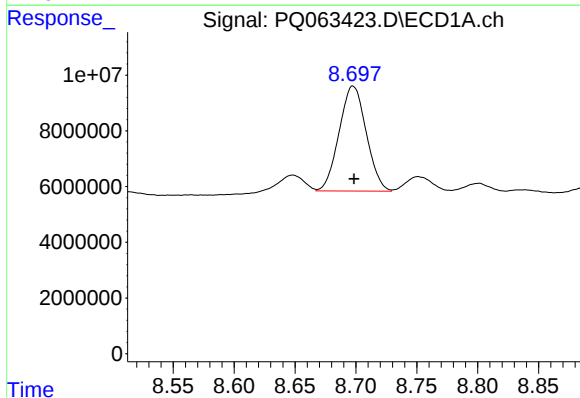

#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: -0.002 min
Response: 58597346
Conc: 16.77 ng/ml m

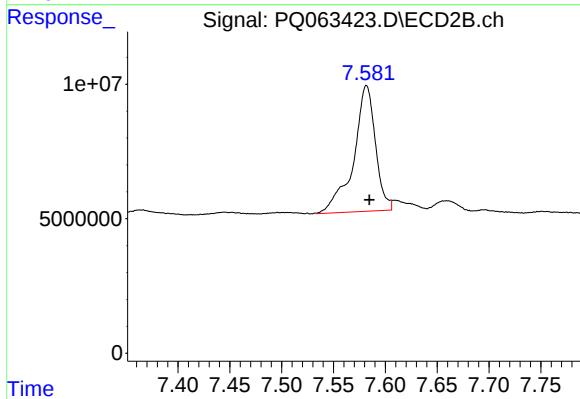

#2 Decachlorobiphenyl

R.T.: 7.581 min
Delta R.T.: -0.003 min
Response: 68725355
Conc: 19.12 ng/ml m