

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ092918\  
Data File : PQ032424.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 Sep 2018 13:52  
Operator : SM\SJ  
Sample : J5126-17 100X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1


Instrument :  
ECD\_Q  
ClientSampleId :  
C0BA5

Manual Integrations  
APPROVED

Sohil  
10/2/2018 6:34:11 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 01 03:57:21 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ092618CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Sep 27 08:45:59 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

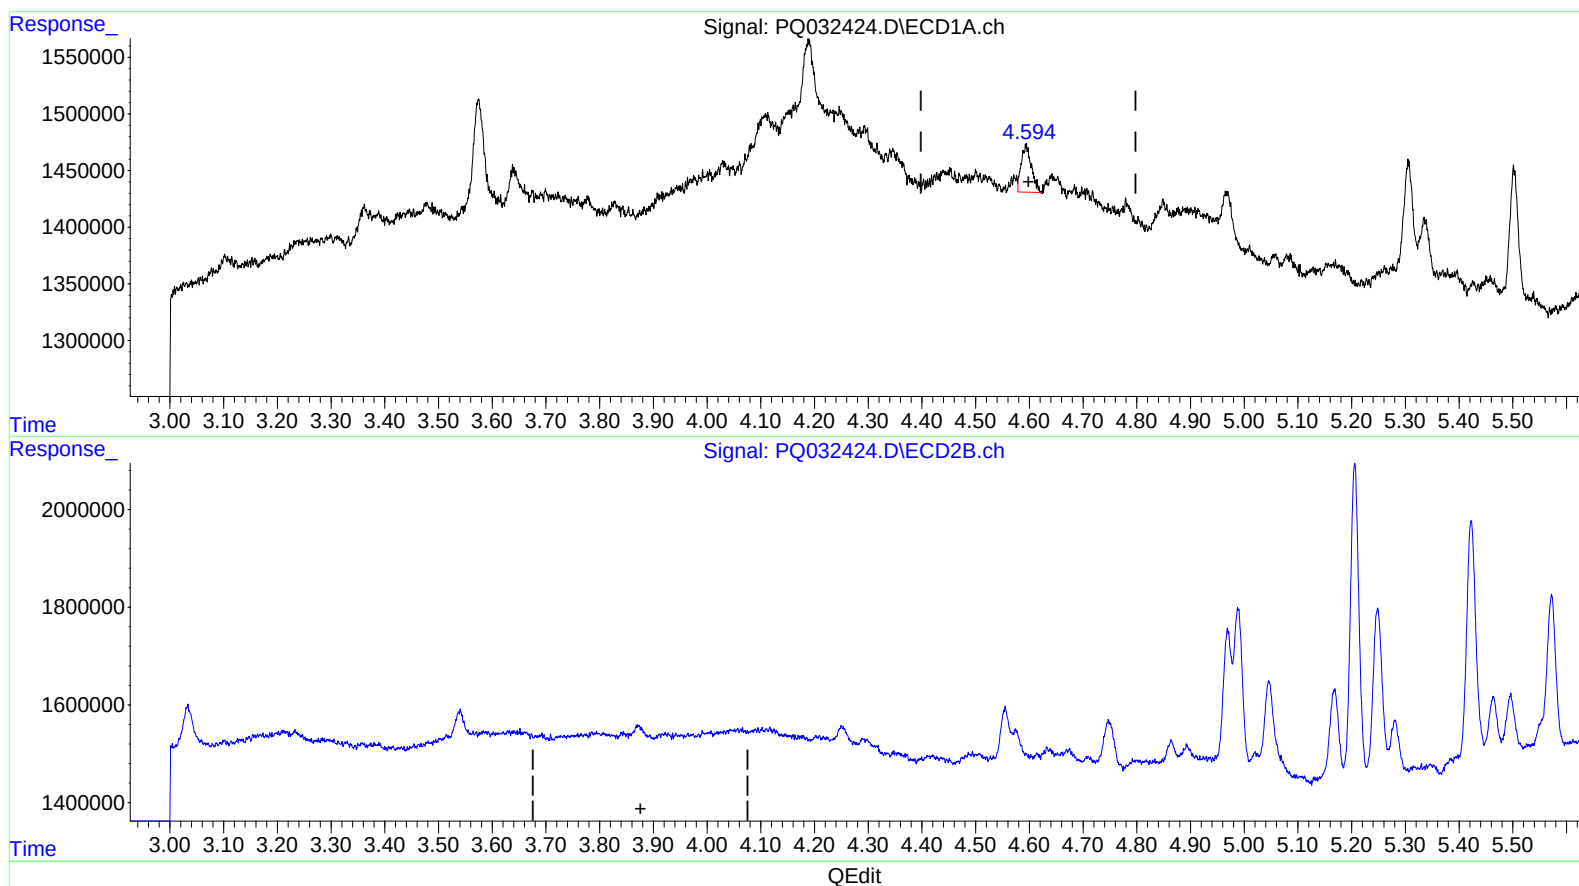

(1) Tetrachloro-m-xylene (SA)

4.594min 0.357 ng/ml

response 548658

(1) Tetrachloro-m-xylene #2 (SA)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ092918\  
Data File : PQ032424.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 Sep 2018 13:52  
Operator : SM\SJ  
Sample : J5126-17 100X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1


Instrument :  
ECD\_Q  
ClientSampleId :  
C0BA5

Manual Integrations  
APPROVED

Sohil  
10/2/2018 6:34:11 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 01 03:57:21 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ092618CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Sep 27 08:45:59 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

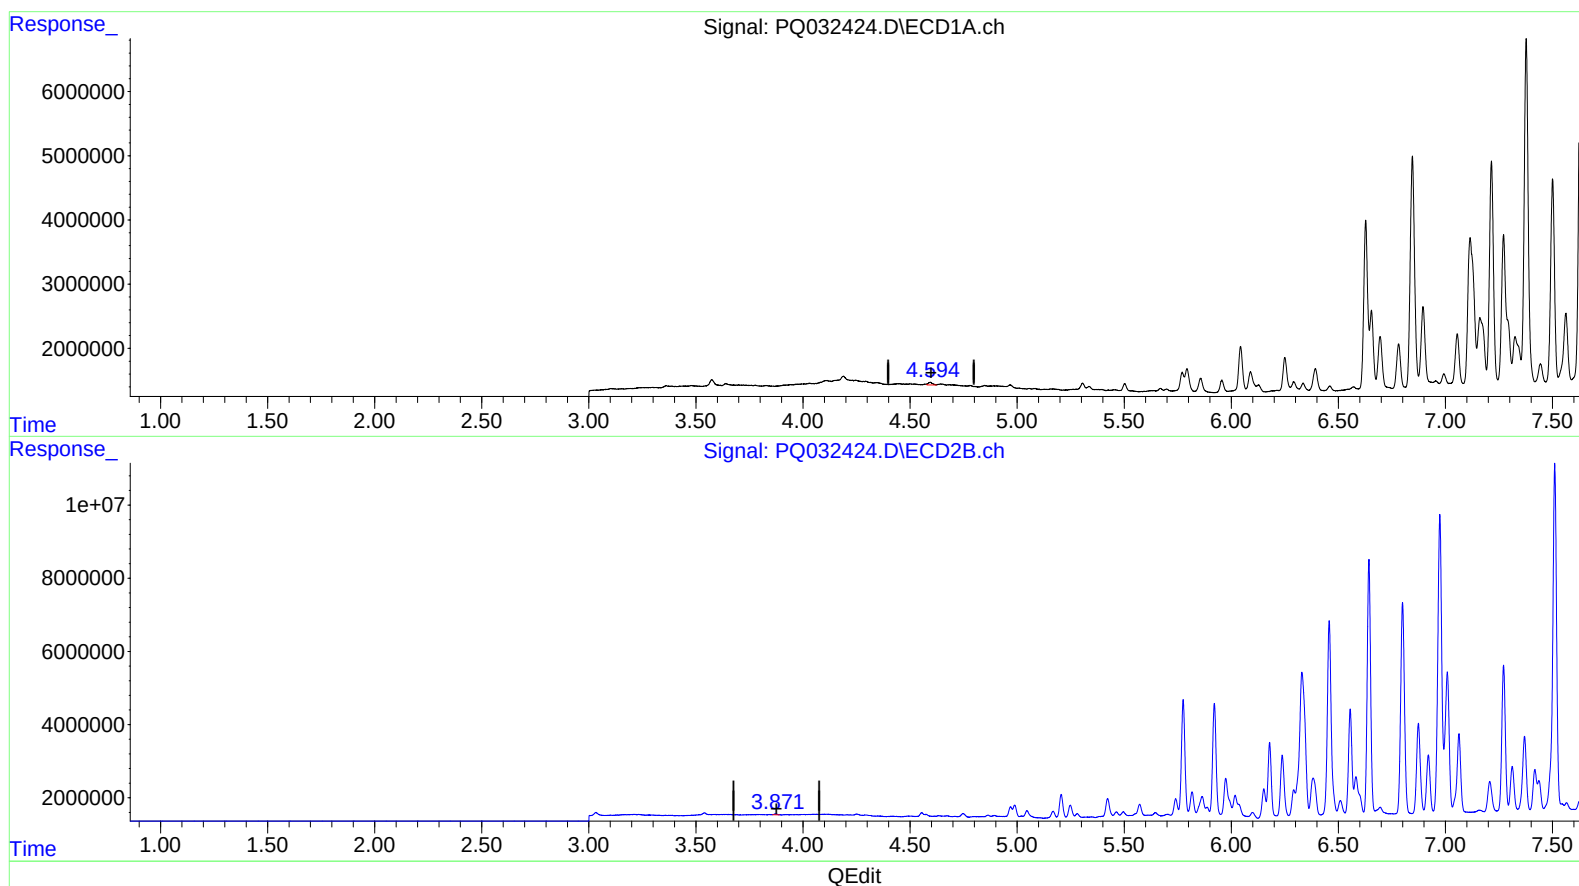

(1) Tetrachloro-m-xylene (SA)

4.594min 0.357 ng/ml

response 548658

(1) Tetrachloro-m-xylene #2 (SA)

3.871min 0.203 ng/ml m

response 233921

## Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ092918\  
 Data File : PQ032424.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 Sep 2018 13:52  
 Operator : SM\SJ  
 Sample : J5126-17 100X  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 ECD\_Q  
 ClientSampleId :  
 C0BA5

Manual Integrations  
 APPROVED

Sohil  
 10/2/2018 6:34:11 AM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 01 03:57:21 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ092618CLP.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Sep 27 08:45:59 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------|-------|----------|----------|---------|-----------|
| -----                       |        |       |          |          |         |           |
| System Monitoring Compounds |        |       |          |          |         |           |
| 1) SA Tetrachlo...          | 4.594  | 3.871 | 548658   | 233921   | 0.357   | 0.203m#   |
| 2) SA Decachlor...          | 10.443 | 8.944 | 1811579  | 1214229  | 0.783   | 0.607     |
| Target Compounds            |        |       |          |          |         |           |
| 31) L7 AR-1260-1            | 7.377  | 6.457 | 70085705 | 67075732 | 592.446 | 614.386   |
| 32) L7 AR-1260-2            | 7.632  | 6.643 | 85527389 | 77710568 | 594.448 | 573.690   |
| 33) L7 AR-1260-3            | 7.993  | 6.800 | 47017705 | 71826282 | 450.140 | 569.807 # |
| 34) L7 AR-1260-4            | 8.224  | 7.272 | 67243591 | 46201550 | 537.101 | 434.296   |
| 35) L7 AR-1260-5            | 8.557  | 7.511 | 116.3E6  | 121.9E6  | 450.147 | 458.880   |
| -----                       |        |       |          |          |         |           |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.