

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100620\
 Data File : PQ050205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 17:54
 Operator : DD\AJ
 Sample : PCB GPC TEST 400 PPB
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PCB GPC TEST 400 PPB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 01:47:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ092420CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 24 08:00:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.202	0.000	23470773	0	2.371	N.D. #
2)	SA Decachlor...	11.397	9.617	12078045	8133436	1.779	1.512
Target Compounds							
3)	L1 AR-1016-1	6.540	5.530	464.5E6	197.4E6	1437.648	1187.686
4)	L1 AR-1016-2	6.564	5.550	670.7E6	278.3E6	1426.850	1245.896
5)	L1 AR-1016-3	6.630	5.743	403.2E6	147.2E6	1328.303	1242.390
6)	L1 AR-1016-4	6.739	5.793	337.9E6	105.8E6	1389.755	1121.582
7)	L1 AR-1016-5	7.052	6.024	304.6E6	147.8E6	1379.897	1195.614
8)	L2 AR-1221-1	5.459	4.527	47412846	14201095	394.234	334.045
9)	L2 AR-1221-2	5.564	4.629	51433467	16790855	610.969	551.725
10)	L2 AR-1221-3	5.653	4.717	237.4E6	82837685	877.334	790.256
11)	L3 AR-1232-1	5.653	4.717	237.4E6	82837685	1134.162	1028.978
12)	L3 AR-1232-2	6.244	5.550	329.3E6	278.3E6	3098.581	2933.701
13)	L3 AR-1232-3	6.564	5.743	670.7E6	147.2E6	3100.699	2972.058
14)	L3 AR-1232-4	6.739	5.839	337.9E6	133.1E6	3206.101	2987.563
15)	L3 AR-1232-5	6.832	6.024	276.7E6	147.8E6	3673.276	2908.742
16)	L4 AR-1242-1	6.540	5.530	464.5E6	197.4E6	1722.304	1553.267
17)	L4 AR-1242-2	6.564	5.550	670.7E6	278.3E6	1776.305	1602.602
18)	L4 AR-1242-3	6.630	5.743	403.2E6	147.2E6	1692.574	1593.014
19)	L4 AR-1242-4	6.739	5.839	337.9E6	133.1E6	1743.721	1487.834
20)	L4 AR-1242-5	7.522	6.402	47830674	124.0E6	248.303	930.285 #
21)	L5 AR-1248-1	6.540	5.530	464.5E6	197.4E6	2136.455	1927.997
22)	L5 AR-1248-2	6.832	5.793	276.7E6	105.8E6	999.133	811.976
23)	L5 AR-1248-3	7.052	5.839	304.6E6	133.1E6	1013.666	1003.704
24)	L5 AR-1248-4	7.482	6.024	54410310	147.8E6	162.666	895.206 #
25)	L5 AR-1248-5	7.522	6.446	47830674	20465294	151.941	112.912 #
26)	L6 AR-1254-1	7.450	6.402	223.8E6	124.0E6	678.616	447.531 #
27)	L6 AR-1254-2	7.677	6.561	240.3E6	121.9E6	493.777	493.009
28)	L6 AR-1254-3	8.065	7.000	129.3E6	237.2E6	265.906	578.237 #
29)	L6 AR-1254-4	8.360	7.220	86558684	28287183	228.182	93.522 #
30)	L6 AR-1254-5	8.791	7.649	698.5E6	549.5E6	1868.988	1370.170 #
31)	L7 AR-1260-1	8.228	7.118	486.2E6	333.2E6	1492.974	1359.738
32)	L7 AR-1260-2	8.494	7.314	577.5E6	466.1E6	1492.024	1321.489
33)	L7 AR-1260-3	8.860	7.470	368.5E6	411.2E6	1227.194	1364.698
34)	L7 AR-1260-4	9.105	7.954	425.7E6	324.8E6	1320.503	1191.417
35)	L7 AR-1260-5	9.452	8.200	836.9E6	962.1E6	1247.126	1248.135
36)	L8 AR-1262-1	8.860	7.649	368.5E6	549.5E6	844.815	2646.139 #
37)	L8 AR-1262-2	9.452	8.200	836.9E6	962.1E6	1085.783	1084.414
38)	L8 AR-1262-3	9.779	8.487	183.1E6	186.8E6	500.356	506.393
39)	L8 AR-1262-4	9.863	8.550	320.8E6	670.6E6	725.097	1050.058 #
40)	L8 AR-1262-5	10.598	9.056	239.8E6	232.8E6	697.411	697.884
41)	L9 AR-1268-1	9.779	8.487	183.1E6	186.8E6	190.511	166.546
42)	L9 AR-1268-2	9.863	8.550	320.8E6	670.6E6	348.661	690.801 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100620\
 Data File : PQ050205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 17:54
 Operator : DD\AJ
 Sample : PCB GPC TEST 400 PPB
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PCB GPC TEST 400 PPB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 01:47:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ092420CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 24 08:00:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	10.121	8.762	20414805	14952110	26.421	18.014 #
44) L9	AR-1268-4	10.598	9.056	239.8E6	232.8E6	620.088	611.508
45) L9	AR-1268-5	11.039	9.356	88856983	69246275	34.586	26.970



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100620\
Data File : PQ050205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 17:54
Operator : DD\AJ
Sample : PCB GPC TEST 400 PPB
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 01:47:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ092420CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 24 08:00:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

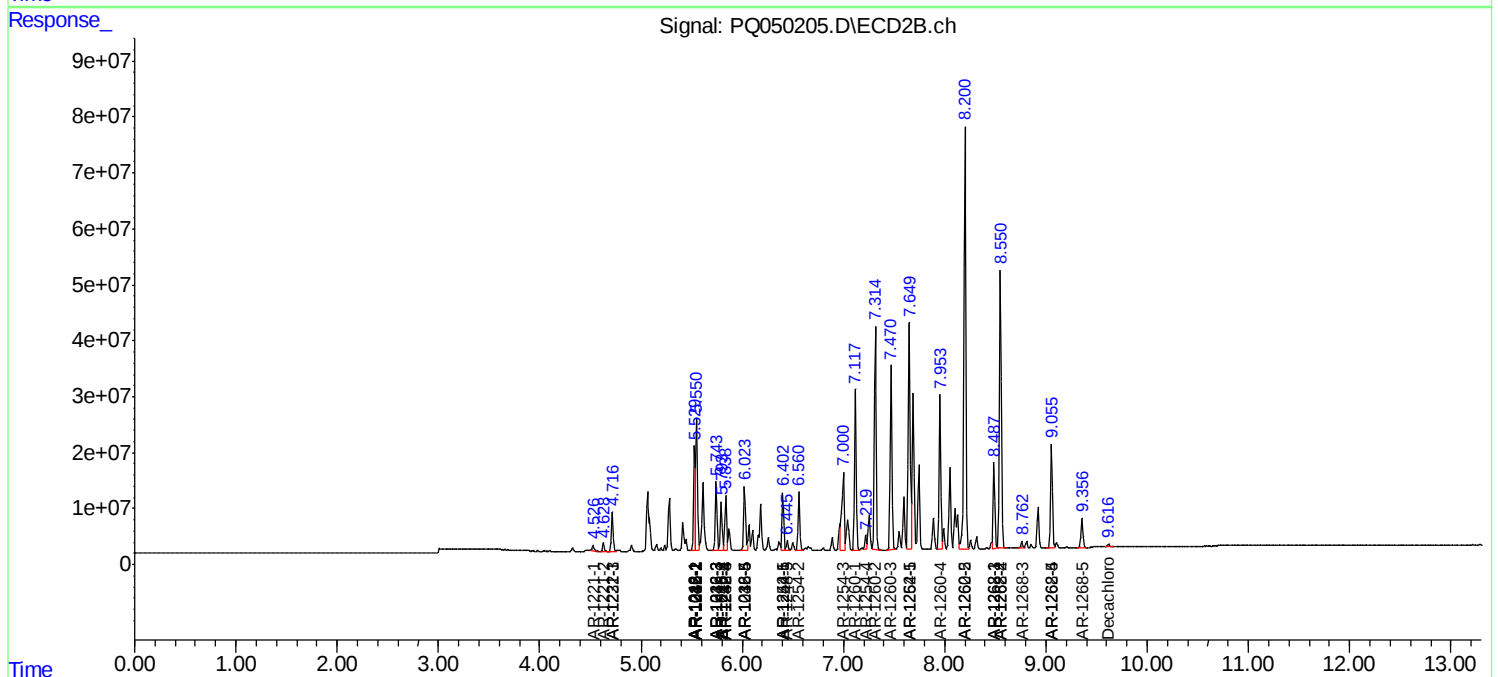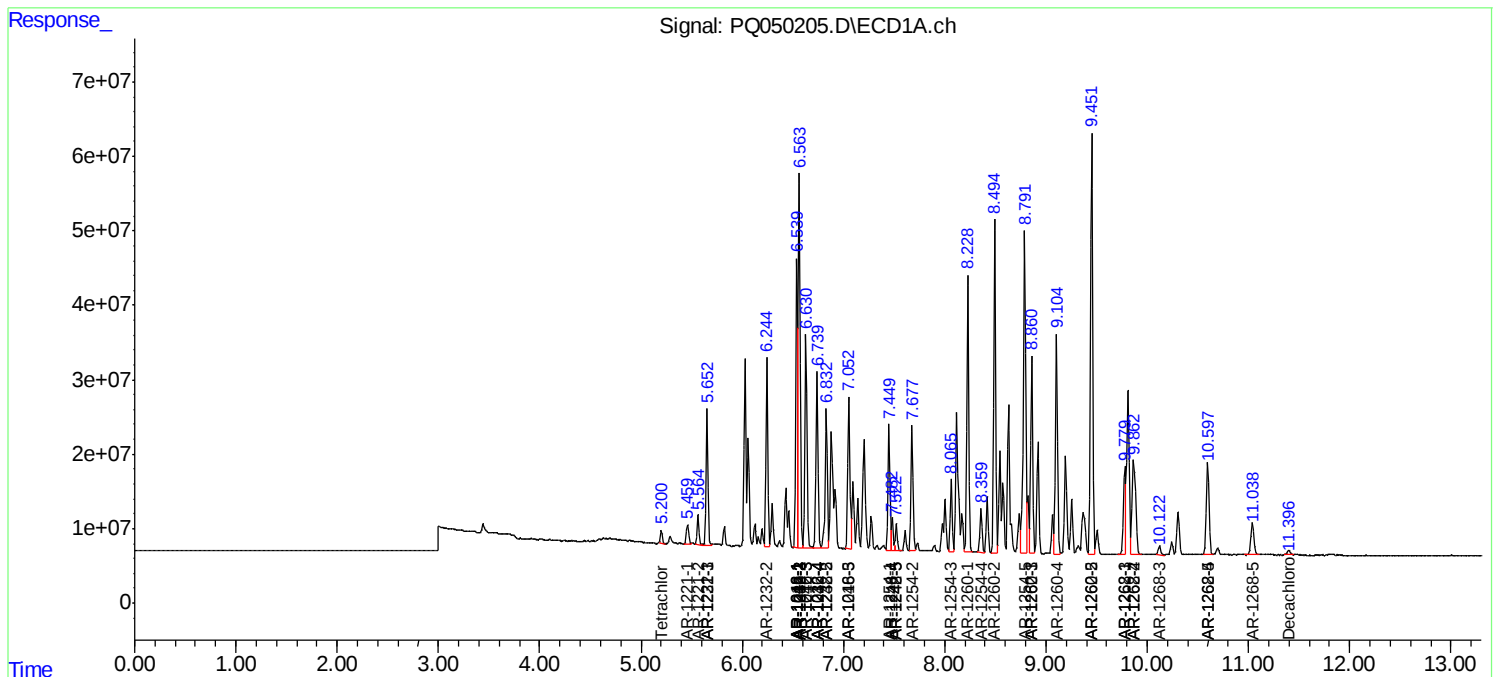


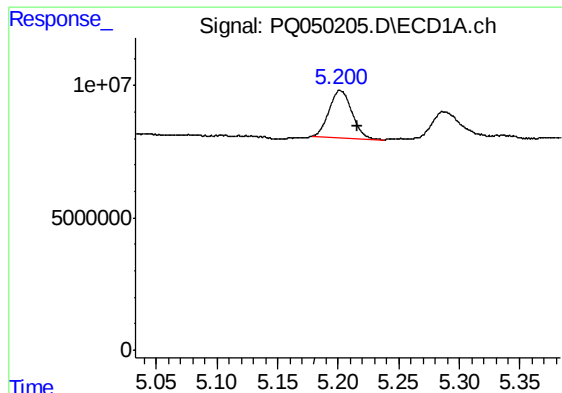

#1 Tetrachloro-m-xylene


R.T.: 5.202 min
Delta R.T.: -0.014 min
Response: 23470773
Conc: 2.37 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

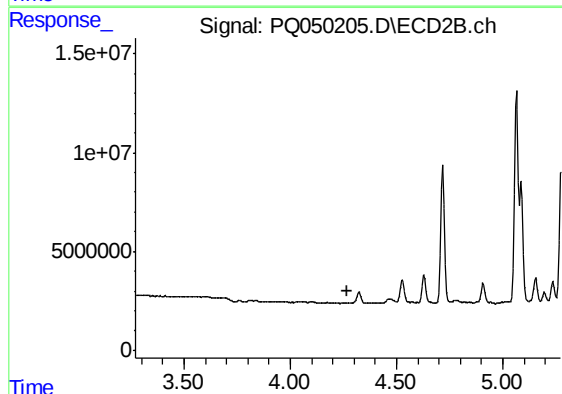


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.271 min
Response: 0
Conc: N.D.




#2 Decachlorobiphenyl

R.T.: 11.397 min
Delta R.T.: -0.019 min
Response: 12078045
Conc: 1.78 ng/ml

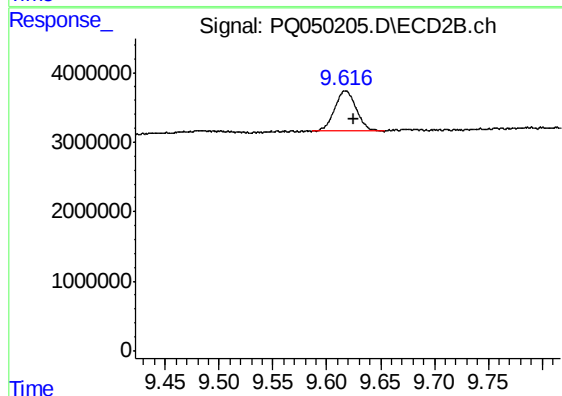

#2 Decachlorobiphenyl


R.T.: 9.617 min
Delta R.T.: -0.008 min
Response: 8133436
Conc: 1.51 ng/ml

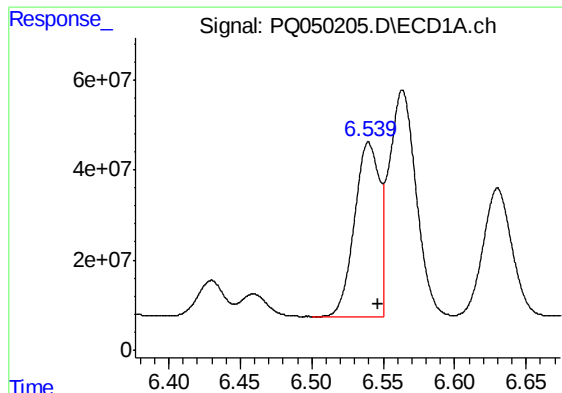

#3 AR-1016-1


R.T.: 6.540 min
Delta R.T.: -0.007 min
Response: 464525888
Conc: 1437.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

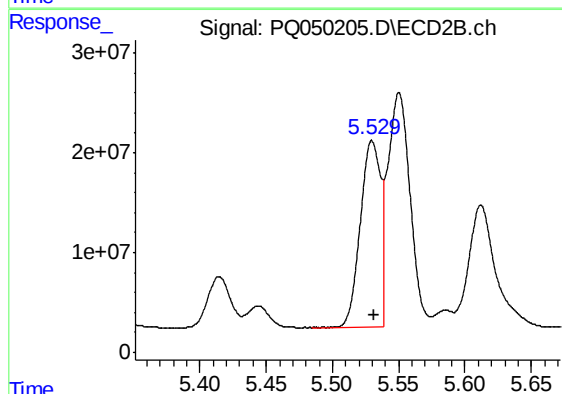


#3 AR-1016-1

R.T.: 5.530 min
Delta R.T.: -0.001 min
Response: 197411387
Conc: 1187.69 ng/ml

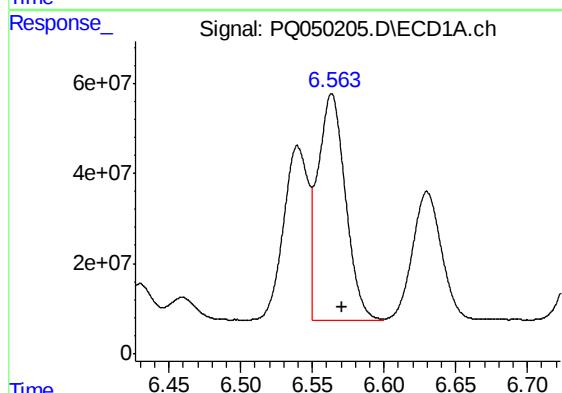


#4 AR-1016-2

R.T.: 6.564 min
Delta R.T.: -0.007 min
Response: 670745765
Conc: 1426.85 ng/ml

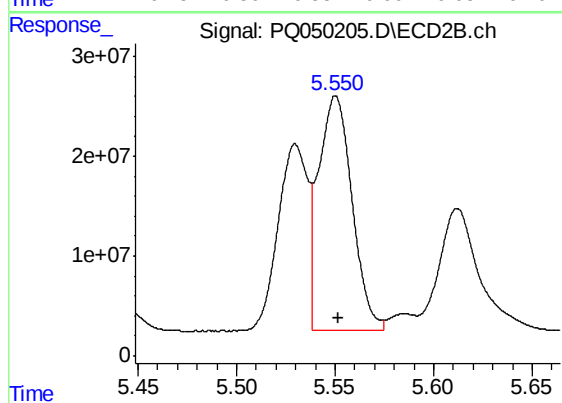

#4 AR-1016-2


R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 278338595
Conc: 1245.90 ng/ml



#5 AR-1016-3


R.T.: 6.630 min
Delta R.T.: -0.007 min
Response: 403235436
Conc: 1328.30 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

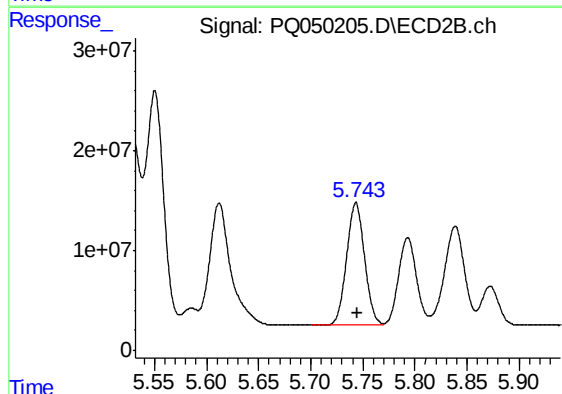


#5 AR-1016-3

R.T.: 5.743 min
Delta R.T.: -0.001 min
Response: 147201685
Conc: 1242.39 ng/ml




#6 AR-1016-4

R.T.: 6.739 min
Delta R.T.: -0.007 min
Response: 337888503
Conc: 1389.76 ng/ml

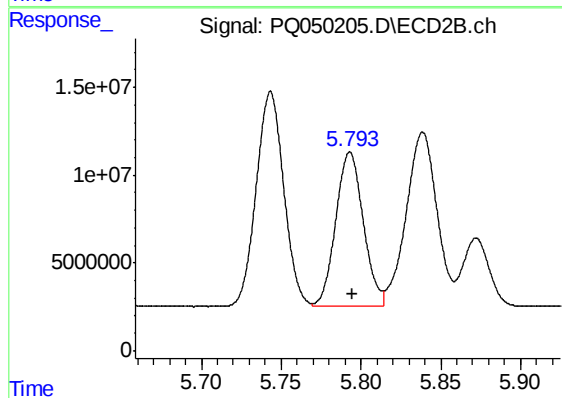

#6 AR-1016-4


R.T.: 5.793 min
Delta R.T.: -0.002 min
Response: 105849515
Conc: 1121.58 ng/ml

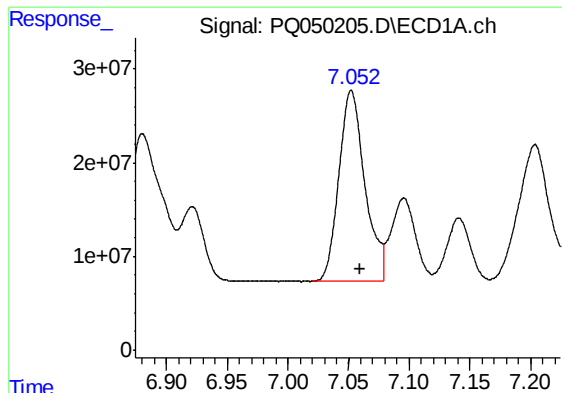

#7 AR-1016-5


R.T.: 7.052 min
Delta R.T.: -0.008 min
Response: 304638615
Conc: 1379.90 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

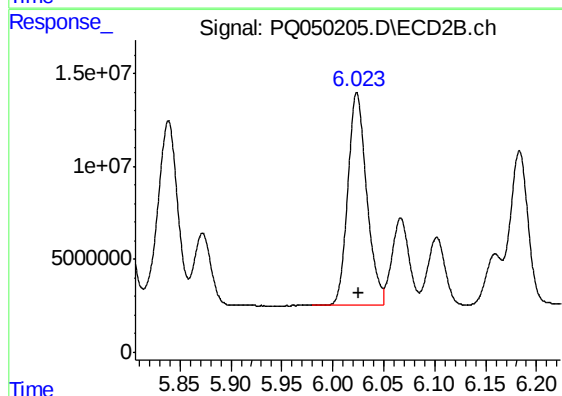


#7 AR-1016-5

R.T.: 6.024 min
Delta R.T.: -0.002 min
Response: 147810884
Conc: 1195.61 ng/ml

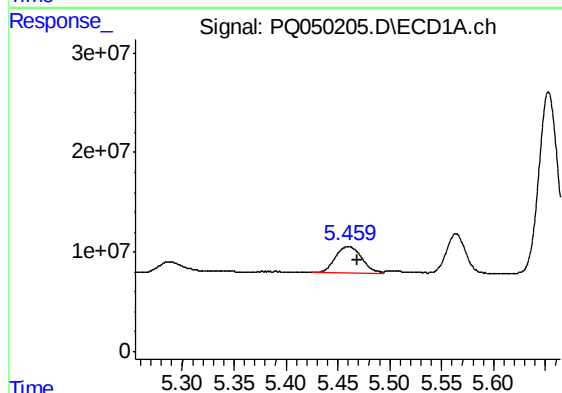


#8 AR-1221-1

R.T.: 5.459 min
Delta R.T.: -0.009 min
Response: 47412846
Conc: 394.23 ng/ml

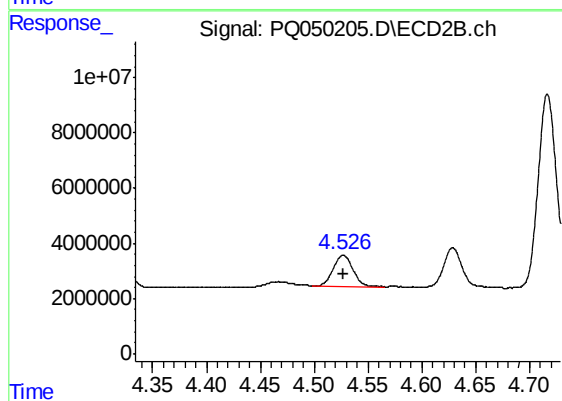

#8 AR-1221-1


R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 14201095
Conc: 334.04 ng/ml



#9 AR-1221-2


R.T.: 5.564 min
Delta R.T.: -0.004 min
Response: 51433467
Conc: 610.97 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

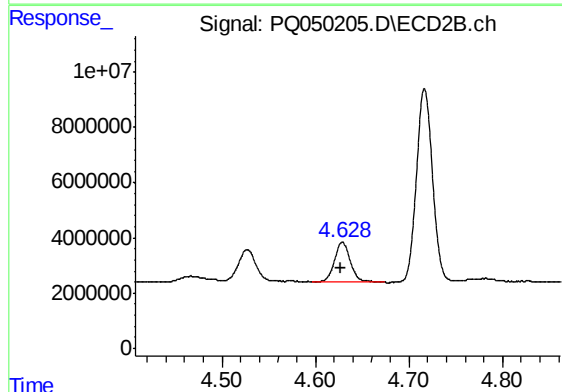


#9 AR-1221-2

R.T.: 4.629 min
Delta R.T.: 0.002 min
Response: 16790855
Conc: 551.72 ng/ml

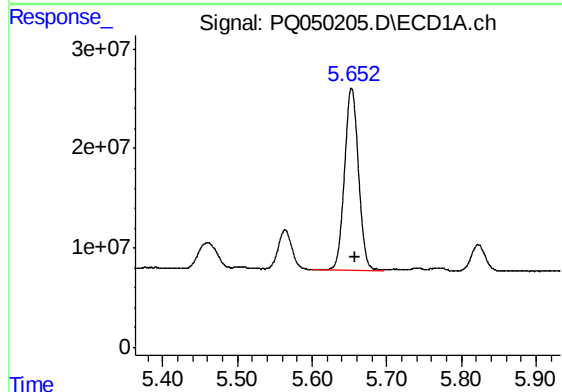


#10 AR-1221-3

R.T.: 5.653 min
Delta R.T.: -0.005 min
Response: 237385001
Conc: 877.33 ng/ml

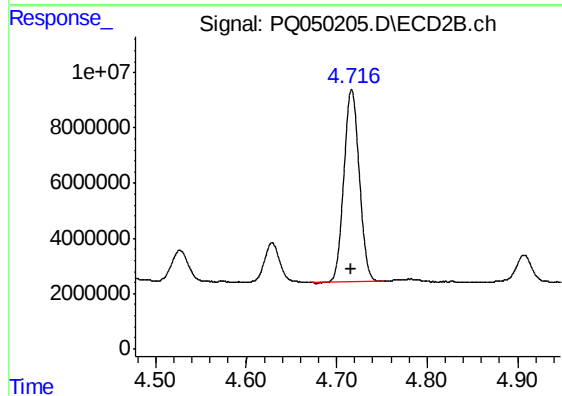

#10 AR-1221-3


R.T.: 4.717 min
Delta R.T.: 0.000 min
Response: 82837685
Conc: 790.26 ng/ml



#11 AR-1232-1


R.T.: 5.653 min
Delta R.T.: -0.005 min
Response: 237385001
Conc: 1134.16 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

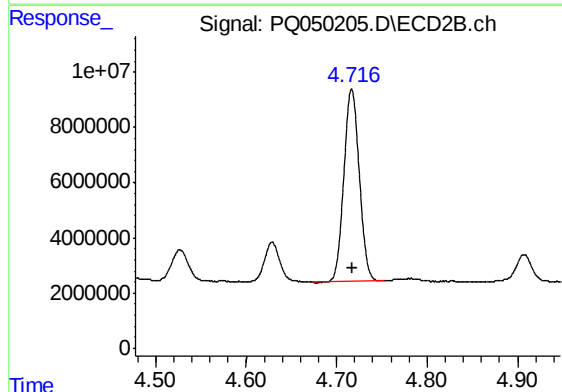


#11 AR-1232-1

R.T.: 4.717 min
Delta R.T.: 0.000 min
Response: 82837685
Conc: 1028.98 ng/ml

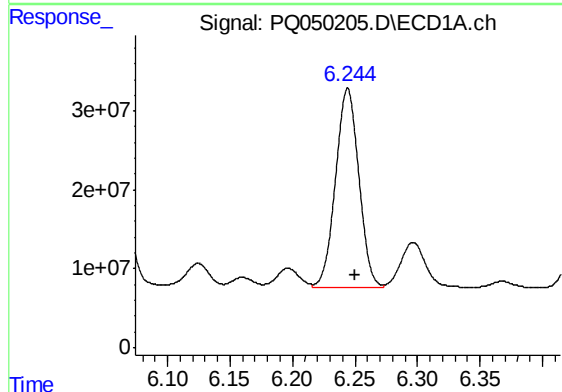


#12 AR-1232-2

R.T.: 6.244 min
Delta R.T.: -0.006 min
Response: 329312551
Conc: 3098.58 ng/ml

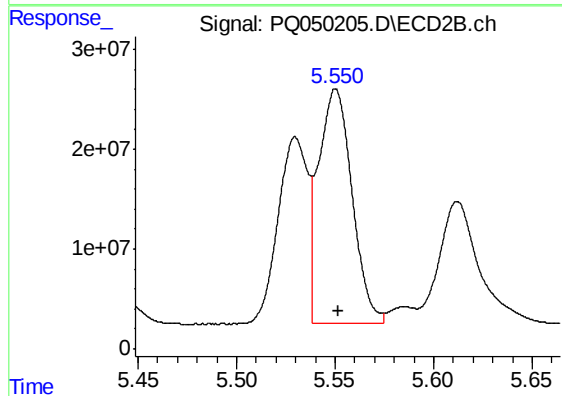

#12 AR-1232-2


R.T.: 5.550 min
Delta R.T.: -0.001 min
Response: 278338595
Conc: 2933.70 ng/ml



#13 AR-1232-3


R.T.: 6.564 min
Delta R.T.: -0.005 min
Response: 670745765
Conc: 3100.70 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

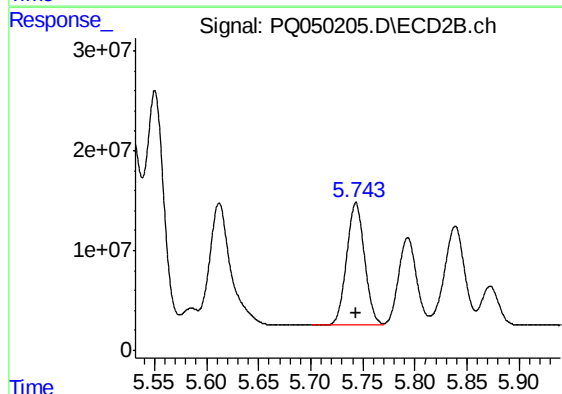


#13 AR-1232-3

R.T.: 5.743 min
Delta R.T.: 0.000 min
Response: 147201685
Conc: 2972.06 ng/ml




#14 AR-1232-4

R.T.: 6.739 min
Delta R.T.: -0.006 min
Response: 337888503
Conc: 3206.10 ng/ml

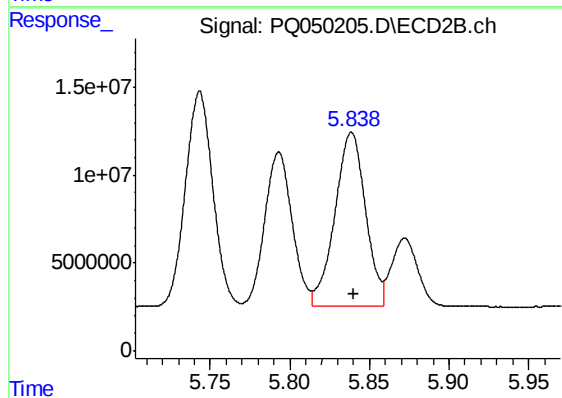

#14 AR-1232-4


R.T.: 5.839 min
Delta R.T.: -0.001 min
Response: 133145660
Conc: 2987.56 ng/ml

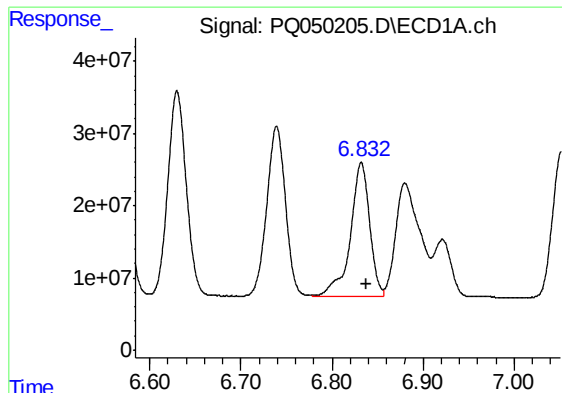

#15 AR-1232-5


R.T.: 6.832 min
Delta R.T.: -0.006 min
Response: 276713343
Conc: 3673.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

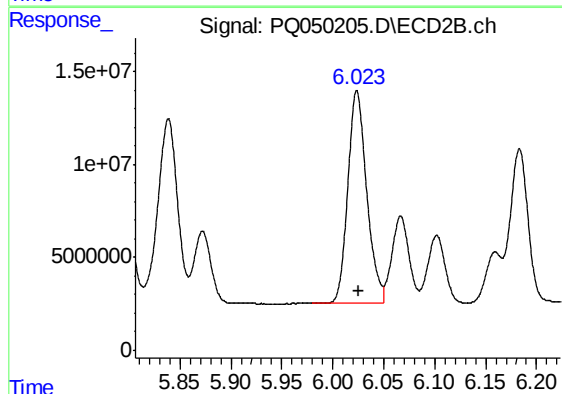


#15 AR-1232-5

R.T.: 6.024 min
Delta R.T.: -0.001 min
Response: 147810884
Conc: 2908.74 ng/ml

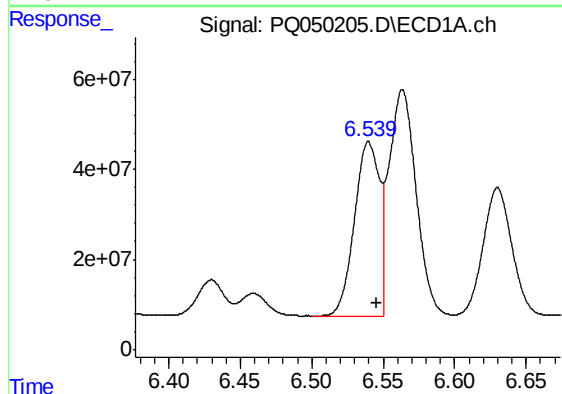


#16 AR-1242-1

R.T.: 6.540 min
Delta R.T.: -0.006 min
Response: 464525888
Conc: 1722.30 ng/ml

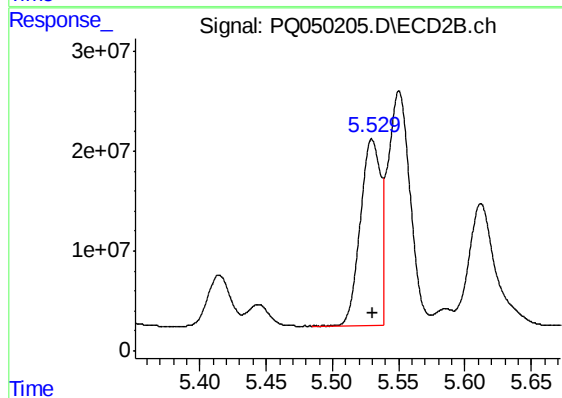

#16 AR-1242-1


R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 197411387
Conc: 1553.27 ng/ml



#17 AR-1242-2


R.T.: 6.564 min
Delta R.T.: -0.005 min
Response: 670745765
Conc: 1776.31 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

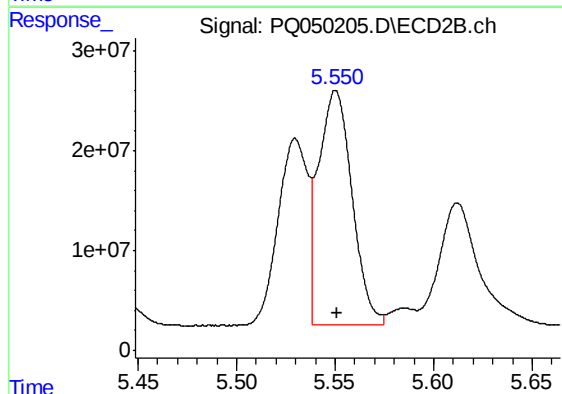


#17 AR-1242-2

R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 278338595
Conc: 1602.60 ng/ml

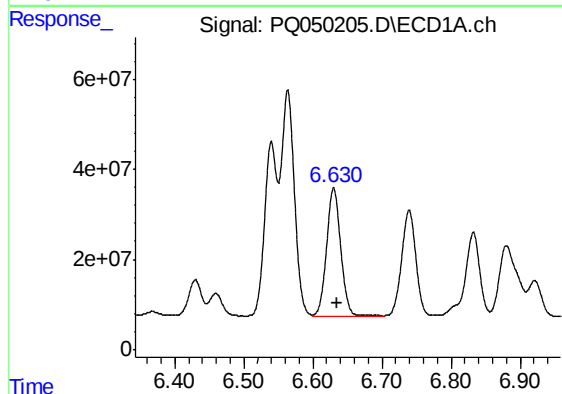


#18 AR-1242-3

R.T.: 6.630 min
Delta R.T.: -0.006 min
Response: 403235436
Conc: 1692.57 ng/ml

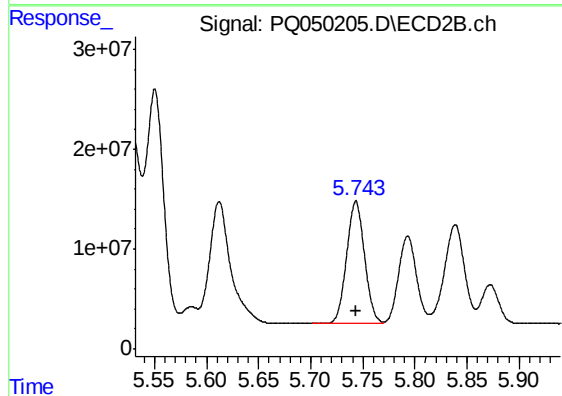

#18 AR-1242-3


R.T.: 5.743 min
Delta R.T.: 0.000 min
Response: 147201685
Conc: 1593.01 ng/ml



#19 AR-1242-4


R.T.: 6.739 min
Delta R.T.: -0.006 min
Response: 337888503
Conc: 1743.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

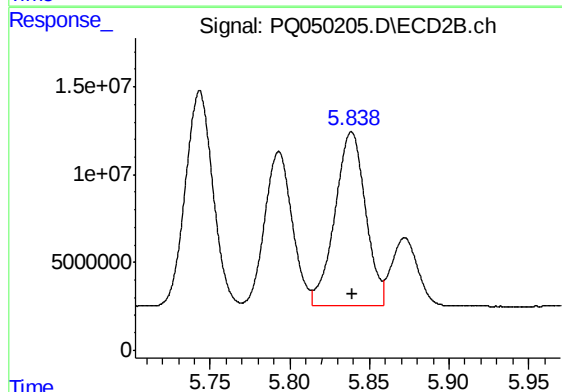


#19 AR-1242-4

R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 133145660
Conc: 1487.83 ng/ml




#20 AR-1242-5

R.T.: 7.522 min
Delta R.T.: -0.007 min
Response: 47830674
Conc: 248.30 ng/ml

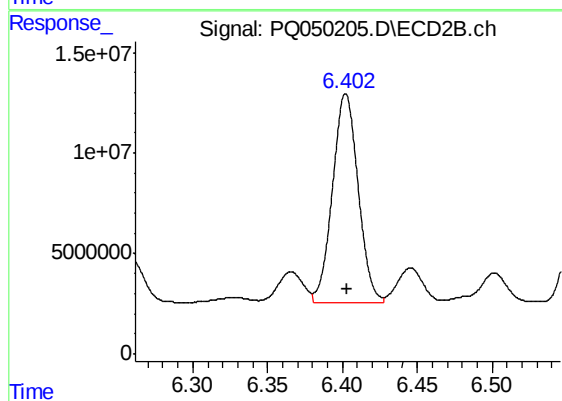

#20 AR-1242-5


R.T.: 6.402 min
Delta R.T.: -0.001 min
Response: 124013083
Conc: 930.28 ng/ml

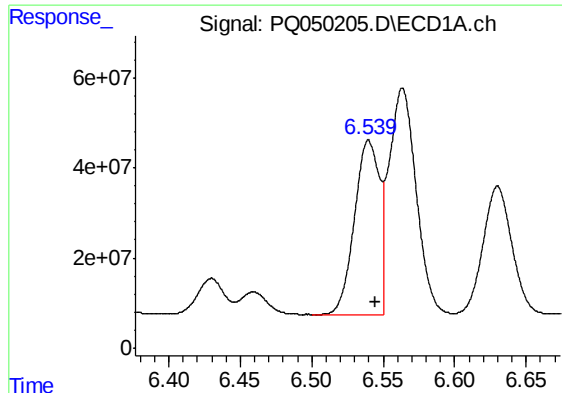

#21 AR-1248-1


R.T.: 6.540 min
Delta R.T.: -0.005 min
Response: 464525888
Conc: 2136.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

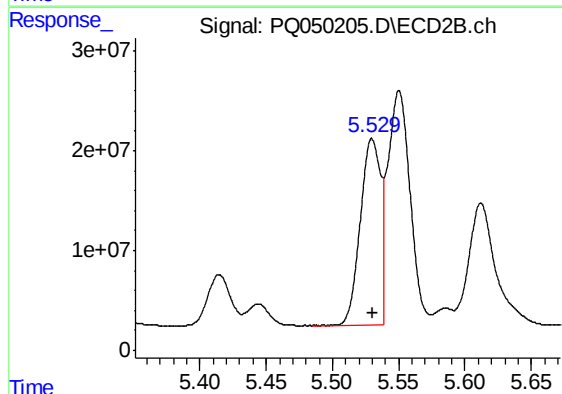


#21 AR-1248-1

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 197411387
Conc: 1928.00 ng/ml

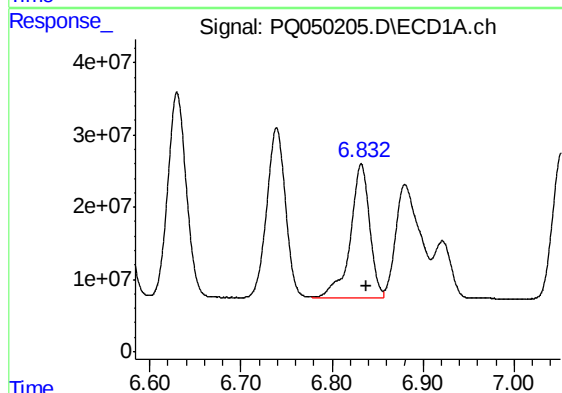


#22 AR-1248-2

R.T.: 6.832 min
Delta R.T.: -0.005 min
Response: 276713343
Conc: 999.13 ng/ml

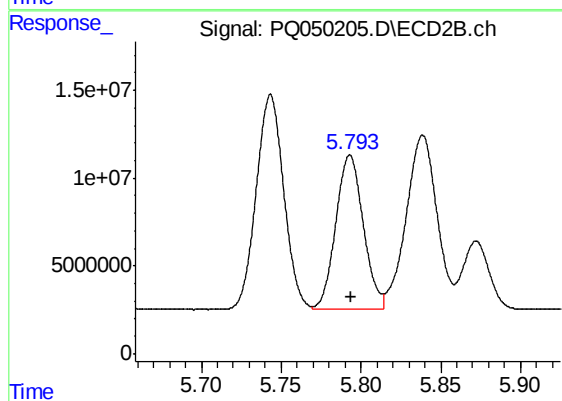

#22 AR-1248-2


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 105849515
Conc: 811.98 ng/ml



#23 AR-1248-3


R.T.: 7.052 min
Delta R.T.: -0.006 min
Response: 304638615
Conc: 1013.67 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

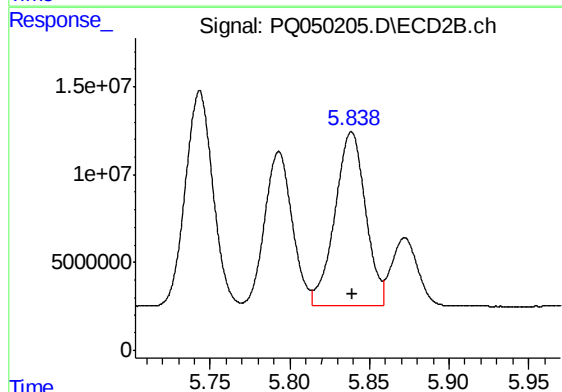


#23 AR-1248-3

R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 133145660
Conc: 1003.70 ng/ml




#24 AR-1248-4

R.T.: 7.482 min
Delta R.T.: -0.006 min
Response: 54410310
Conc: 162.67 ng/ml

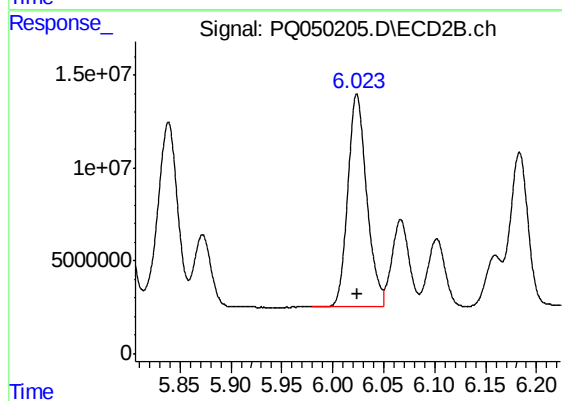

#24 AR-1248-4


R.T.: 6.024 min
Delta R.T.: -0.001 min
Response: 147810884
Conc: 895.21 ng/ml

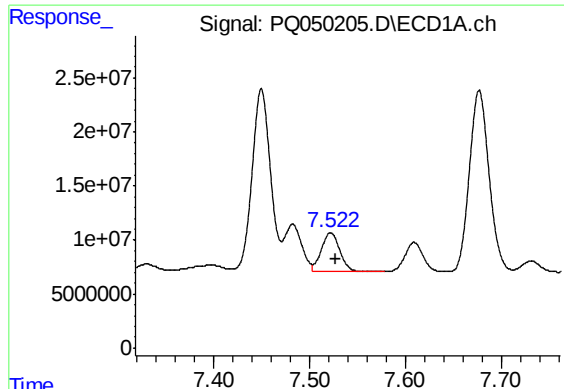

#25 AR-1248-5


R.T.: 7.522 min
Delta R.T.: -0.006 min
Response: 47830674
Conc: 151.94 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

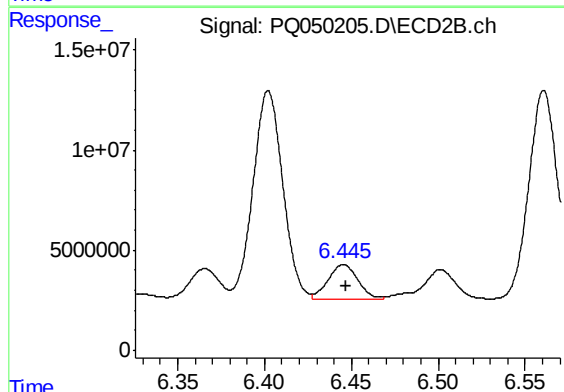


#25 AR-1248-5

R.T.: 6.446 min
Delta R.T.: -0.001 min
Response: 20465294
Conc: 112.91 ng/ml

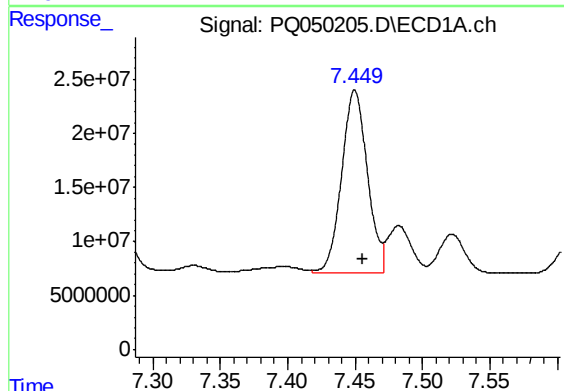


#26 AR-1254-1

R.T.: 7.450 min
Delta R.T.: -0.006 min
Response: 223846420
Conc: 678.62 ng/ml

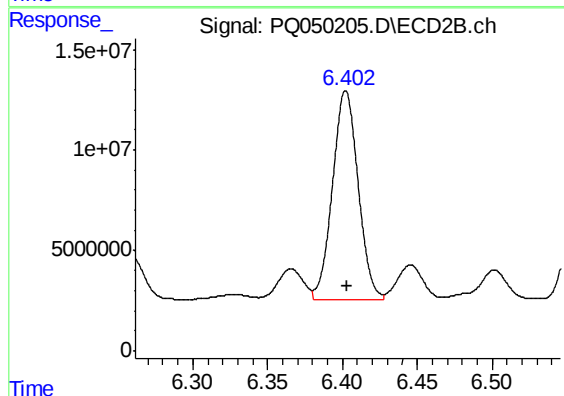

#26 AR-1254-1


R.T.: 6.402 min
Delta R.T.: -0.001 min
Response: 124013083
Conc: 447.53 ng/ml



#27 AR-1254-2


R.T.: 7.677 min
Delta R.T.: -0.007 min
Response: 240296328
Conc: 493.78 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

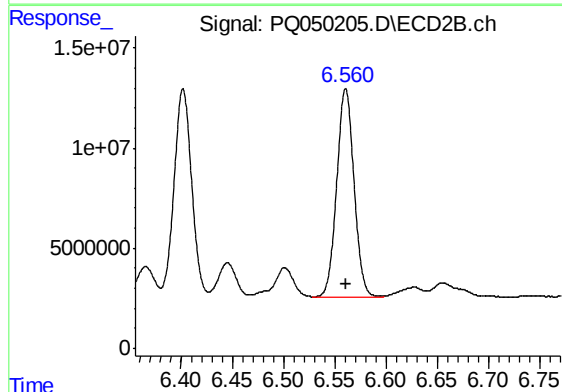


#27 AR-1254-2

R.T.: 6.561 min
Delta R.T.: 0.000 min
Response: 121932731
Conc: 493.01 ng/ml

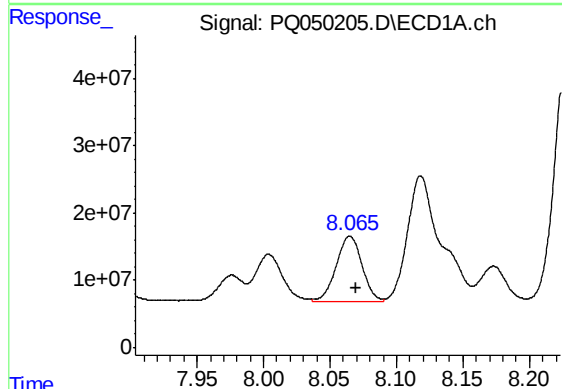


#28 AR-1254-3

R.T.: 8.065 min
Delta R.T.: -0.005 min
Response: 129264198
Conc: 265.91 ng/ml

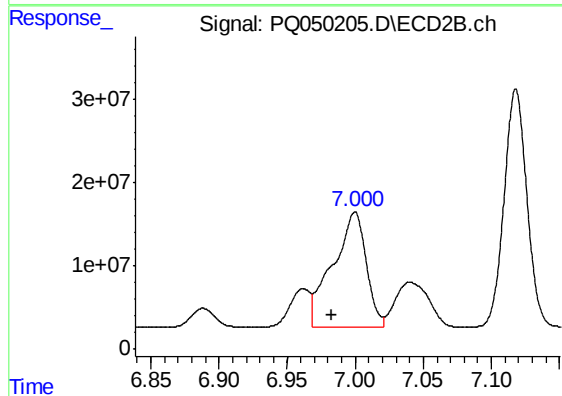

#28 AR-1254-3


R.T.: 7.000 min
Delta R.T.: 0.017 min
Response: 237169655
Conc: 578.24 ng/ml

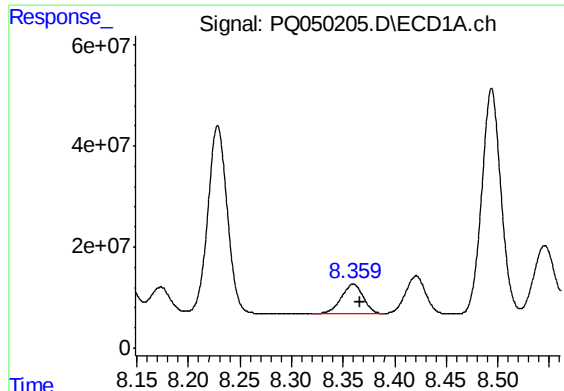

#29 AR-1254-4


R.T.: 8.360 min
Delta R.T.: -0.007 min
Response: 86558684
Conc: 228.18 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

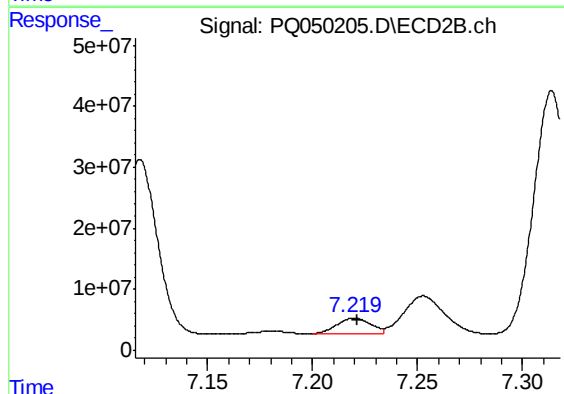


#29 AR-1254-4

R.T.: 7.220 min
Delta R.T.: -0.001 min
Response: 28287183
Conc: 93.52 ng/ml

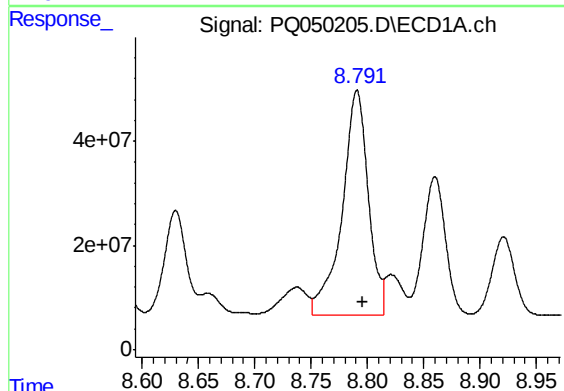


#30 AR-1254-5

R.T.: 8.791 min
Delta R.T.: -0.005 min
Response: 698453802
Conc: 1868.99 ng/ml

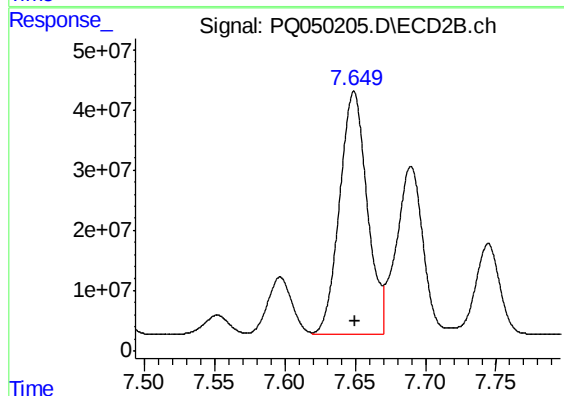

#30 AR-1254-5


R.T.: 7.649 min
Delta R.T.: -0.001 min
Response: 549489351
Conc: 1370.17 ng/ml



#31 AR-1260-1


R.T.: 8.228 min
Delta R.T.: -0.010 min
Response: 486219353
Conc: 1492.97 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

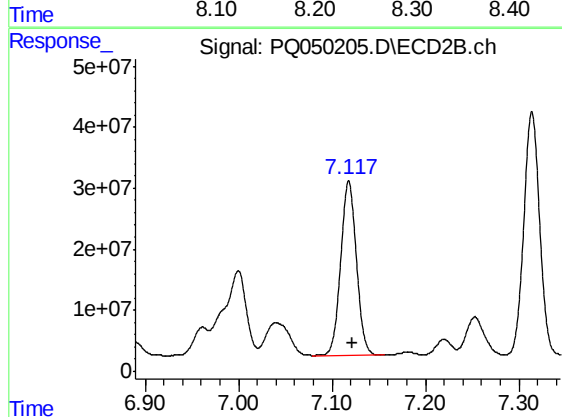


#31 AR-1260-1

R.T.: 7.118 min
Delta R.T.: -0.004 min
Response: 333208865
Conc: 1359.74 ng/ml

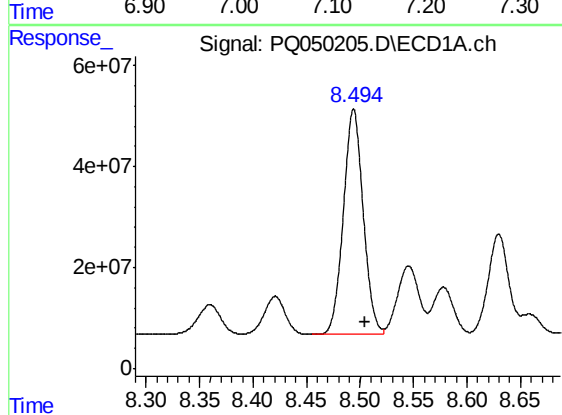


#32 AR-1260-2

R.T.: 8.494 min
Delta R.T.: -0.010 min
Response: 577465799
Conc: 1492.02 ng/ml

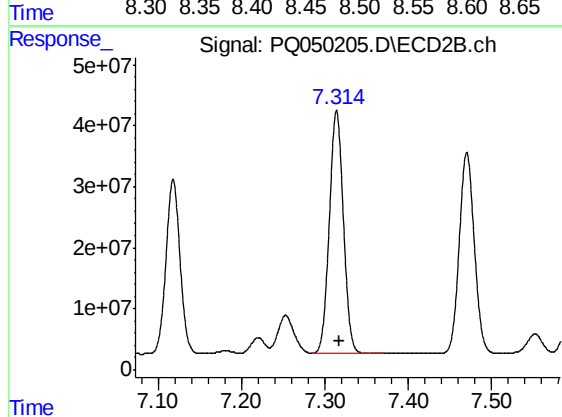

#32 AR-1260-2


R.T.: 7.314 min
Delta R.T.: -0.004 min
Response: 466050122
Conc: 1321.49 ng/ml



#33 AR-1260-3


R.T.: 8.860 min
Delta R.T.: -0.011 min
Response: 368482959
Conc: 1227.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

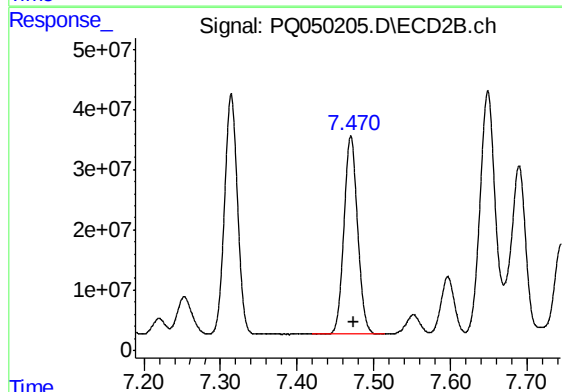


#33 AR-1260-3

R.T.: 7.470 min
Delta R.T.: -0.005 min
Response: 411224699
Conc: 1364.70 ng/ml




#34 AR-1260-4

R.T.: 9.105 min
Delta R.T.: -0.012 min
Response: 425706094
Conc: 1320.50 ng/ml

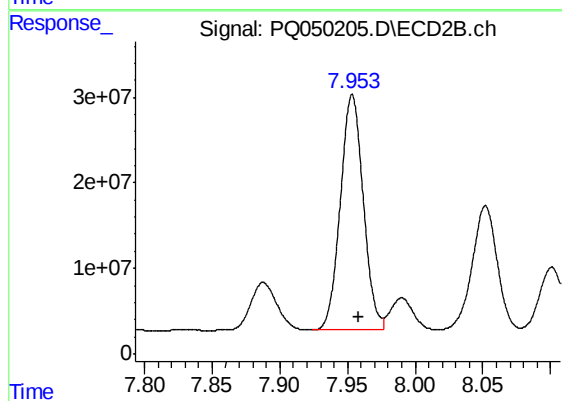

#34 AR-1260-4


R.T.: 7.954 min
Delta R.T.: -0.005 min
Response: 324847442
Conc: 1191.42 ng/ml



#35 AR-1260-5


R.T.: 9.452 min
Delta R.T.: -0.012 min
Response: 836892704
Conc: 1247.13 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

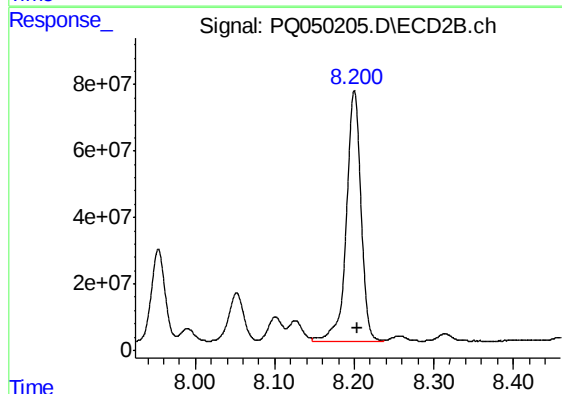


#35 AR-1260-5

R.T.: 8.200 min
Delta R.T.: -0.005 min
Response: 962129841
Conc: 1248.14 ng/ml




#36 AR-1262-1

R.T.: 8.860 min
Delta R.T.: -0.004 min
Response: 368482959
Conc: 844.82 ng/ml

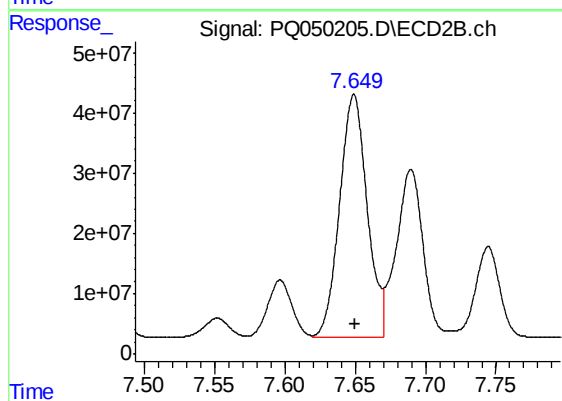

#36 AR-1262-1


R.T.: 7.649 min
Delta R.T.: 0.000 min
Response: 549489351
Conc: 2646.14 ng/ml

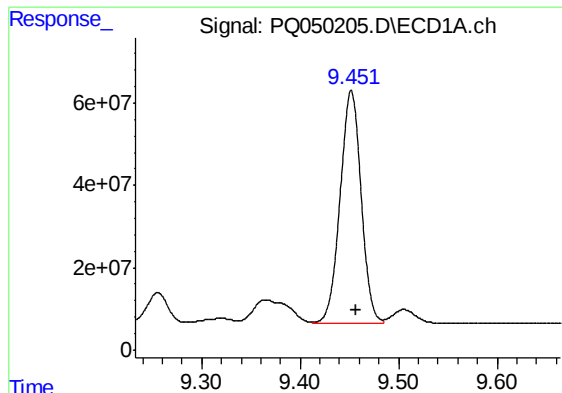

#37 AR-1262-2


R.T.: 9.452 min
Delta R.T.: -0.005 min
Response: 836892704
Conc: 1085.78 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

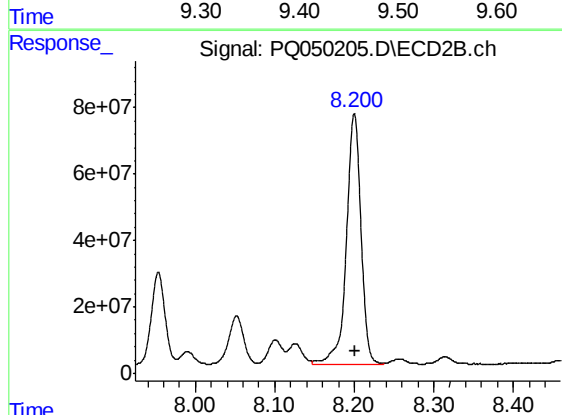


#37 AR-1262-2

R.T.: 8.200 min
Delta R.T.: 0.000 min
Response: 962129841
Conc: 1084.41 ng/ml

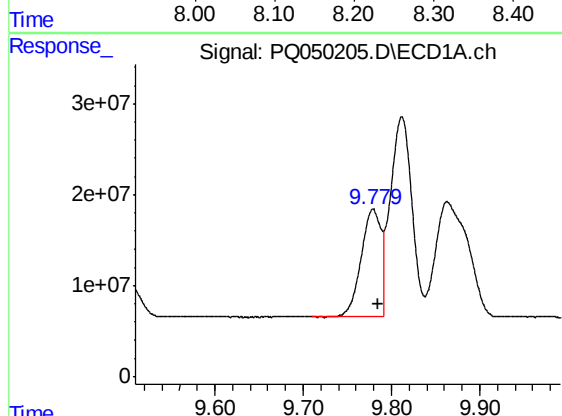


#38 AR-1262-3

R.T.: 9.779 min
Delta R.T.: -0.005 min
Response: 183108675
Conc: 500.36 ng/ml

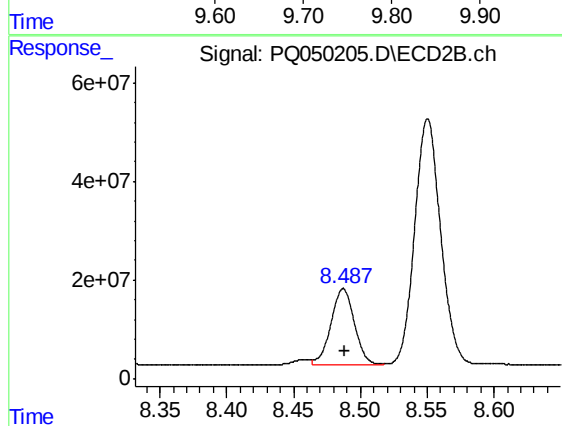

#38 AR-1262-3


R.T.: 8.487 min
Delta R.T.: 0.000 min
Response: 186768786
Conc: 506.39 ng/ml



#39 AR-1262-4


R.T.: 9.863 min
Delta R.T.: -0.022 min
Response: 320765927
Conc: 725.10 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

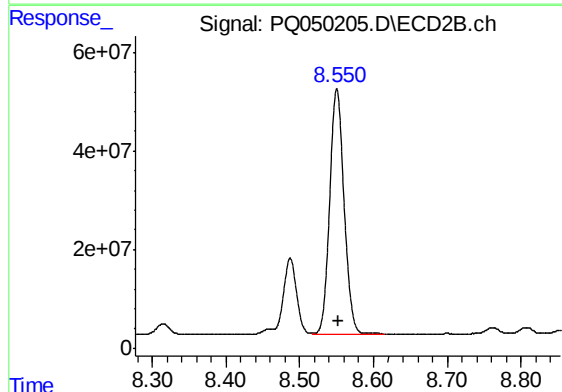


#39 AR-1262-4

R.T.: 8.550 min
Delta R.T.: -0.002 min
Response: 670571120
Conc: 1050.06 ng/ml

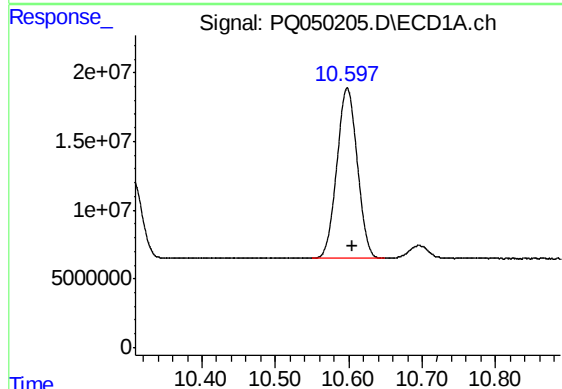


#40 AR-1262-5

R.T.: 10.598 min
Delta R.T.: -0.008 min
Response: 239781127
Conc: 697.41 ng/ml

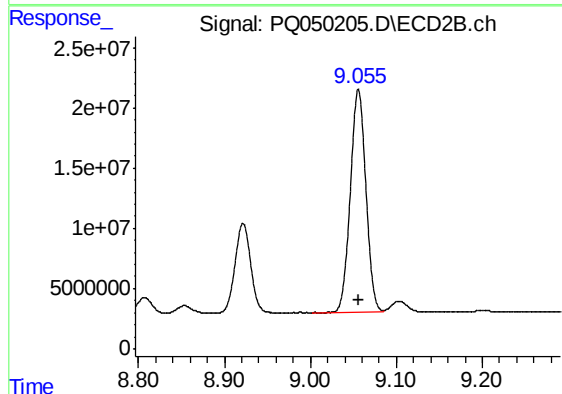

#40 AR-1262-5


R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 232846606
Conc: 697.88 ng/ml

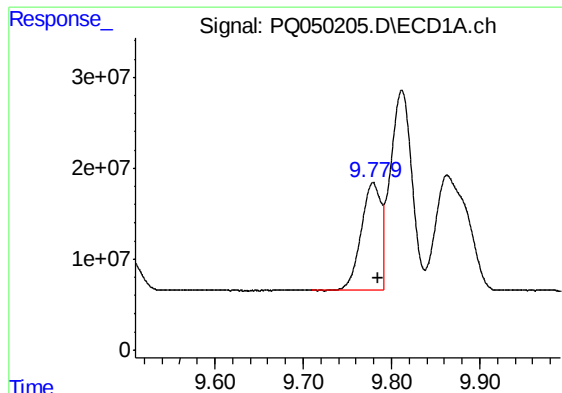

#41 AR-1268-1


R.T.: 9.779 min
Delta R.T.: -0.006 min
Response: 183108675
Conc: 190.51 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

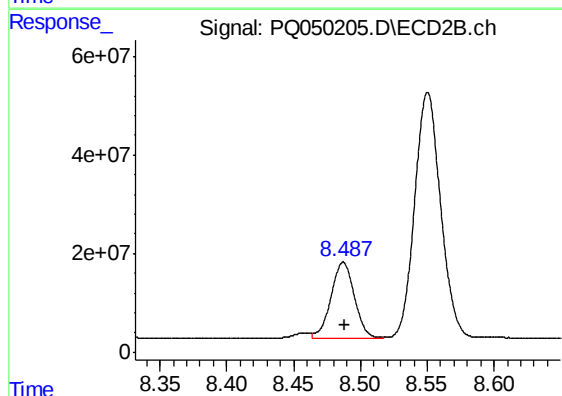


#41 AR-1268-1

R.T.: 8.487 min
Delta R.T.: 0.000 min
Response: 186768786
Conc: 166.55 ng/ml

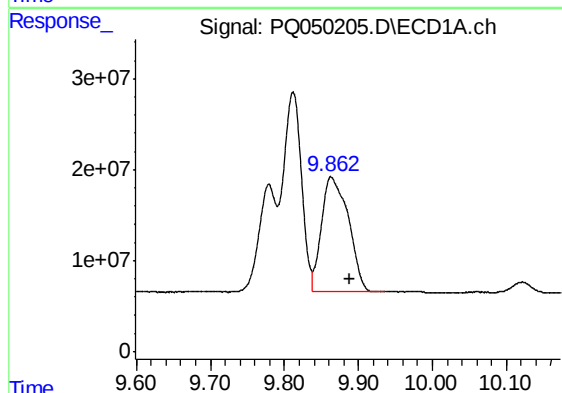


#42 AR-1268-2

R.T.: 9.863 min
Delta R.T.: -0.026 min
Response: 320765927
Conc: 348.66 ng/ml

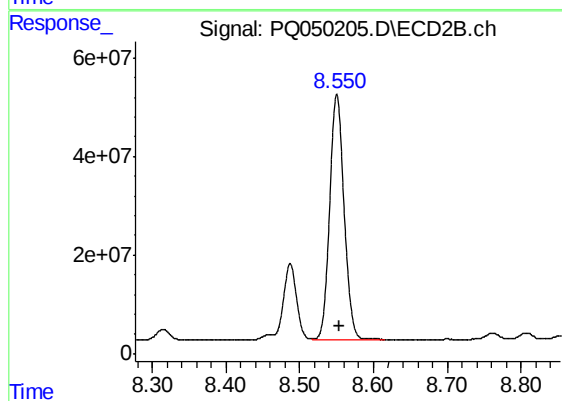

#42 AR-1268-2


R.T.: 8.550 min
Delta R.T.: -0.003 min
Response: 670571120
Conc: 690.80 ng/ml



#43 AR-1268-3


R.T.: 10.121 min
Delta R.T.: -0.007 min
Response: 20414805
Conc: 26.42 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

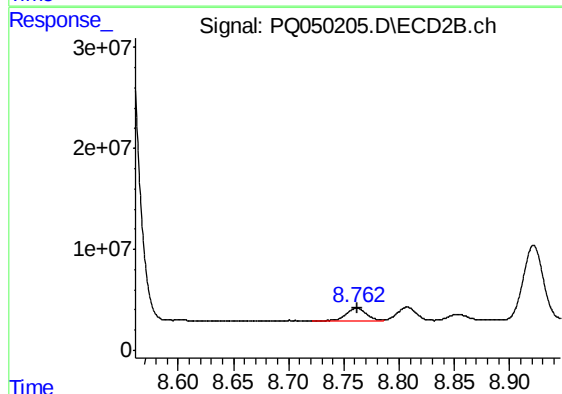


#43 AR-1268-3

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 14952110
Conc: 18.01 ng/ml




#44 AR-1268-4

R.T.: 10.598 min
Delta R.T.: -0.008 min
Response: 239781127
Conc: 620.09 ng/ml

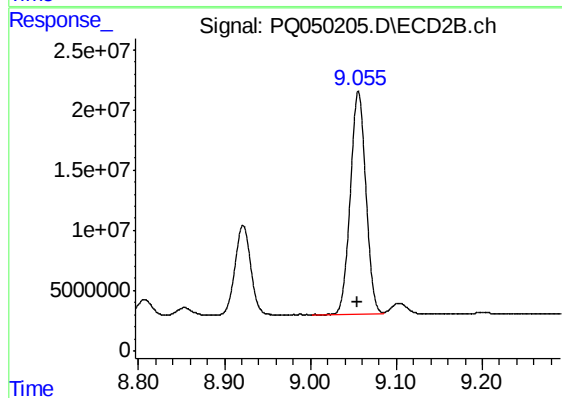

#44 AR-1268-4


R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 232846606
Conc: 611.51 ng/ml

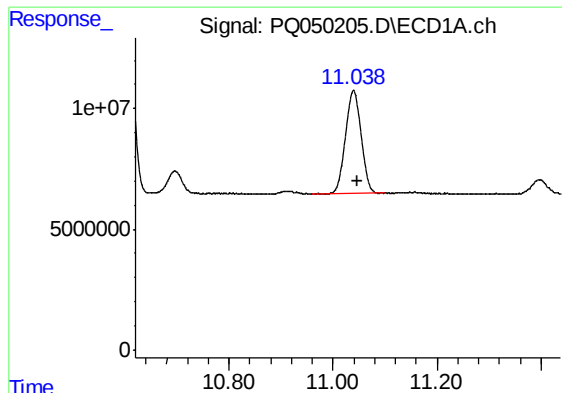

#45 AR-1268-5

R.T.: 11.039 min
Delta R.T.: -0.009 min
Response: 88856983
Conc: 34.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PCB GPC TEST 400 PPB

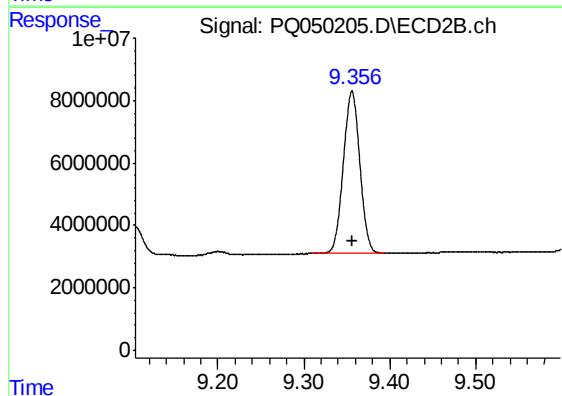

#45 AR-1268-5

R.T.: 9.356 min
Delta R.T.: 0.000 min
Response: 69246275
Conc: 26.97 ng/ml