

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100621\
 Data File : PQ054878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2021 02:12
 Operator : AJ\MA
 Sample : M4088-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 WC-20211005-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 03:55:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.195	4.203	411.4E6	197.7E6	17.227	14.954
2)	SA Decachlor...	11.354	9.522	201.8E6	151.1E6	11.958	11.148

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100621\
Data File : PQ054878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2021 02:12
Operator : AJ\MA
Sample : M4088-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
WC-20211005-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 03:55:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

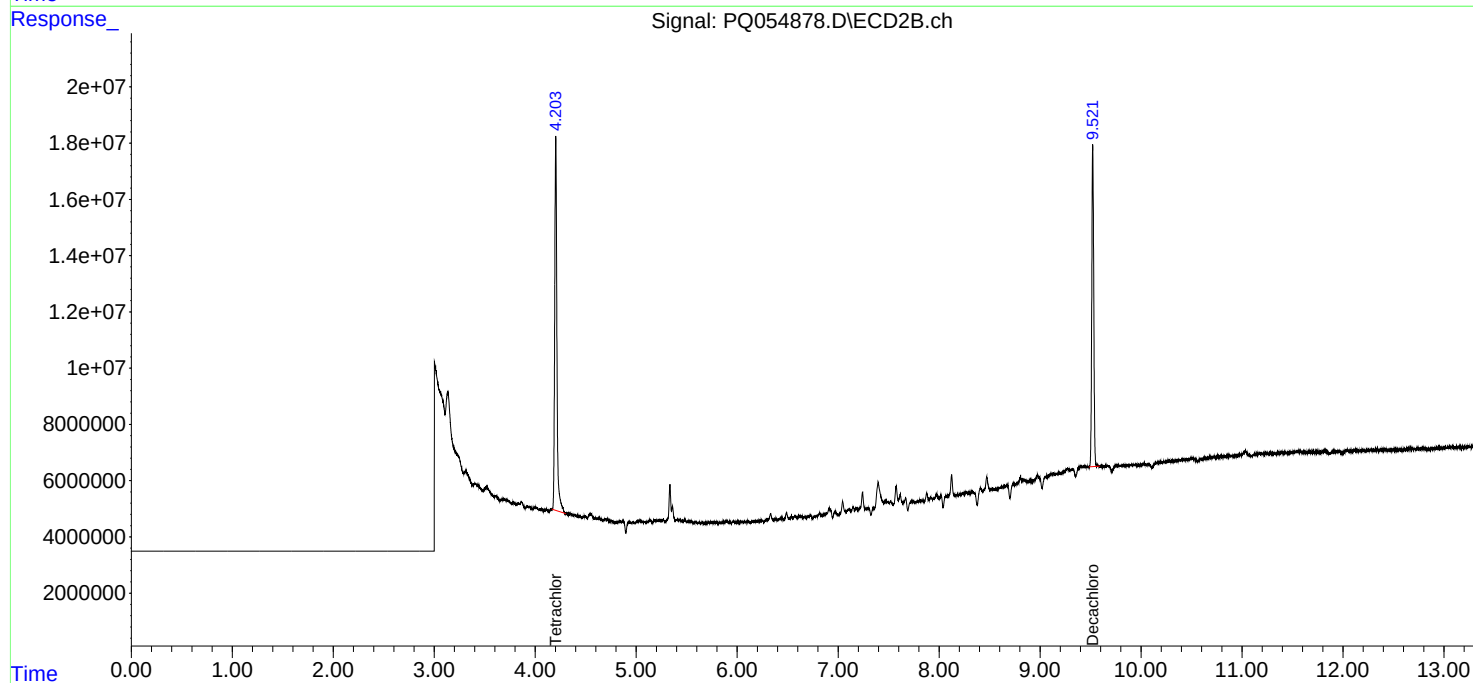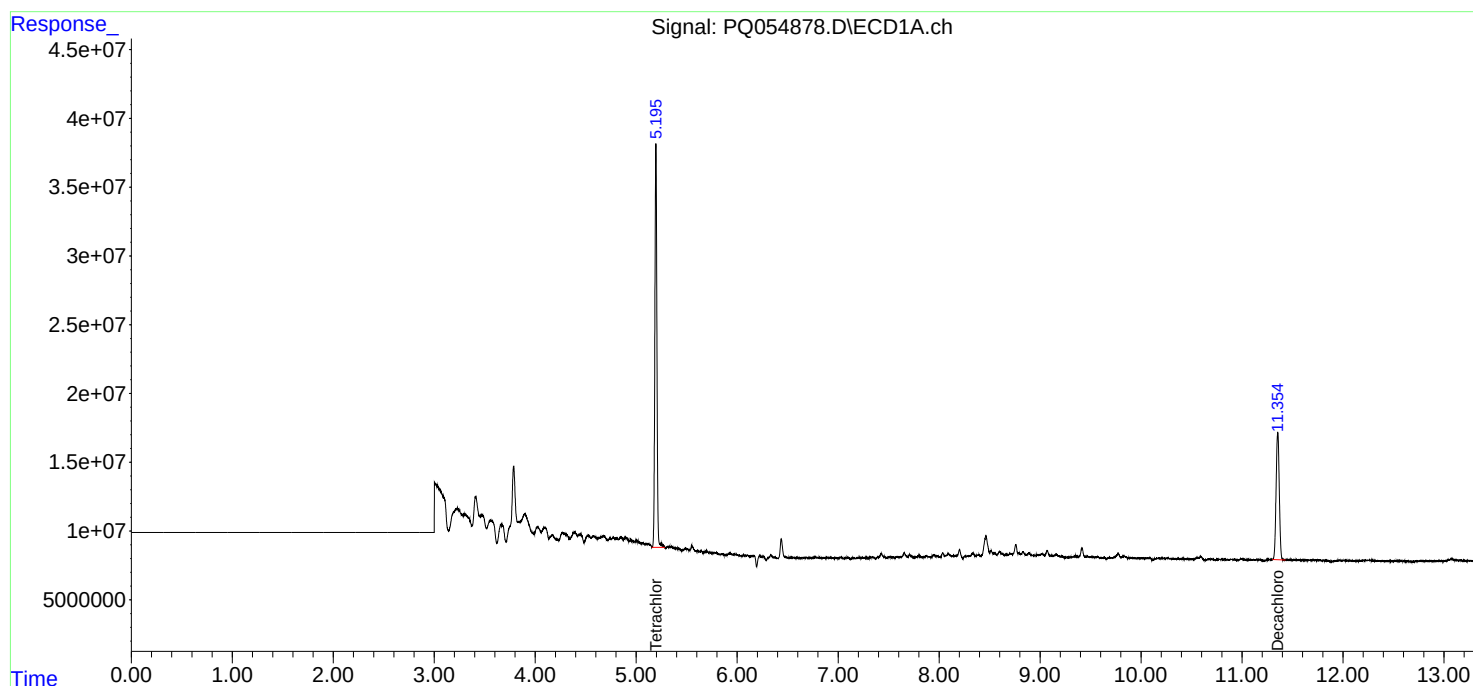


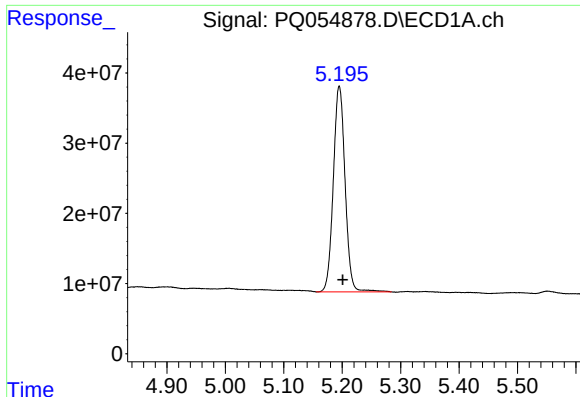

#1 Tetrachloro-m-xylene


R.T.: 5.195 min
Delta R.T.: -0.006 min
Response: 411411624
Conc: 17.23 ng/ml

Instrument :
ECD_Q
ClientSampleId :
WC-20211005-WATER

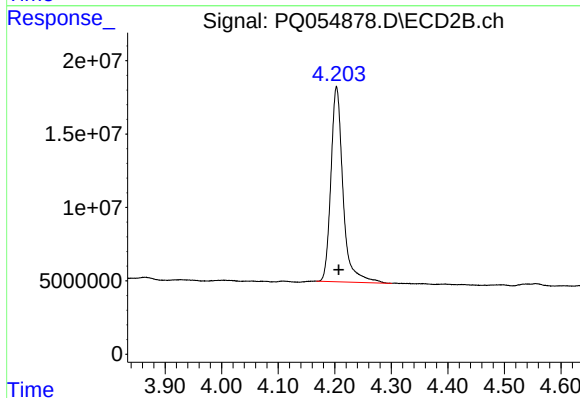


#1 Tetrachloro-m-xylene

R.T.: 4.203 min
Delta R.T.: -0.004 min
Response: 197686199
Conc: 14.95 ng/ml

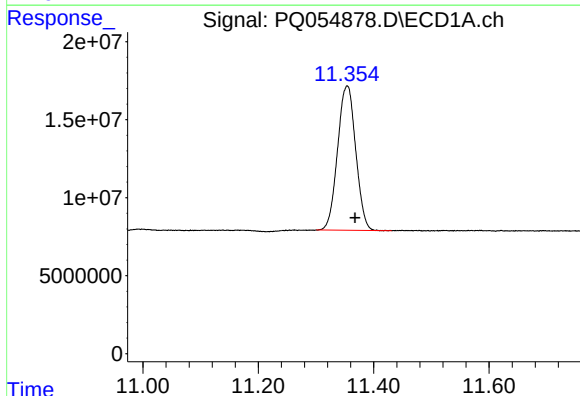

#2 Decachlorobiphenyl

R.T.: 11.354 min
Delta R.T.: -0.014 min
Response: 201828114
Conc: 11.96 ng/ml

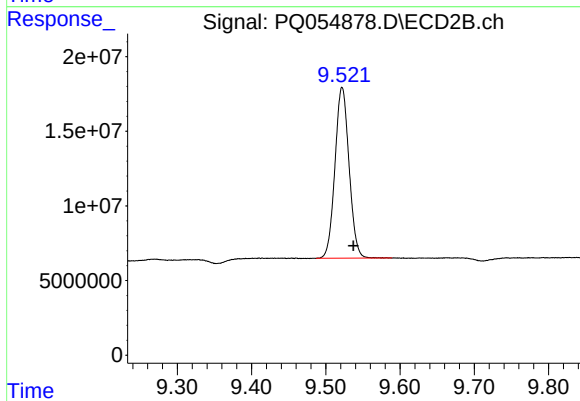

#2 Decachlorobiphenyl

R.T.: 9.522 min
Delta R.T.: -0.015 min
Response: 151077629
Conc: 11.15 ng/ml