

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100621\
 Data File : PQ054886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2021 05:05
 Operator : AJ\MA
 Sample : M4089-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20-SB-2-20211005-5.5-6.0-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 09:09:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.194	4.201	396.3E6	199.1E6	16.592	15.058
2) SA Decachlor...	11.355	9.523	223.5E6	146.5E6	13.243	10.810

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100621\
Data File : PQ054886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2021 05:05
Operator : AJ\MA
Sample : M4089-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
20-SB-2-20211005-5.5-6.0-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 09:09:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

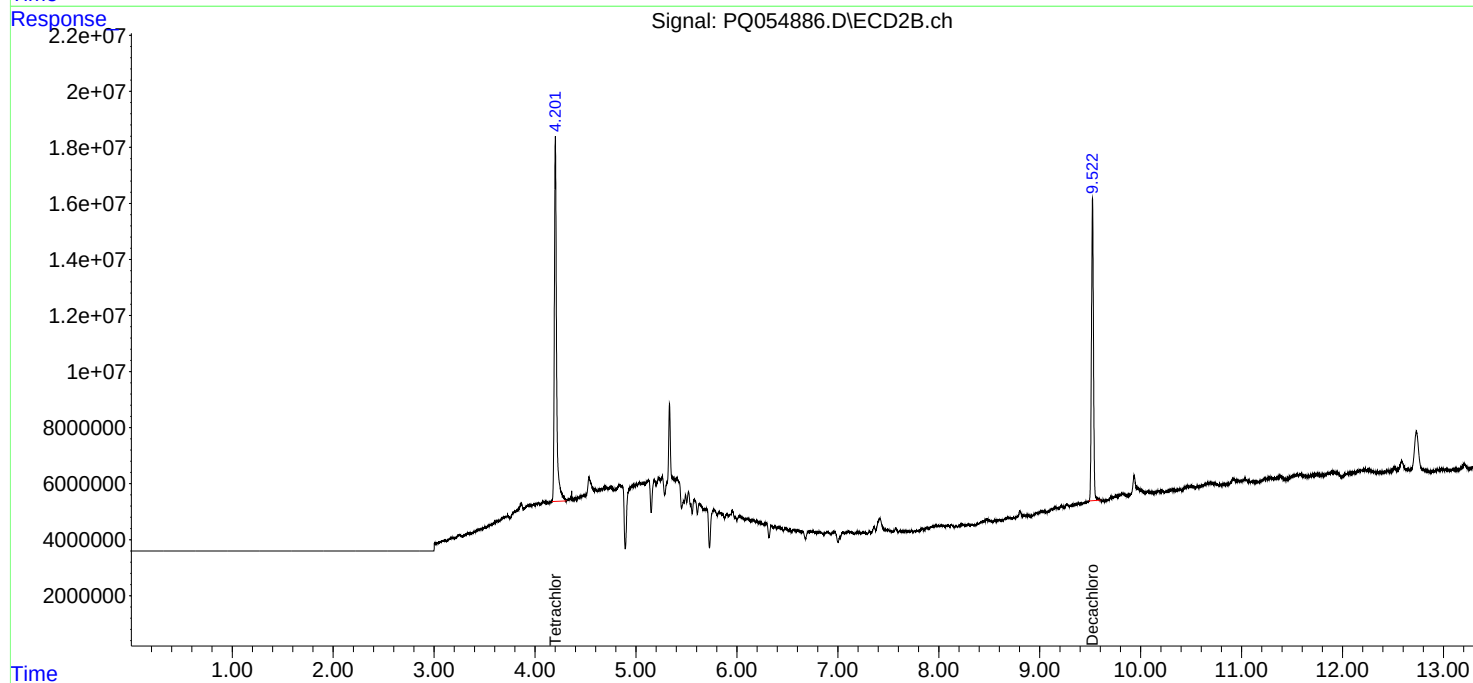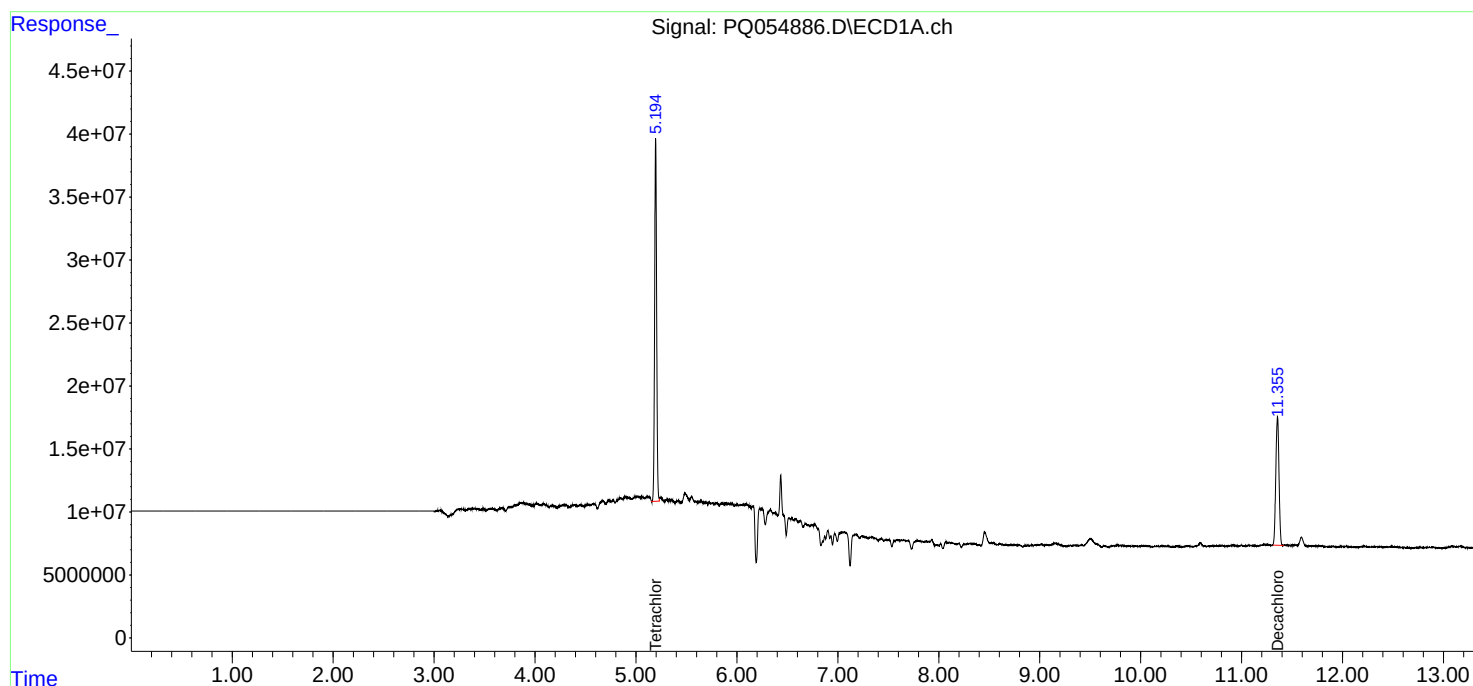


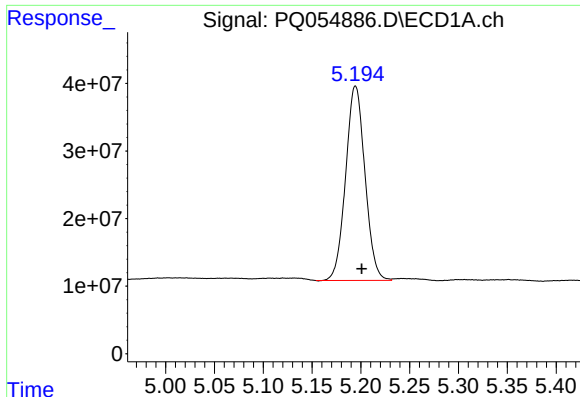

#1 Tetrachloro-m-xylene


R.T.: 5.194 min
Delta R.T.: -0.006 min
Response: 396251418
Conc: 16.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
20-SB-2-20211005-5.5-6.0-A

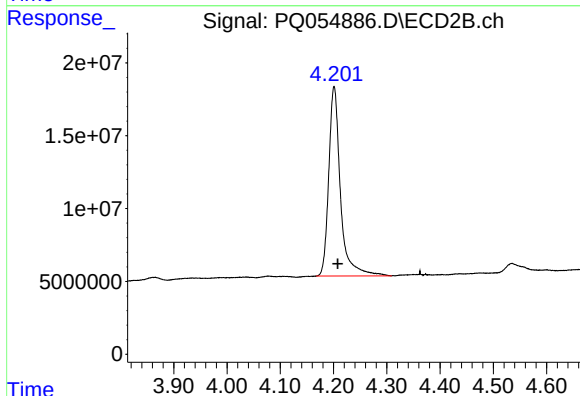


#1 Tetrachloro-m-xylene

R.T.: 4.201 min
Delta R.T.: -0.007 min
Response: 199060975
Conc: 15.06 ng/ml

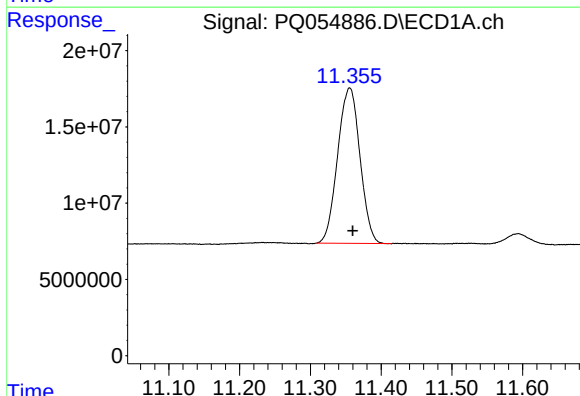

#2 Decachlorobiphenyl

R.T.: 11.355 min
Delta R.T.: -0.005 min
Response: 223512201
Conc: 13.24 ng/ml

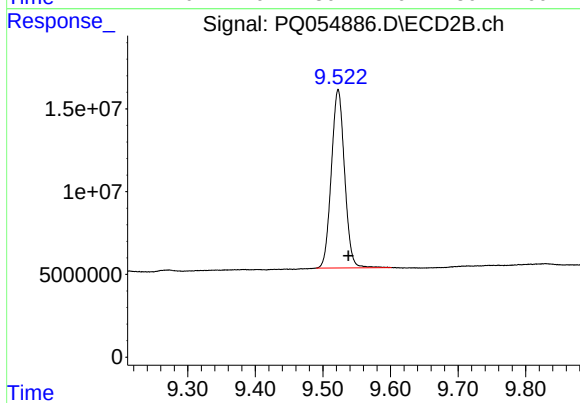

#2 Decachlorobiphenyl

R.T.: 9.523 min
Delta R.T.: -0.015 min
Response: 146500519
Conc: 10.81 ng/ml