

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100621\
 Data File : PQ054890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2021 06:10
 Operator : AJ\MA
 Sample : M4087-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MW-20-20211005-F2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 09:11:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 15 05:25:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.195	4.200	516.2E6	264.0E6	21.616	19.969
2) SA Decachlor...	11.354	9.523	346.9E6	244.3E6	20.554	18.027

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ100621\
Data File : PQ054890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2021 06:10
Operator : AJ\MA
Sample : M4087-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MW-20-20211005-F2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 09:11:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091421.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 15 05:25:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

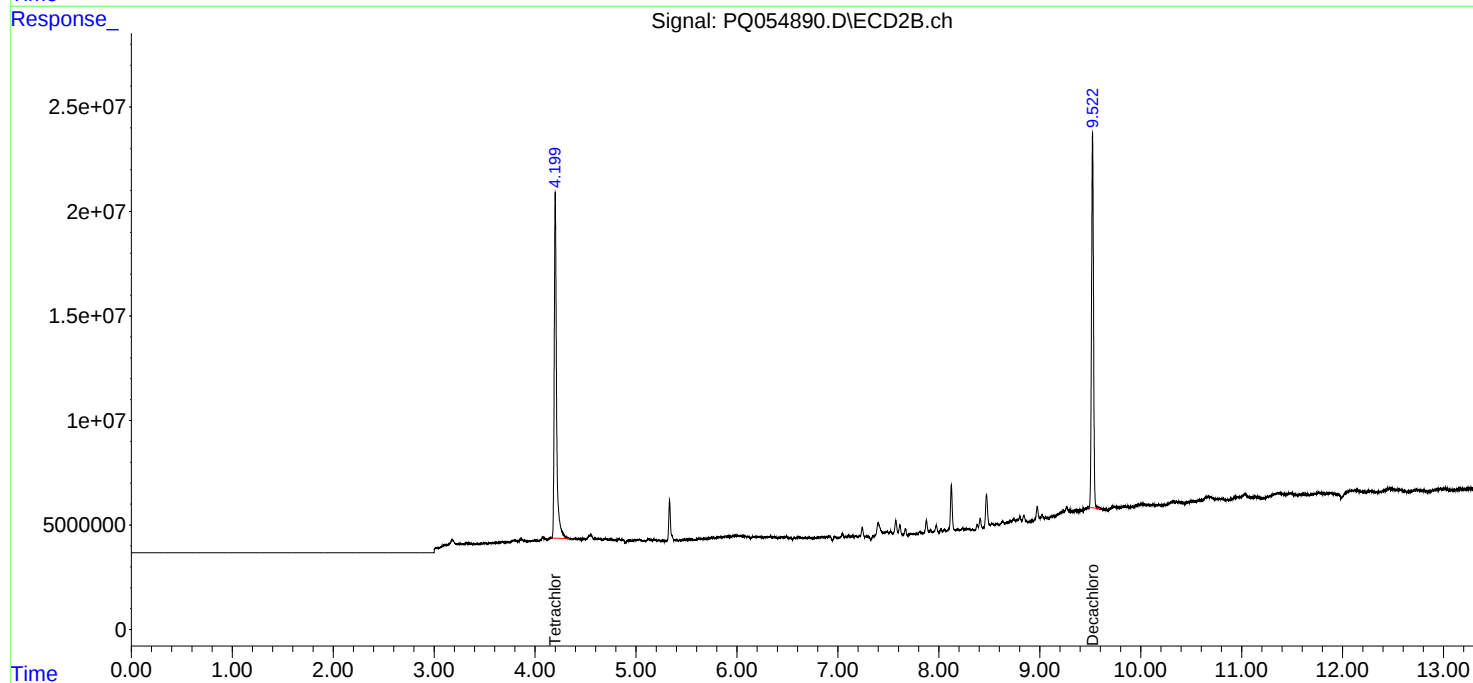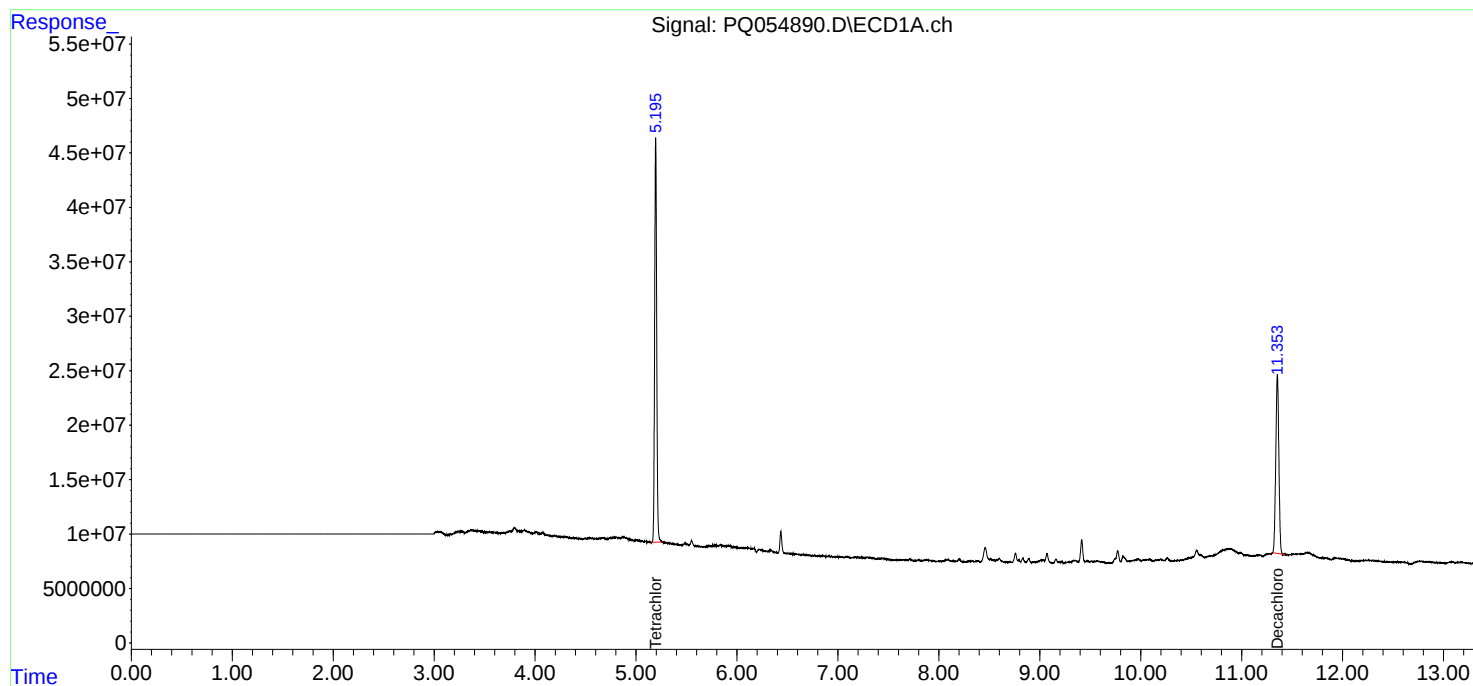


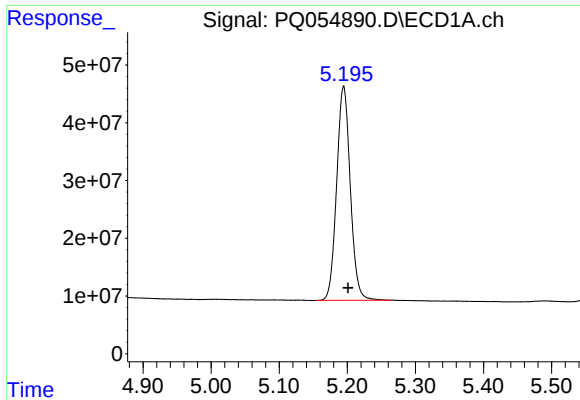

#1 Tetrachloro-m-xylene


R.T.: 5.195 min
Delta R.T.: -0.006 min
Response: 51622345
Conc: 21.62 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MW-20-20211005-F2

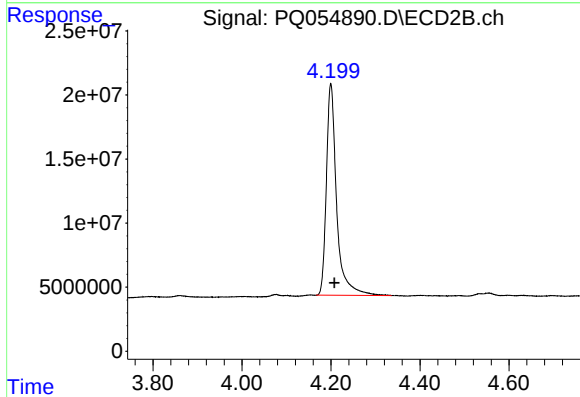


#1 Tetrachloro-m-xylene

R.T.: 4.200 min
Delta R.T.: -0.008 min
Response: 263984746
Conc: 19.97 ng/ml

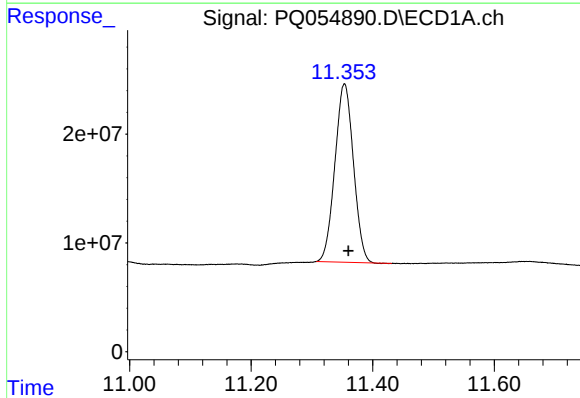

#2 Decachlorobiphenyl

R.T.: 11.354 min
Delta R.T.: -0.006 min
Response: 346912692
Conc: 20.55 ng/ml

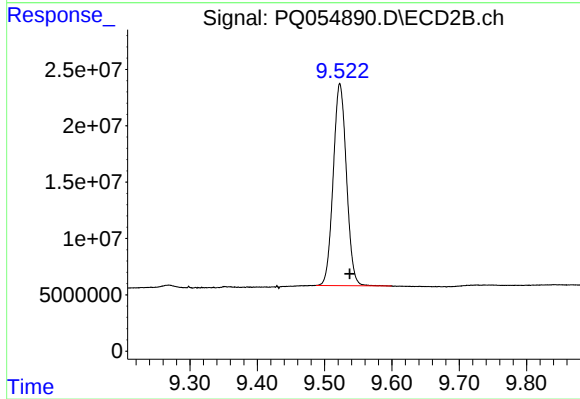

#2 Decachlorobiphenyl

R.T.: 9.523 min
Delta R.T.: -0.015 min
Response: 244304193
Conc: 18.03 ng/ml