

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101022\
 Data File : PS020761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2022 08:54
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 00:04:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.477f	0.000	511771	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.485	0.000	84836	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.805	0.000	1739885	0	<MDL	N.D. #
5) T	DICAMBA	6.508f	0.000	673091	0	<MDL	N.D. #
6) T	MCP	6.746	0.000	3581076	0	<MDL	N.D. #
8) T	DICHLORPROP	7.184	7.677	145748	628896	<MDL	<MDL #
10) T	Pentachlo...	7.648f	0.000	550113	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.152	0.000	457912	0	<MDL	N.D. #
12) T	2,4,5-T	8.384	9.170	966522	2132632	<MDL	<MDL #
13) T	2,4-DB	8.876	0.000	443855	0	<MDL	N.D. #
14) T	DINOSEB	9.967	0.000	362398	0	<MDL	N.D. #
15) T	Picloram	9.785	10.937	18029956	11154614	1.083	<MDL #
16) T	DCPA	10.227	10.937	1512375	11154614	<MDL	1.086 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101022\
Data File : PS020761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2022 08:54
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 00:04:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

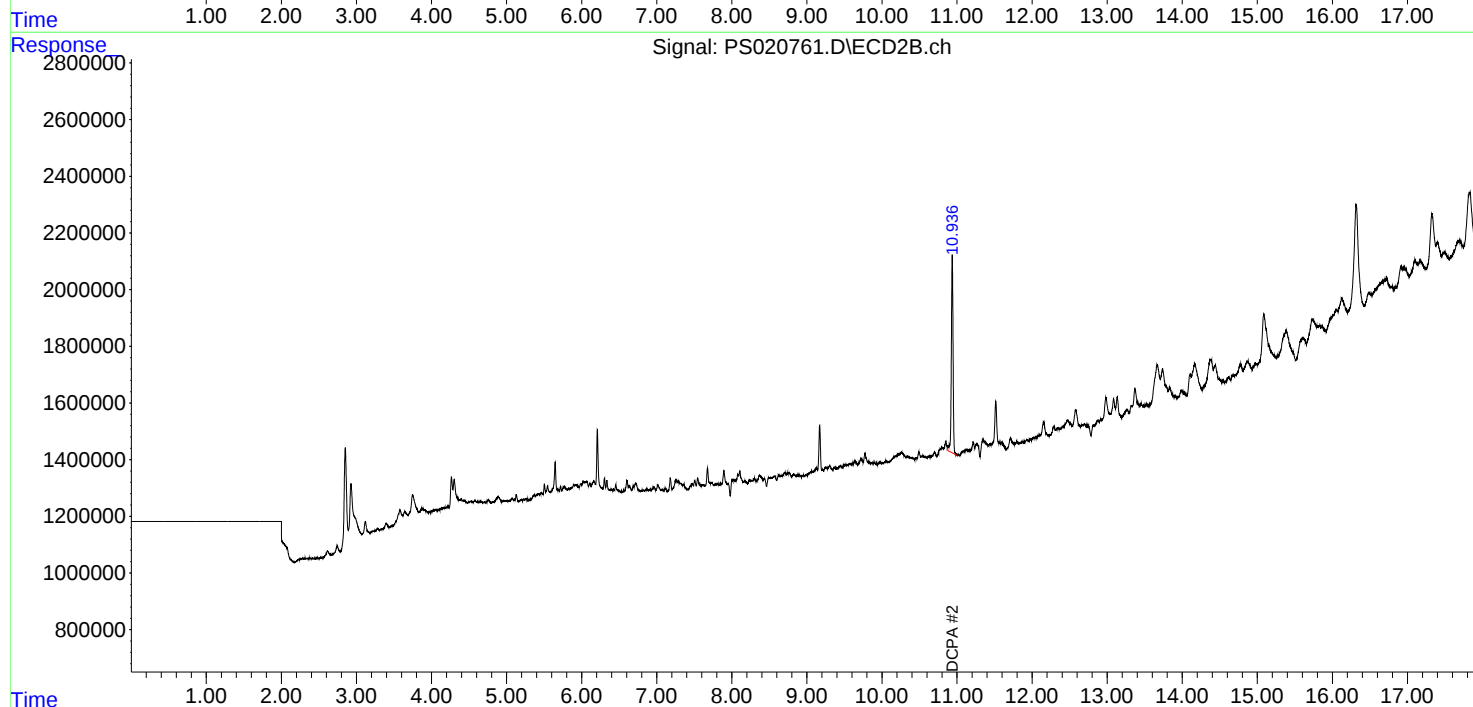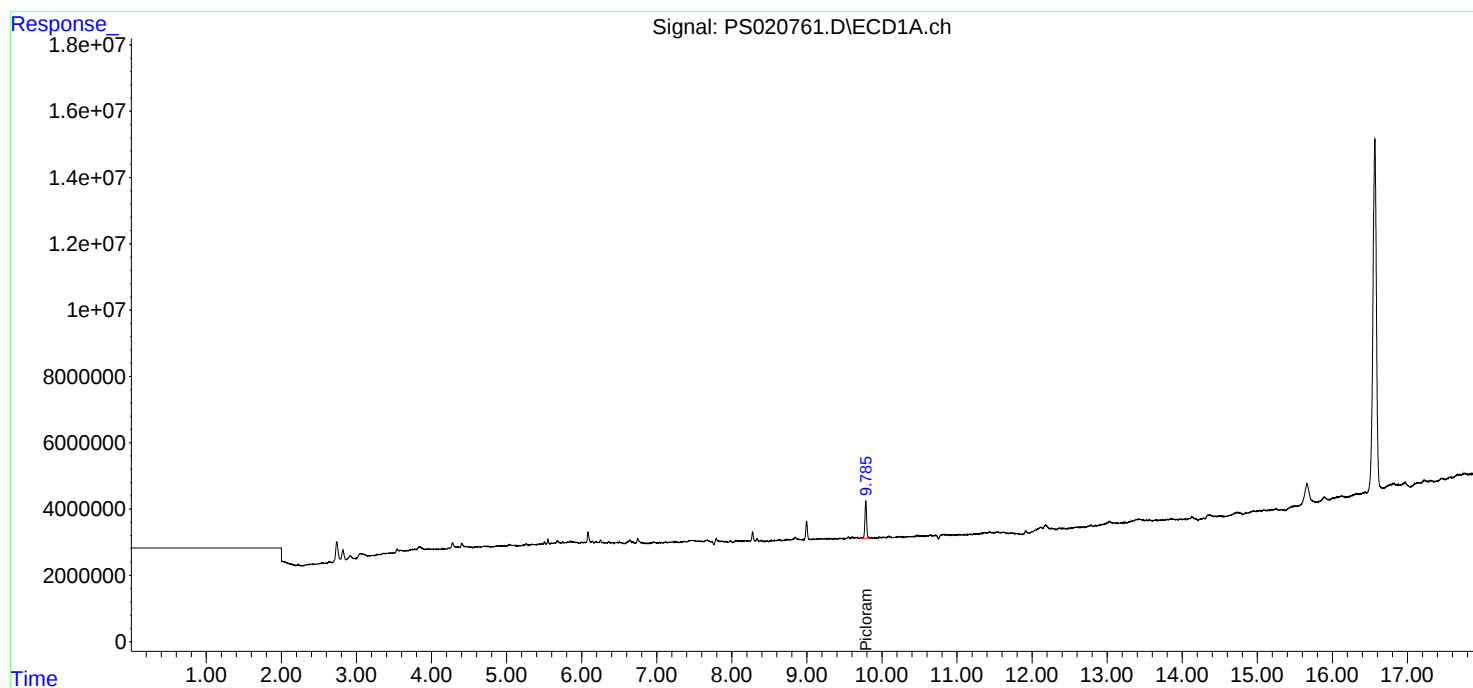


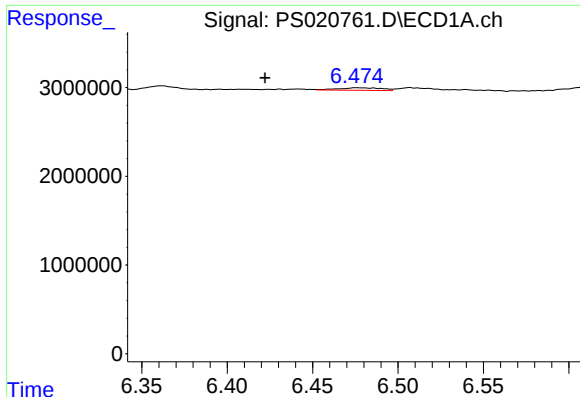

#4 2,4-DCAA


R.T.: 6.477 min
Delta R.T.: 0.055 min
Response: 511771
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

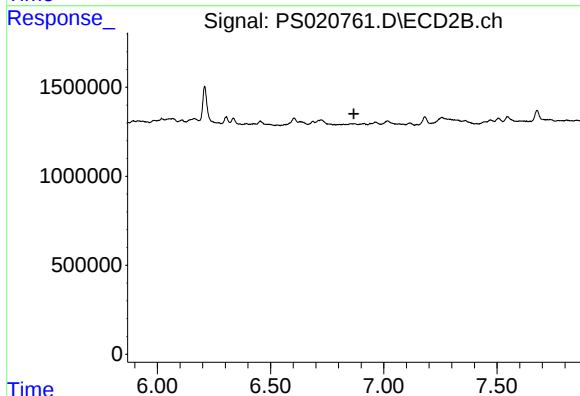


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.868 min
Response: 0
Conc: N.D.

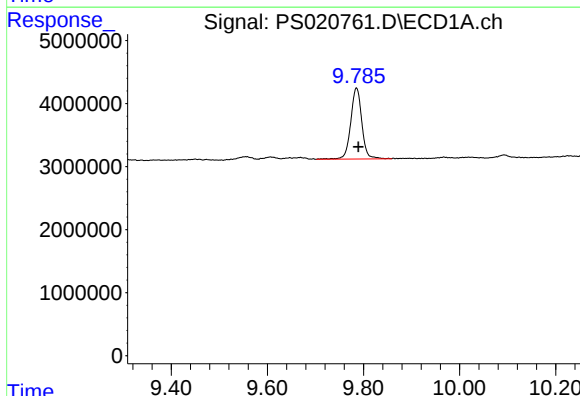


#15 Picloram

R.T.: 9.785 min
Delta R.T.: -0.004 min
Response: 18029956
Conc: 1.08 ng/ml

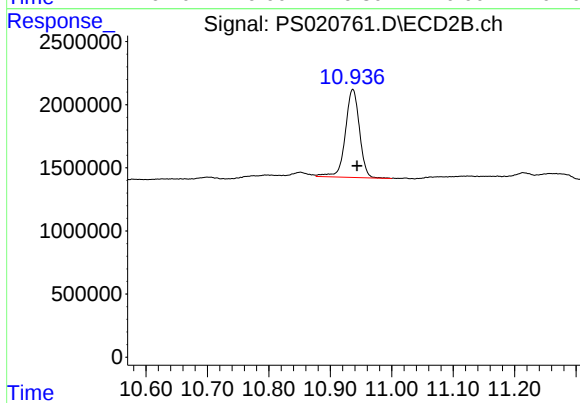

#15 Picloram


R.T.: 10.937 min
Delta R.T.: -0.007 min
Response: 11154614
Conc: N.D.

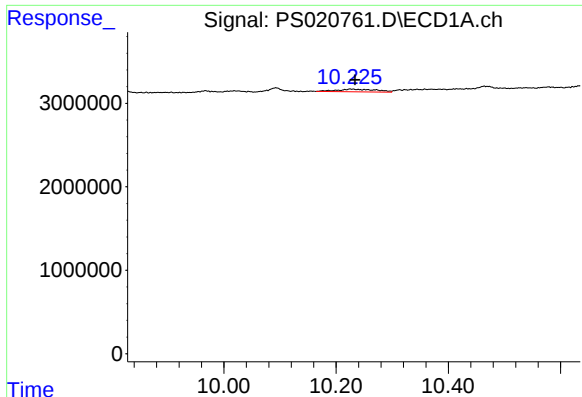

#16 DCPA

R.T.: 10.227 min
Delta R.T.: -0.007 min
Response: 1512375
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

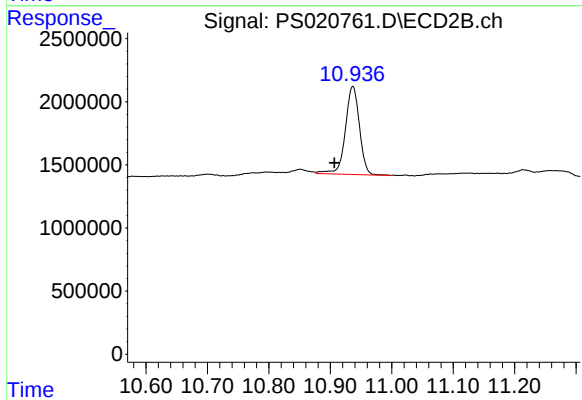

#16 DCPA

R.T.: 10.937 min
Delta R.T.: 0.030 min
Response: 11154614
Conc: 1.09 ng/ml