

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101022\
 Data File : PS020762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2022 09:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 00:05:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.418	6.862	936.6E6	641.7E6	496.479	479.262
Target Compounds							
1) T	Dalapon	2.503	0.000	283029	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.803	6.020	1459344	938367	<MDL	<MDL #
3) T	4-Nitroph...	6.256	6.454	7071653	774300	<MDL	<MDL #
5) T	DICAMBA	6.615f	0.000	2624454	0	<MDL	N.D. #
6) T	MCPD	6.749	0.000	5176108	0	<MDL	N.D. #
7) T	MCPA	6.788f	0.000	6402517	0	<MDL	N.D. #
8) T	DICHLORPROP	7.185	7.676	161140	1115400	<MDL	<MDL #
9) T	2,4-D	7.373	8.001f	732662	302324	<MDL	<MDL #
10) T	Pentachlo...	7.650f	0.000	2466856	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.114	0.000	1252203	0	<MDL	N.D. #
12) T	2,4,5-T	8.395	9.169	293588	1865074	<MDL	<MDL #
13) T	2,4-DB	8.846f	0.000	2377429	0	1.041	N.D. #
14) T	DINOSEB	9.965	0.000	765782	0	<MDL	N.D. #
15) T	Picloram	9.784	10.936	14546146	9535178	<MDL	<MDL #
16) T	DCPA	10.229	10.936	615718	9535178	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101022\
Data File : PS020762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2022 09:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 00:05:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

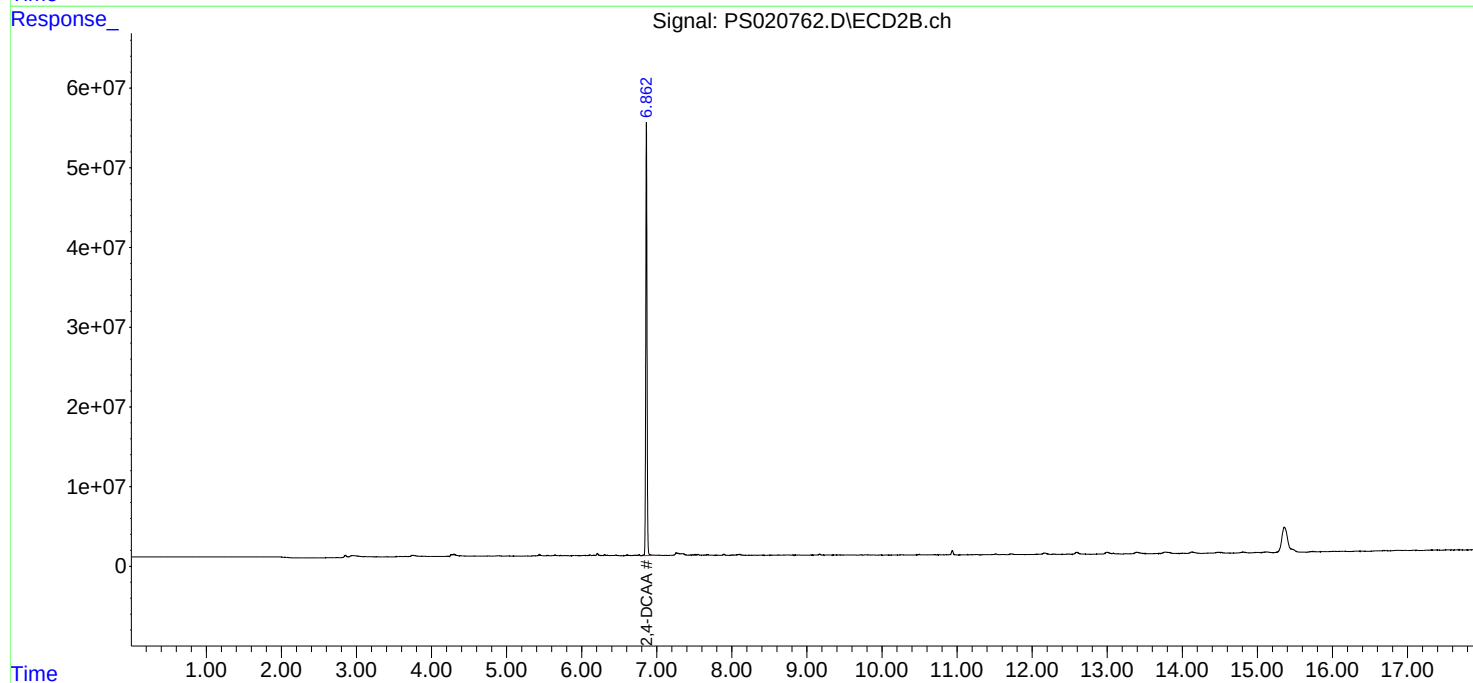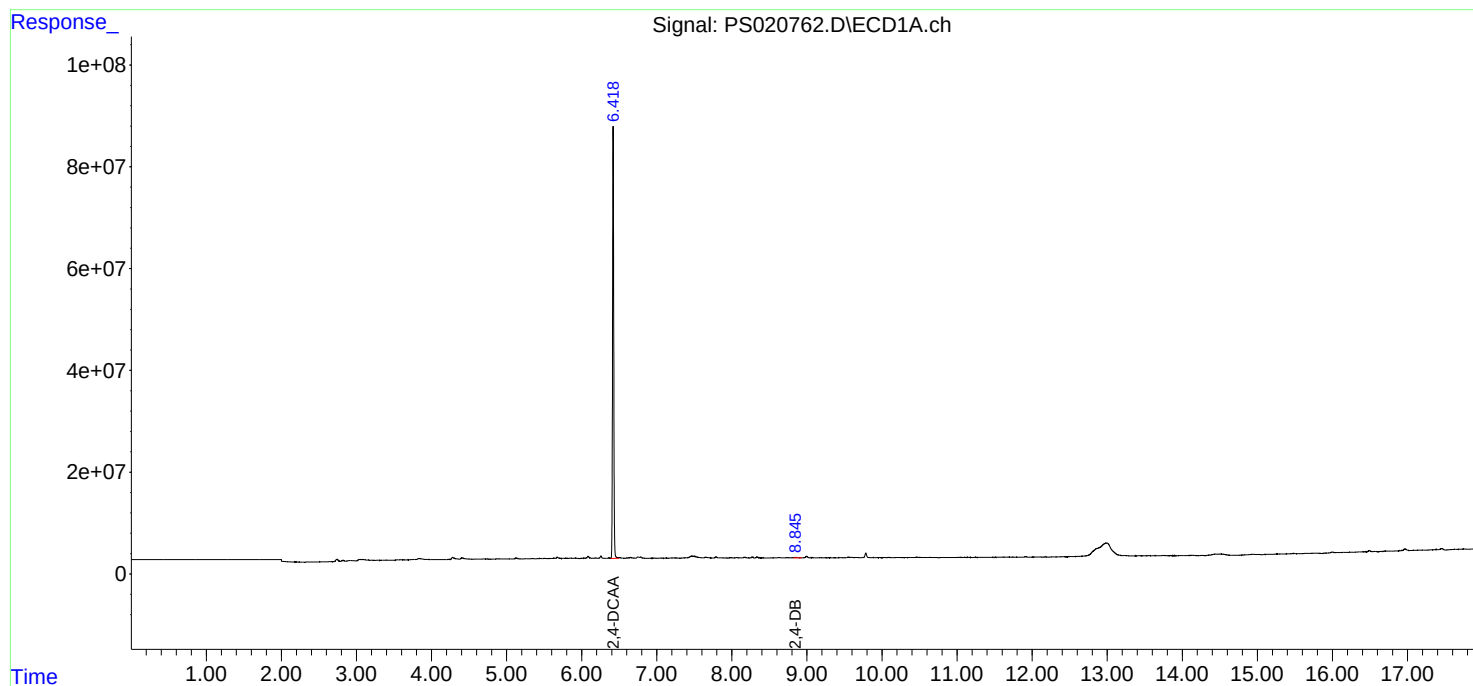


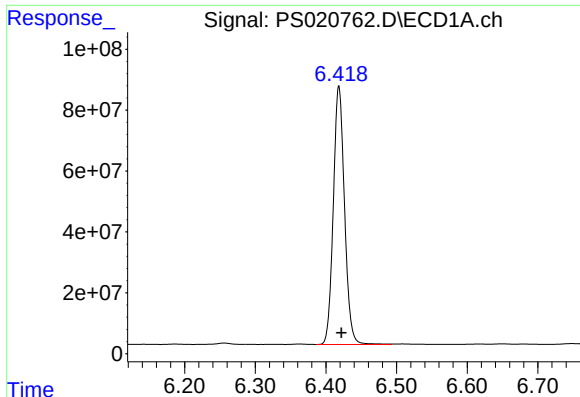

#4 2,4-DCAA


R.T.: 6.418 min
Delta R.T.: -0.004 min
Response: 936582086
Conc: 496.48 ng/ml

Instrument :
ECD_Q
ClientSampleId :

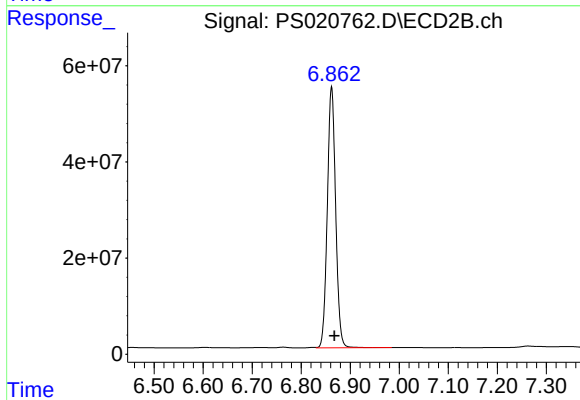


#4 2,4-DCAA

R.T.: 6.862 min
Delta R.T.: -0.006 min
Response: 641722969
Conc: 479.26 ng/ml

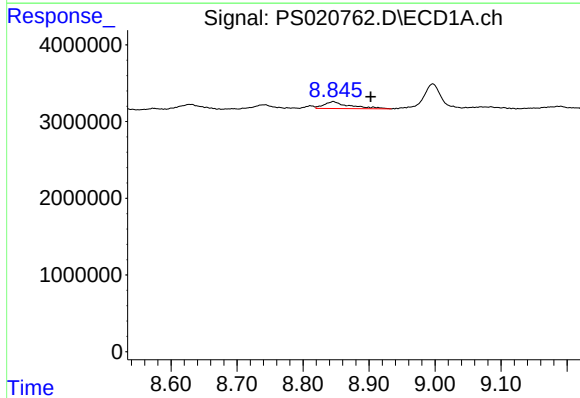

#13 2,4-DB

R.T.: 8.846 min
Delta R.T.: -0.057 min
Response: 2377429
Conc: 1.04 ng/ml

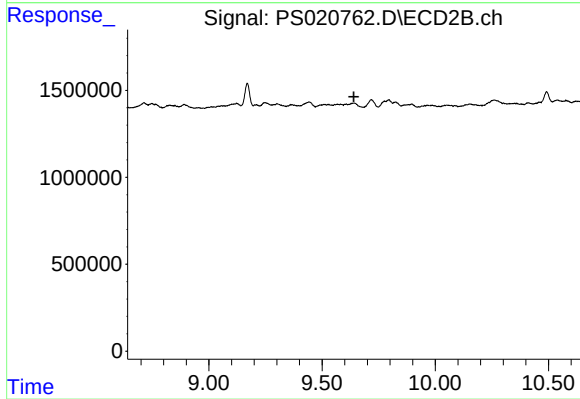

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.641 min
Response: 0
Conc: N.D.