

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101022\
 Data File : PS020768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2022 13:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 00:07:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.420	6.863	937.8E6	649.6E6	497.150	485.145
Target Compounds							
1) T	Dalapon	2.496	0.000	235366	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.744f	0.000	3089545	0	1.028	N.D. #
5) T	DICAMBA	6.568	0.000	354818	0	<MDL	N.D. #
6) T	MCP	6.747	0.000	4549957	0	<MDL	N.D. #
7) T	MCPA	6.789f	0.000	3985739	0	<MDL	N.D. #
8) T	DICHLORPROP	7.216f	7.677	510422	1555903	<MDL	1.073 #
11) T	2,4,5-TP ...	8.131	0.000	2336245	0	<MDL	N.D. #
12) T	2,4,5-T	8.389	9.170	2121846	1953275	<MDL	<MDL #
13) T	2,4-DB	8.846f	0.000	1820708	0	<MDL	N.D. #
14) T	DINOSEB	9.965	0.000	1302910	0	<MDL	N.D. #
15) T	Picloram	9.785	10.936	9538300	5768031	<MDL	<MDL #
16) T	DCPA	10.250	10.936	2994679	5768031	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101022\
Data File : PS020768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2022 13:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 00:07:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

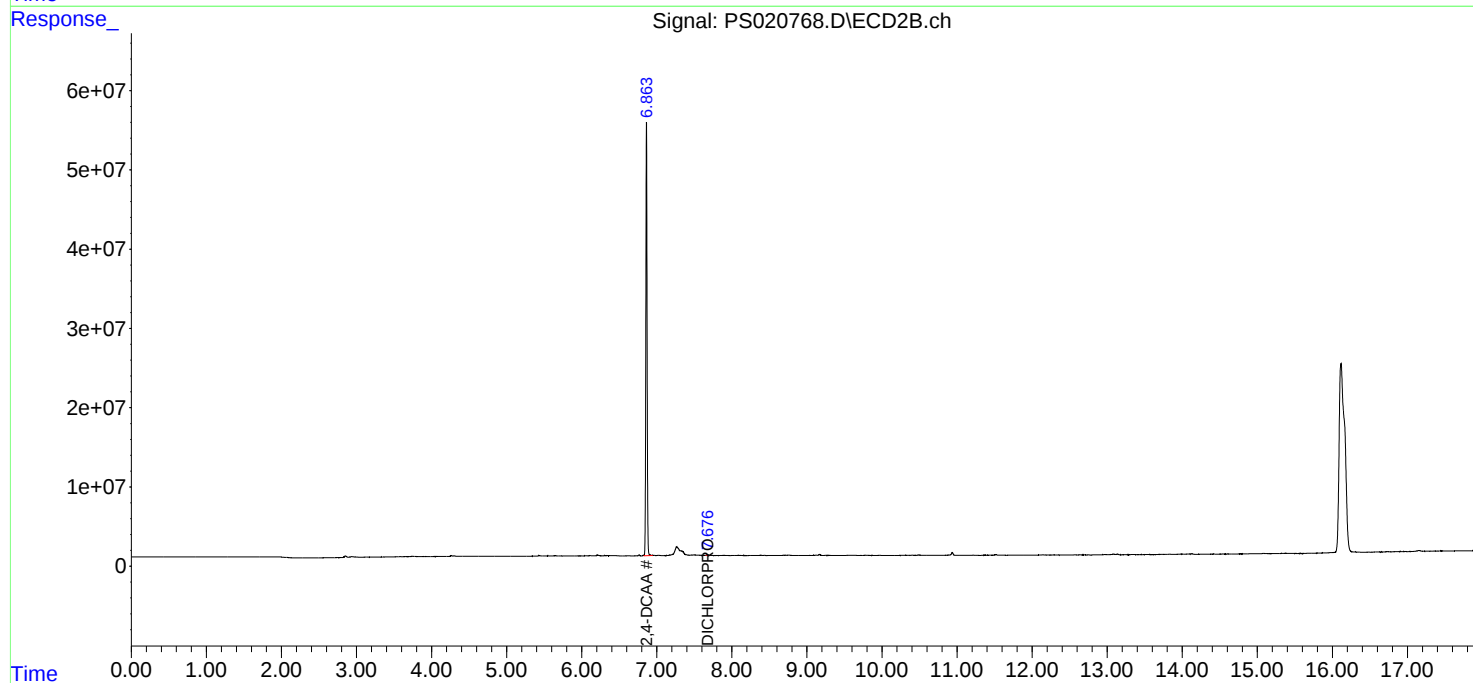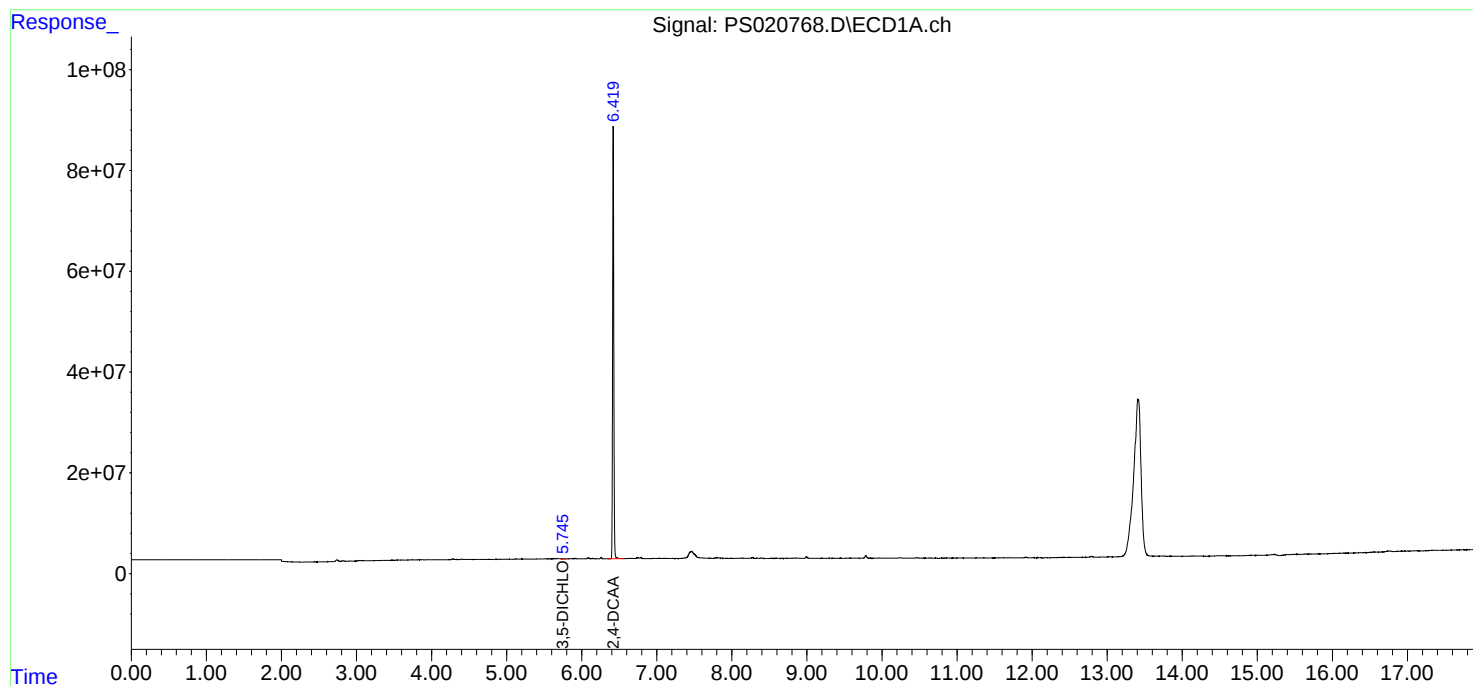


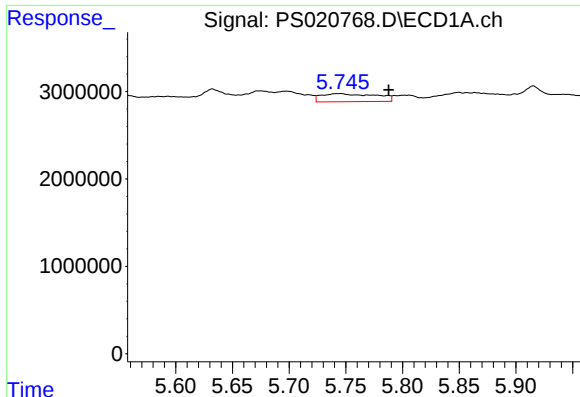

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.744 min
Delta R.T.: -0.044 min
Response: 3089545
Conc: 1.03 ng/ml

Instrument :
ECD_Q
ClientSampleId :

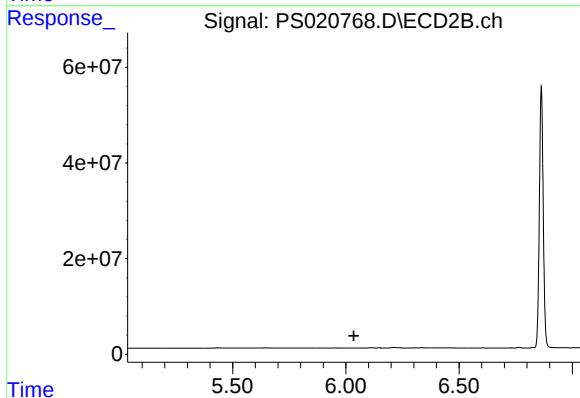


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

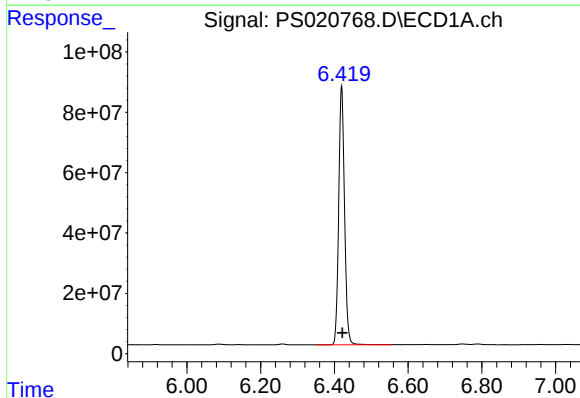


#4 2,4-DCAA

R.T.: 6.420 min
Delta R.T.: -0.003 min
Response: 937848920
Conc: 497.15 ng/ml

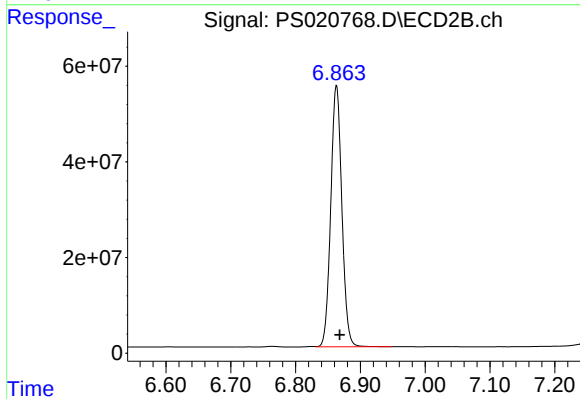

#4 2,4-DCAA


R.T.: 6.863 min
Delta R.T.: -0.005 min
Response: 649599244
Conc: 485.14 ng/ml

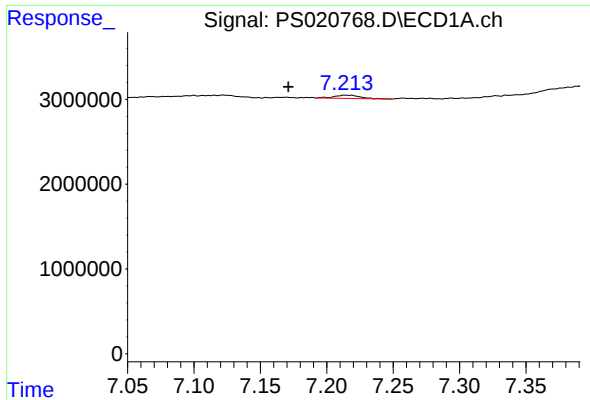

#8 DICHLORPROP

R.T.: 7.216 min
Delta R.T.: 0.045 min
Response: 510422
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

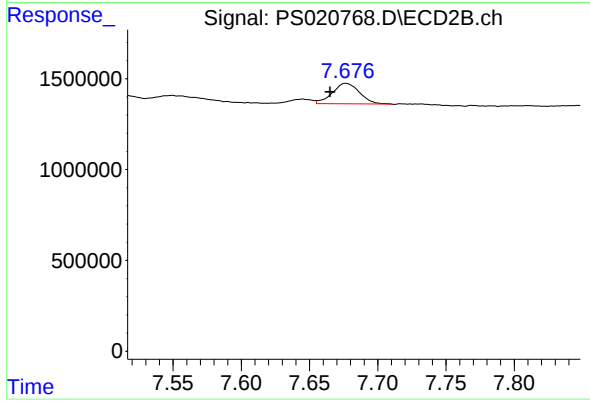

#8 DICHLORPROP

R.T.: 7.677 min
Delta R.T.: 0.012 min
Response: 1555903
Conc: 1.07 ng/ml