

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101119\
 Data File : PQ044289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2019 14:02
 Operator : HP\AJ
 Sample : K5343-06 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 C0AY6

Manual Integrations
 APPROVED

Ankita
 10/14/2019 3:06:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 01:27:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100819CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 10 02:55:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	5.326	4.357	10826846	11623210	2.785	2.604
2) SA Decachlor...	11.614	9.802	48133151	44697606	8.984	7.473m

Target Compounds

26) L6 AR-1254-1	7.565	6.523	8195.8E6	12152.0E6	60909.202	41663.892 #
27) L6 AR-1254-2	7.795	6.681	12352.1E6	15910.2E6	57821.355	60935.536
28) L6 AR-1254-3	8.180	7.110	16367.6E6	27618.8E6	66521.819	63214.260
29) L6 AR-1254-4	8.478	7.349	14884.5E6	20456.8E6	74214.890	76153.473
30) L6 AR-1254-5	8.912	7.784	17708.0E6	30163.2E6	73985.352	75433.785

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101119\
Data File : PQ044289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 14:02
Operator : HP\AJ
Sample : K5343-06 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
C0AY6

Manual Integrations
APPROVED

Ankita
10/14/2019 3:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 02:55:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

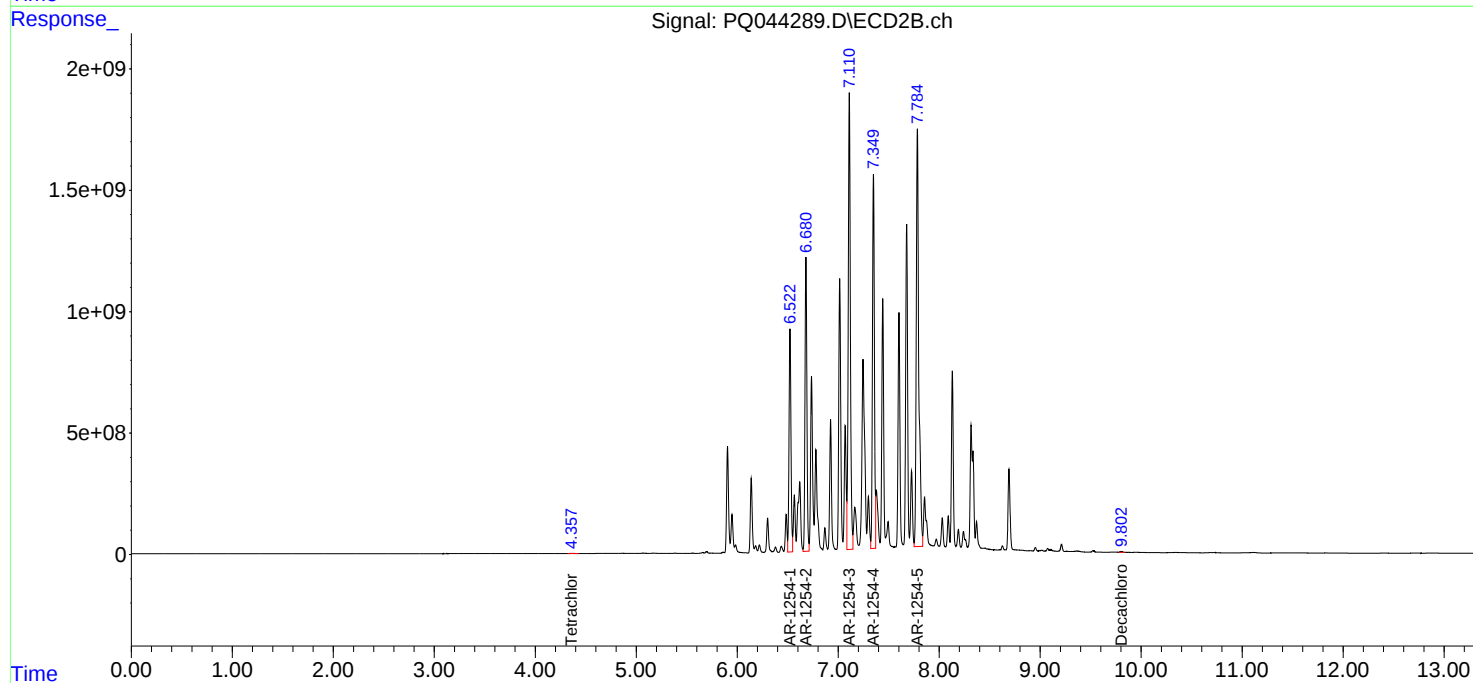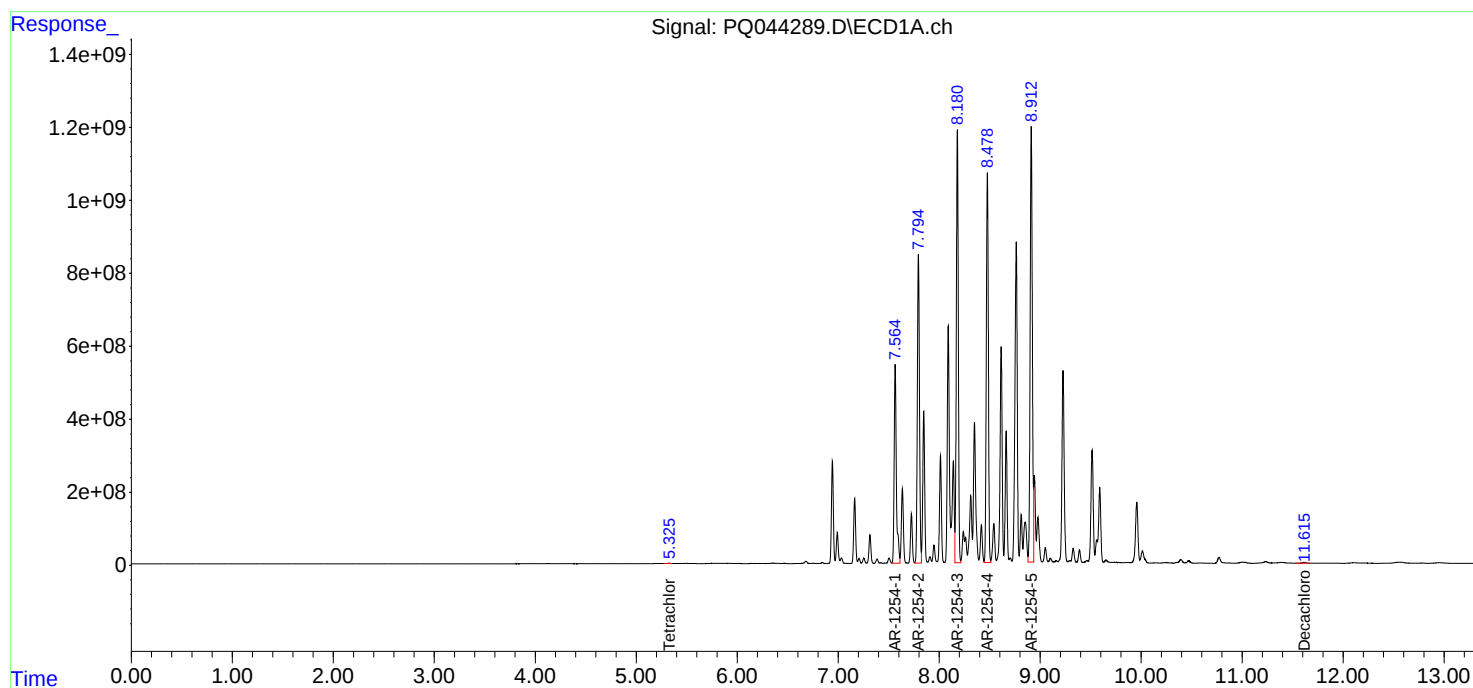

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101119\
Data File : PQ044289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 14:02
Operator : HP\AJ
Sample : K5343-06 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0AY6

Manual Integrations
APPROVED

Ankita
10/14/2019 3:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 02:55:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

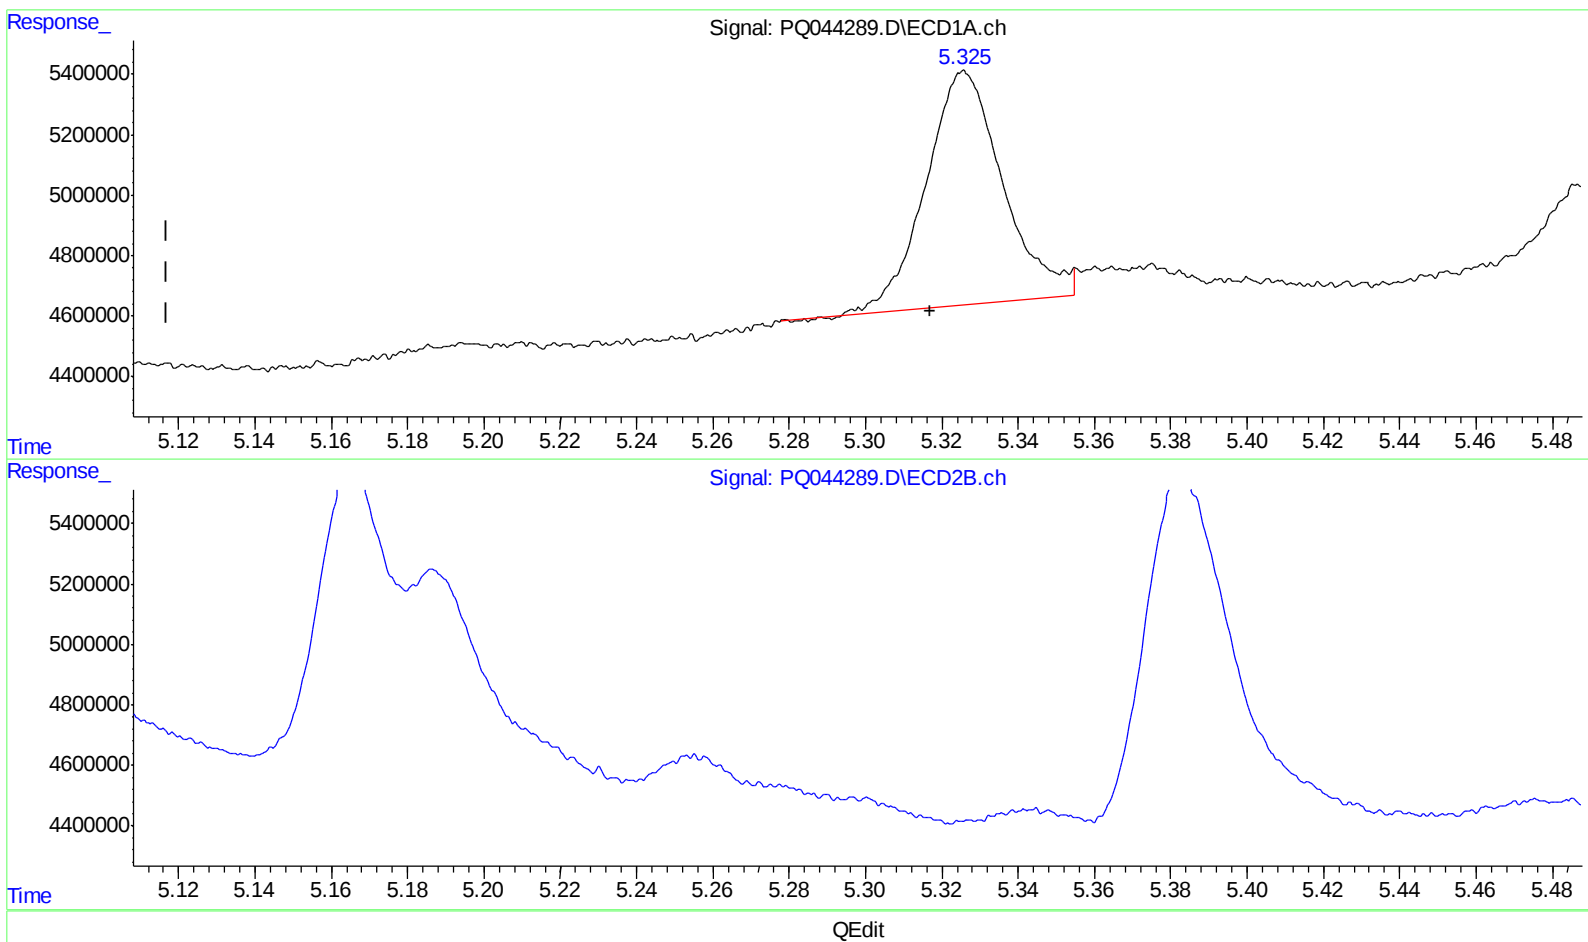

(1) Tetrachloro-m-xylene (SA)

5.326min 2.785 ng/ml

response 10826846

(1) Tetrachloro-m-xylene #2 (SA)

4.357min 2.604 ng/ml

response 11623210

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101119\
Data File : PQ044289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 14:02
Operator : HP\AJ
Sample : K5343-06 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0AY6

Manual Integrations
APPROVED

Ankita
10/14/2019 3:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 02:55:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

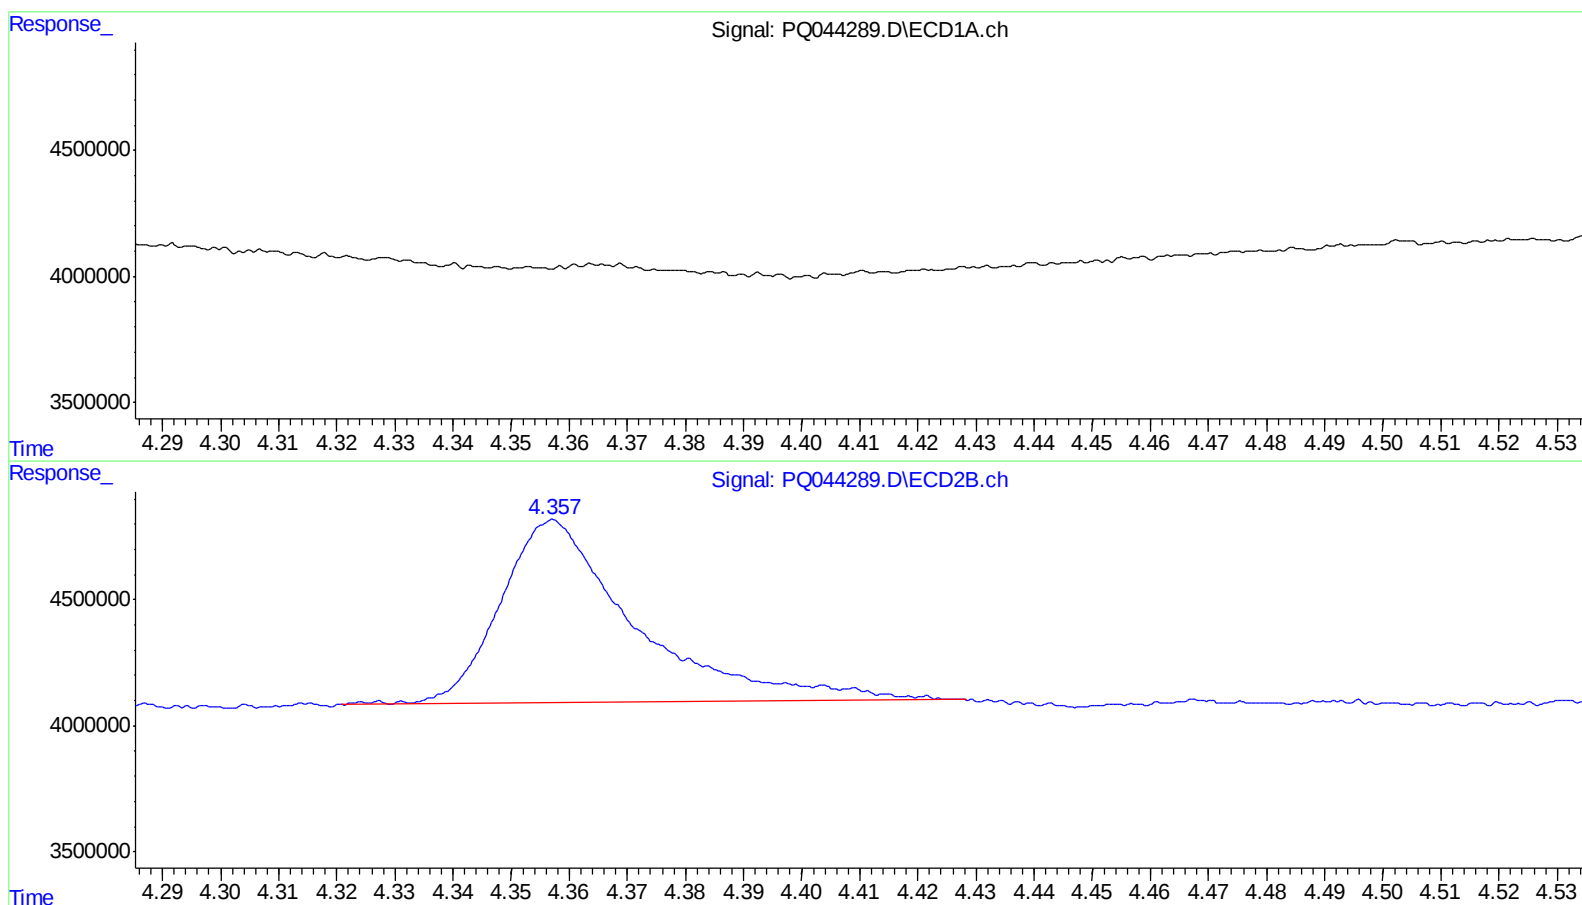

QEdit

(1) Tetrachloro-m-xylene (SA)

5.326min 2.785 ng/ml

response 10826846

(1) Tetrachloro-m-xylene #2 (SA)

4.357min 2.604 ng/ml

response 11623210

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101119\
Data File : PQ044289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 14:02
Operator : HP\AJ
Sample : K5343-06 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0AY6

Manual Integrations
APPROVED

Ankita
10/14/2019 3:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 02:55:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

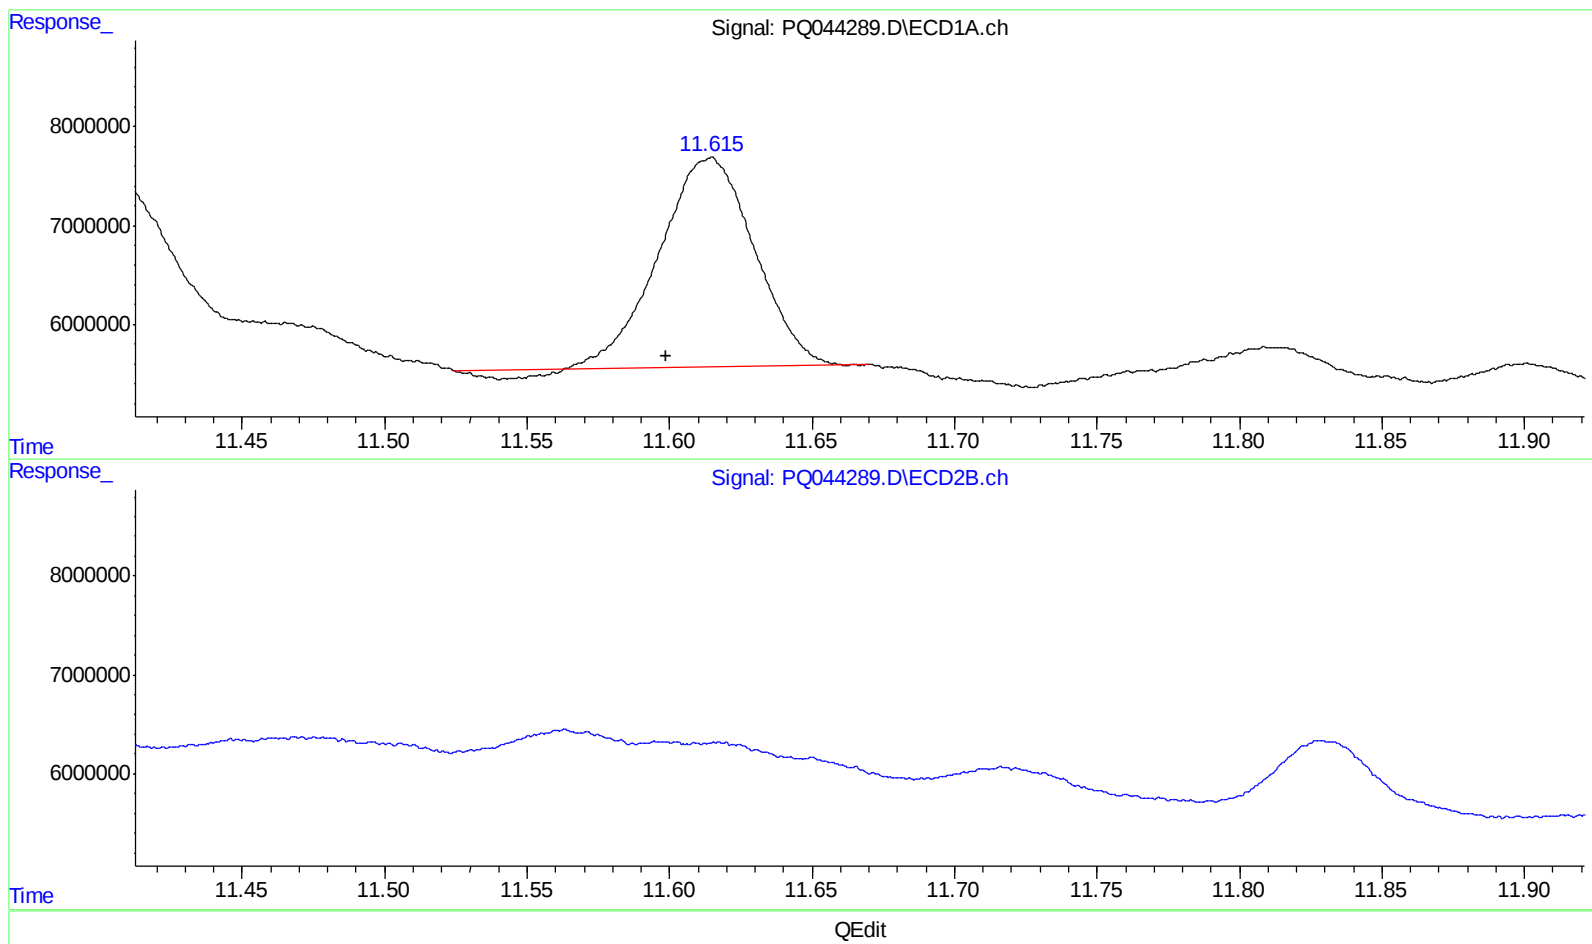

(2) Decachlorobiphenyl (SA)

11.614min 8.984 ng/ml

response 48133151

(2) Decachlorobiphenyl #2 (SA)

9.802min 7.473 ng/ml m

response 44697606

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101119\
Data File : PQ044289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2019 14:02
Operator : HP\AJ
Sample : K5343-06 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0AY6

Manual Integrations
APPROVED

Ankita
10/14/2019 3:06:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 02:55:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

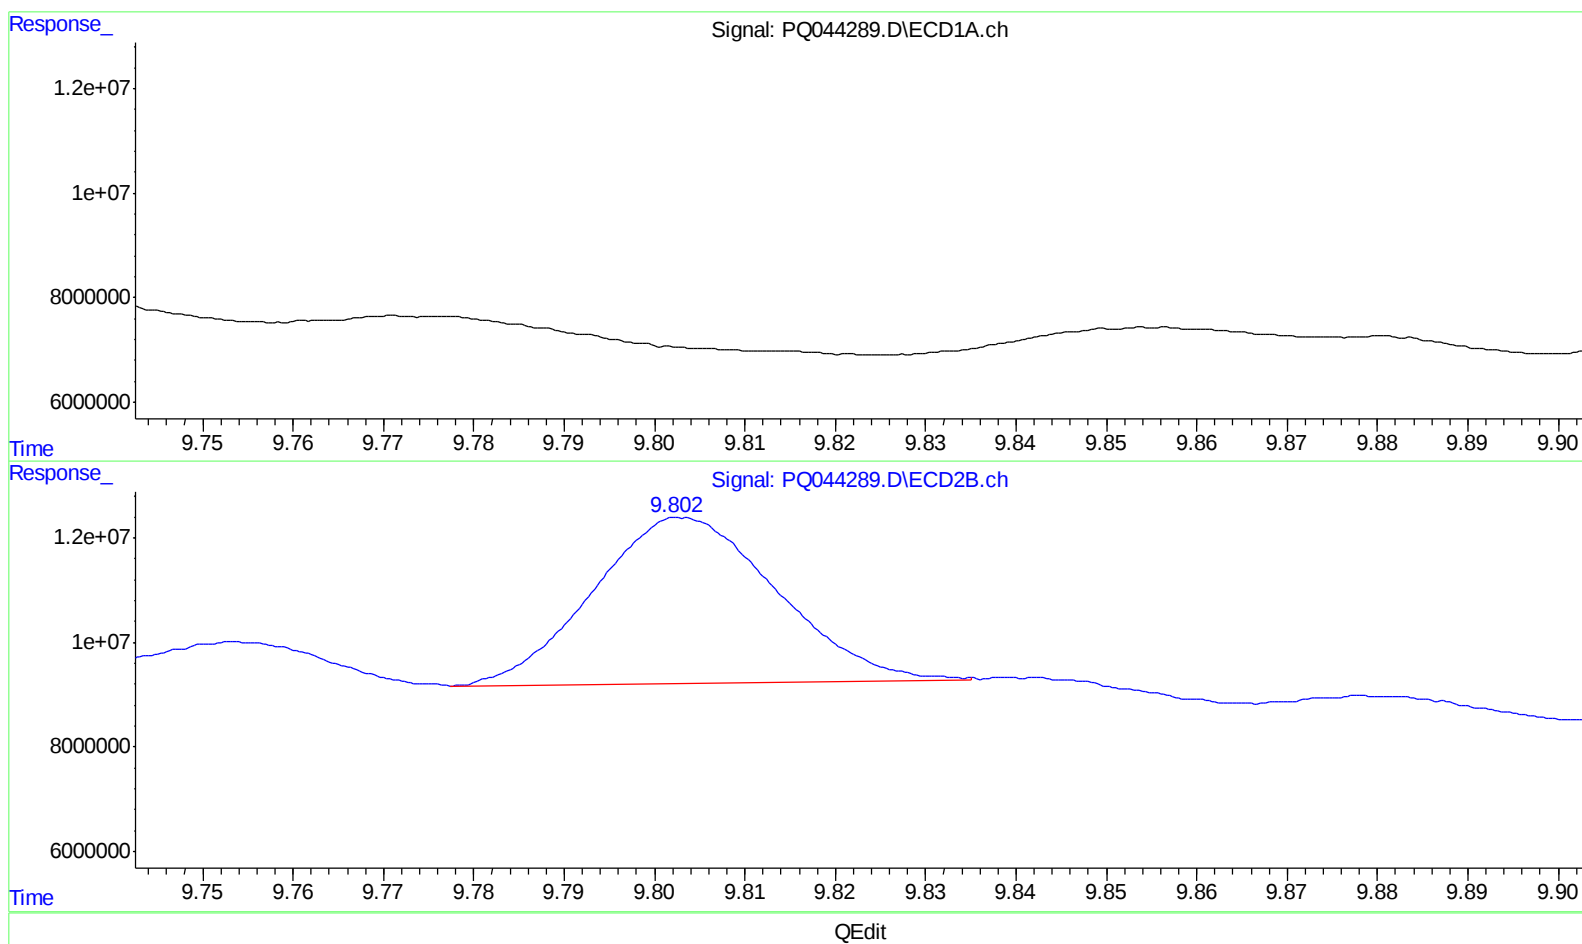

(2) Decachlorobiphenyl (SA)

11.614min 8.984 ng/ml

response 48133151

(2) Decachlorobiphenyl #2 (SA)

9.802min 7.473 ng/ml m

response 44697606