

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101918\
 Data File : PQ033316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 14:04
 Operator : SM\SJ
 Sample : J5541-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 101518-SIDI-E-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:19:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ101918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 20 01:08:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.570	3.849	43625643	30110436	16.901	17.015
2)	SA Decachlor...	10.399	8.897	38064753	31874116	18.553	19.260

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ101918\
Data File : PQ033316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 14:04
Operator : SM\SJ
Sample : J5541-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
101518-SIDI-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:19:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ101918.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 20 01:08:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

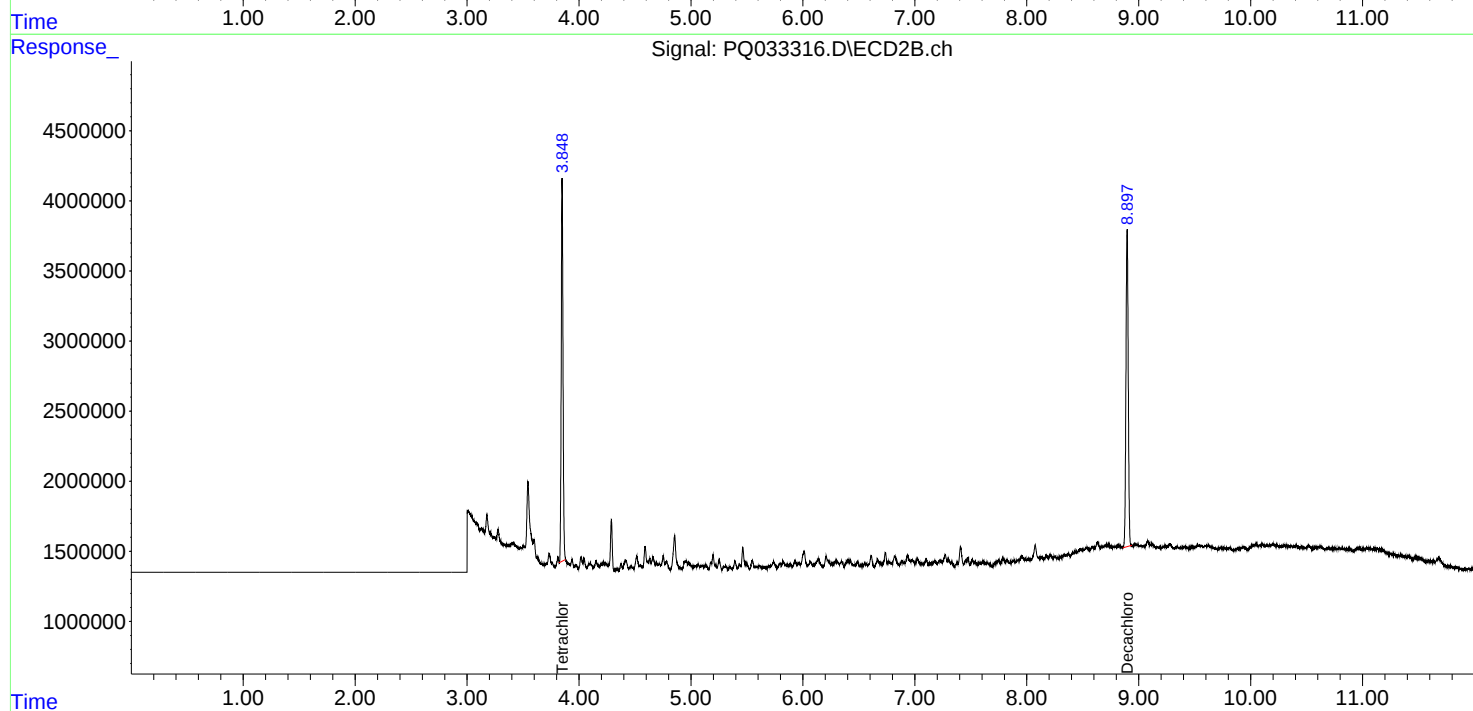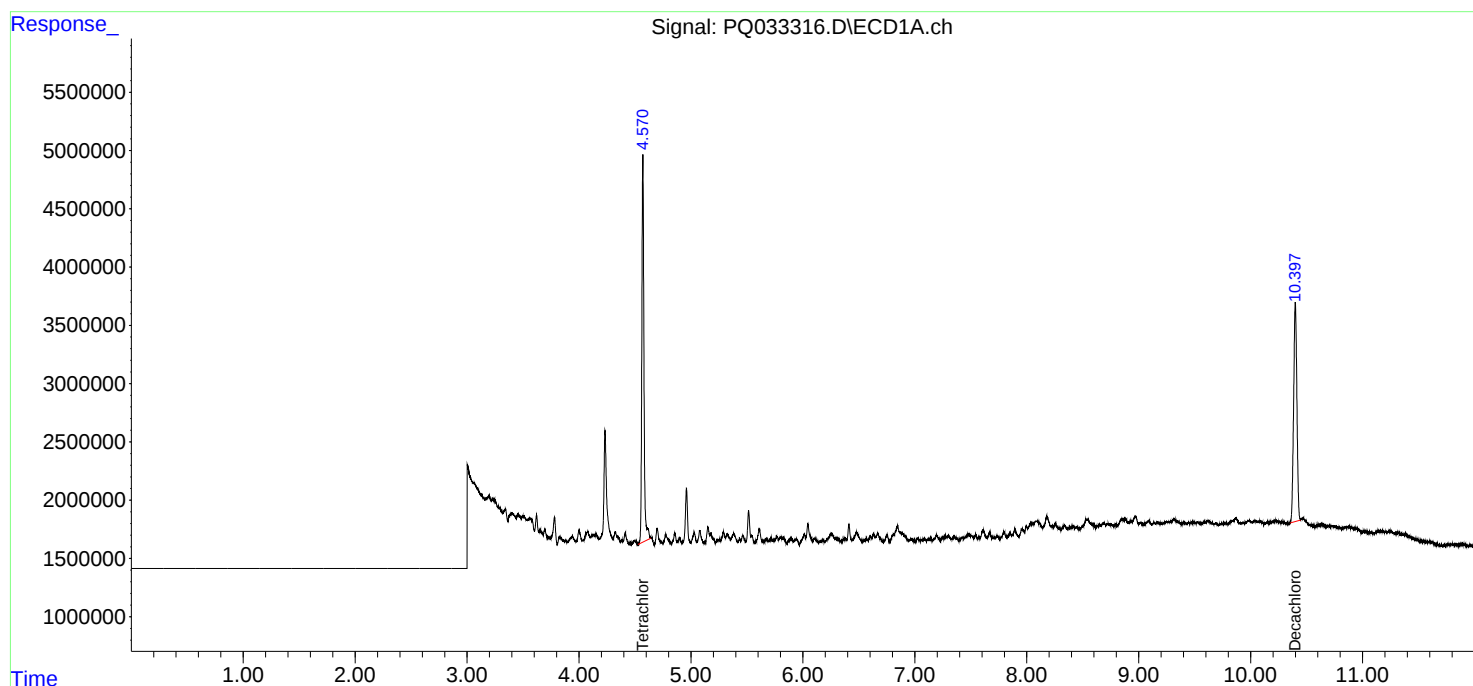


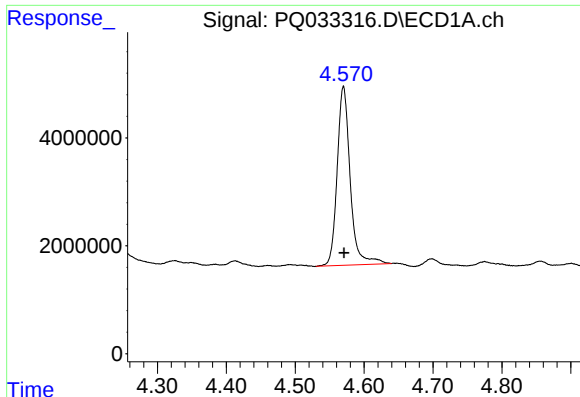

#1 Tetrachloro-m-xylene


R.T.: 4.570 min
Delta R.T.: 0.000 min
Response: 43625643
Conc: 16.90 ng/ml

Instrument :
ECD_Q
ClientSampleId :
101518-SIDI-E-D-S

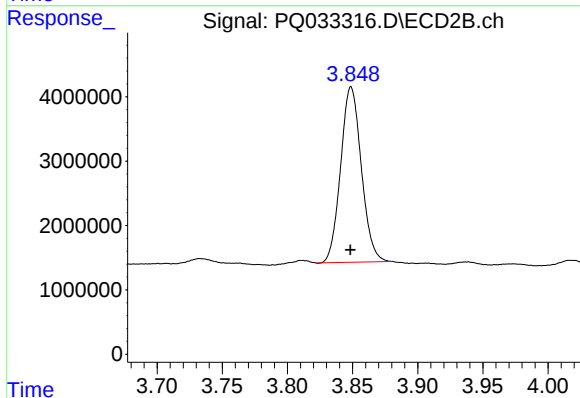


#1 Tetrachloro-m-xylene

R.T.: 3.849 min
Delta R.T.: 0.000 min
Response: 30110436
Conc: 17.02 ng/ml

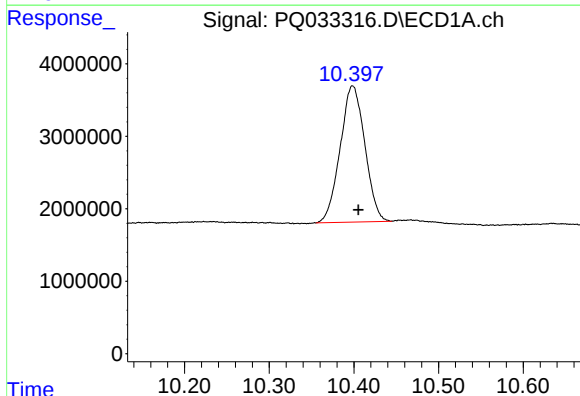

#2 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.007 min
Response: 38064753
Conc: 18.55 ng/ml

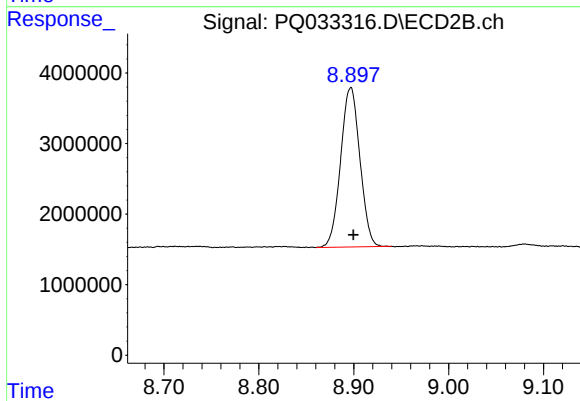

#2 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: -0.003 min
Response: 31874116
Conc: 19.26 ng/ml