

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102225\
 Data File : PQ071075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2025 16:39
 Operator : YP\AJ
 Sample : Q3407-24 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 L46-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2025
 Supervised By :mohammad ahmed 10/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 13:38:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ101025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 11 01:55:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.399	2.776	9638056	9710009	2.216	1.911
2) SA Decachlor...	8.498	7.533	6730040	8245257	2.318m	1.633 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102225\
Data File : PQ071075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2025 16:39
Operator : YP\AJ
Sample : Q3407-24 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
L46-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2025
Supervised By :mohammad ahmed 10/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 13:38:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ101025.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 11 01:55:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

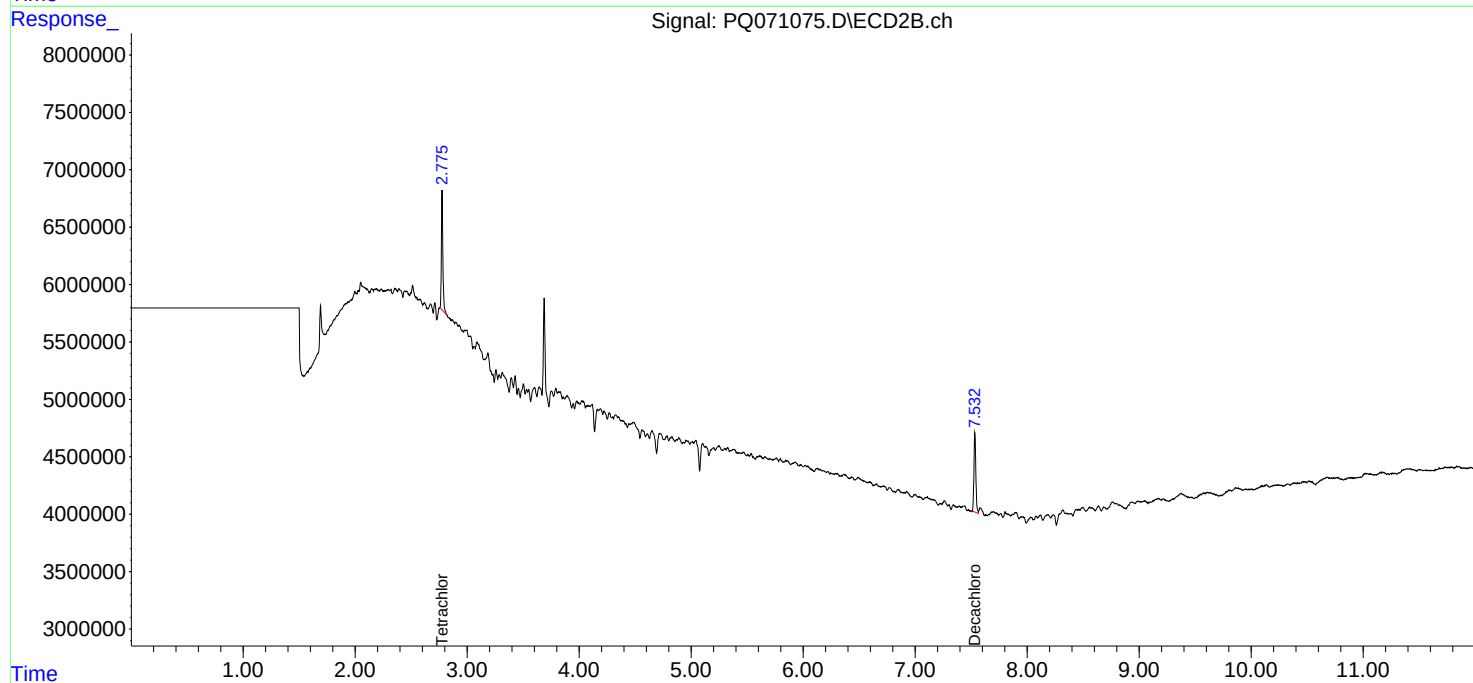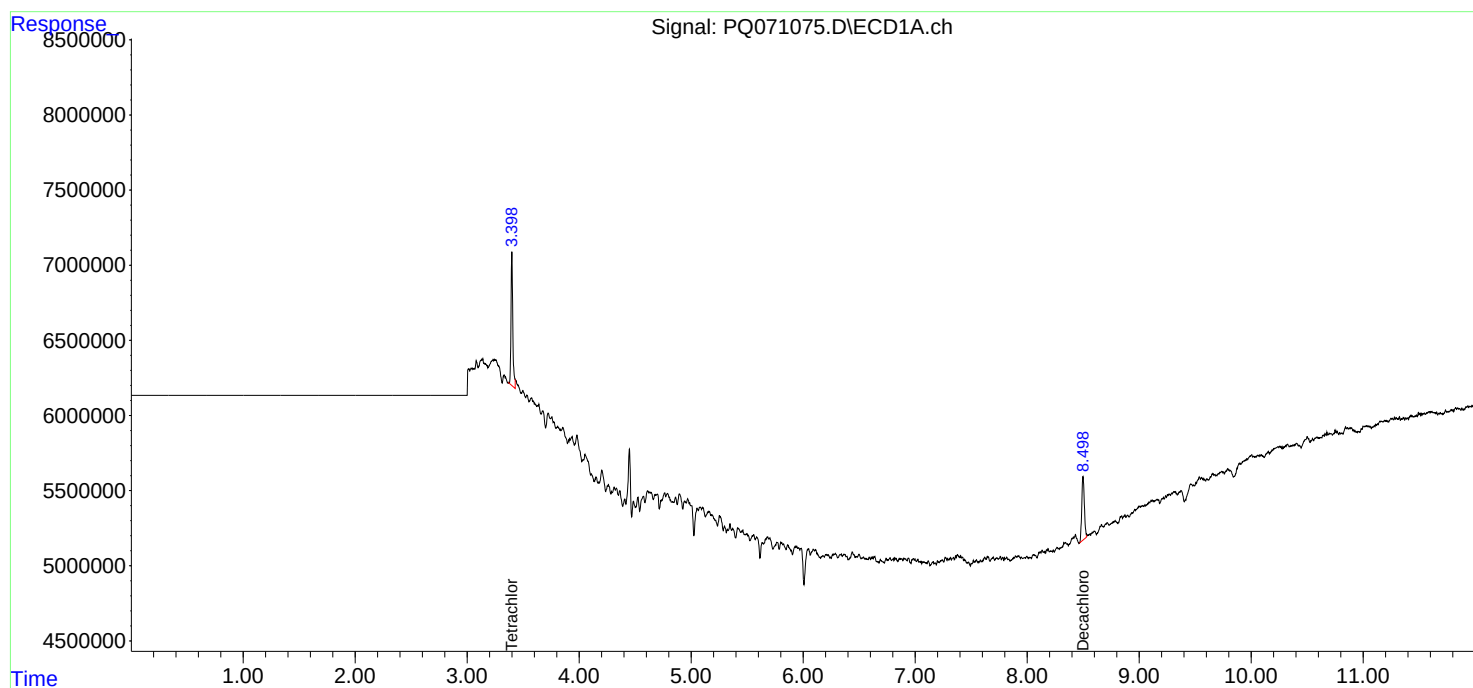

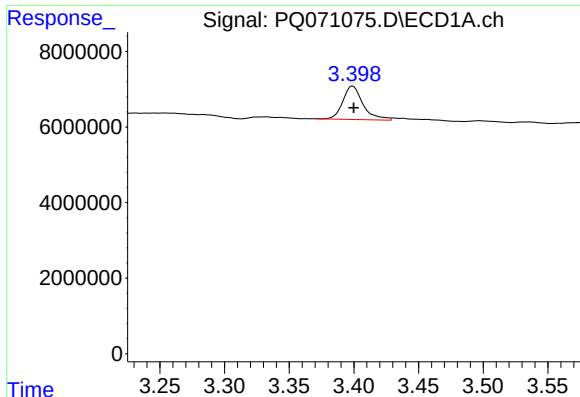


#1 Tetrachloro-m-xylene

R.T.: 3.399 min
Delta R.T.: 0.000 min
Response: 9638056
Conc: 2.22 ng/ml

Instrument :
ECD_Q
ClientSampleId :
L46-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2025
Supervised By :mohammad ahmed 10/24/2025

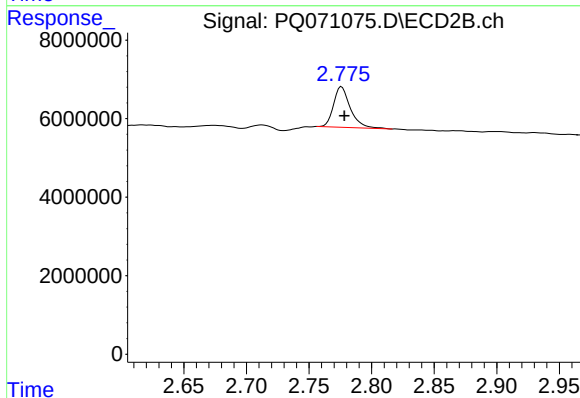


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: -0.002 min
Response: 9710009
Conc: 1.91 ng/ml

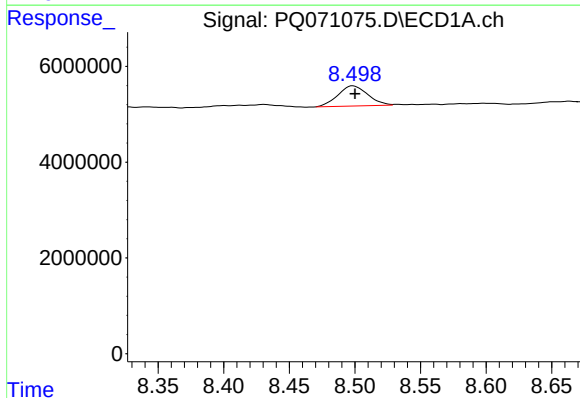

#2 Decachlorobiphenyl

R.T.: 8.498 min
Delta R.T.: -0.002 min
Response: 6730040
Conc: 2.32 ng/ml m

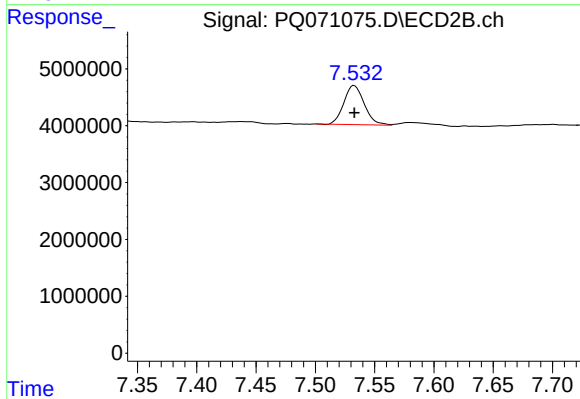

#2 Decachlorobiphenyl

R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 8245257
Conc: 1.63 ng/ml