

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102720\
 Data File : PQ050741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 00:46
 Operator : DD\AJ
 Sample : L4515-01 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 OS-1-BLDG-9-N-ELEVATOR

Manual Integrations
 APPROVED

Ankita
 10/29/2020 8:22:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 03:27:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 23 16:18:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.188	4.263	31565810	7246431	1.452	1.157
2) SA Decachlor...	11.365	9.613	27348322	8199499	2.186m	1.235m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102720\
Data File : PQ050741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 00:46
Operator : DD\AJ
Sample : L4515-01 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
OS-1-BLDG-9-N-ELEVATOR


Manual Integrations
APPROVED

Ankita
10/29/2020 8:22:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 03:27:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 23 16:18:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

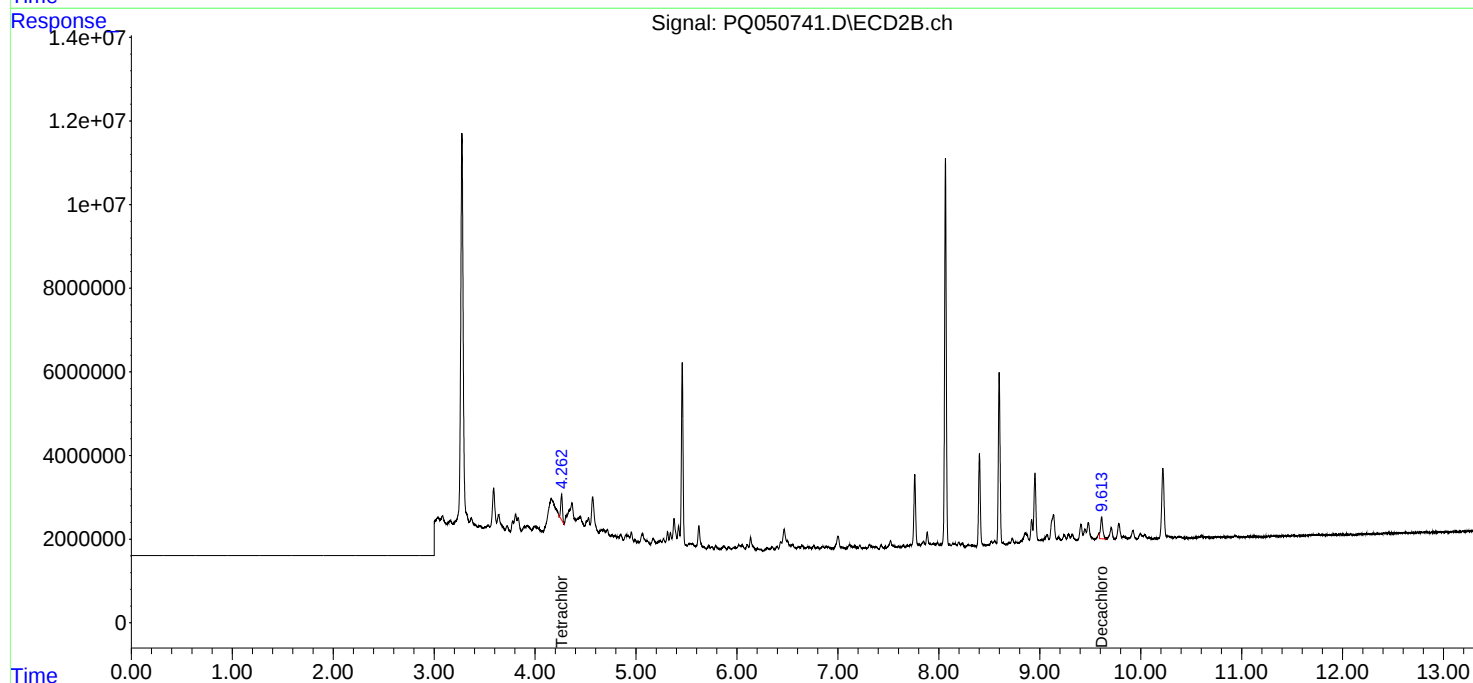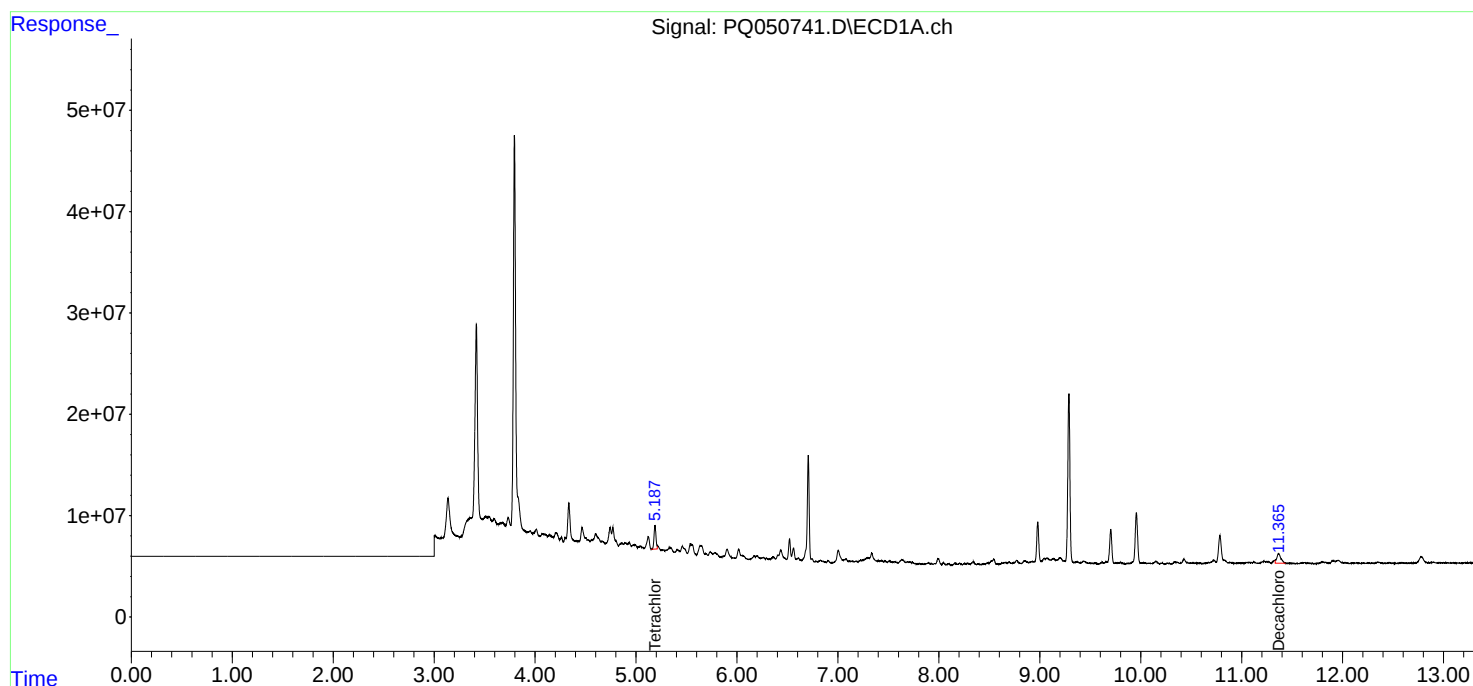

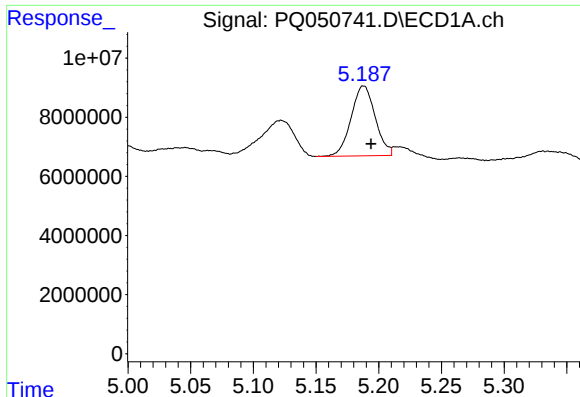


#1 Tetrachloro-m-xylene

R.T.: 5.188 min
Delta R.T.: -0.006 min
Response: 31565810
Conc: 1.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
OS-1-BLDG-9-N-ELEVATOR


Manual Integrations
APPROVED

Ankita
10/29/2020 8:22:52 AM

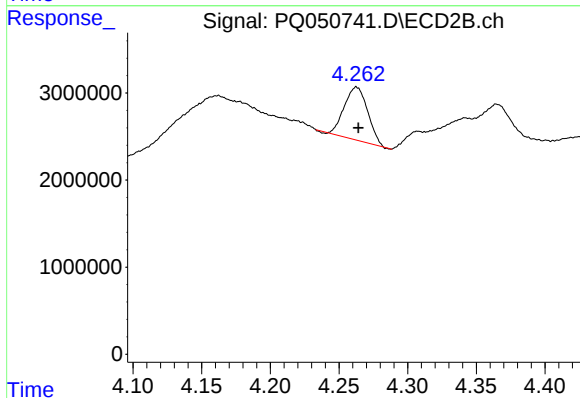


#1 Tetrachloro-m-xylene

R.T.: 4.263 min
Delta R.T.: -0.001 min
Response: 7246431
Conc: 1.16 ng/ml

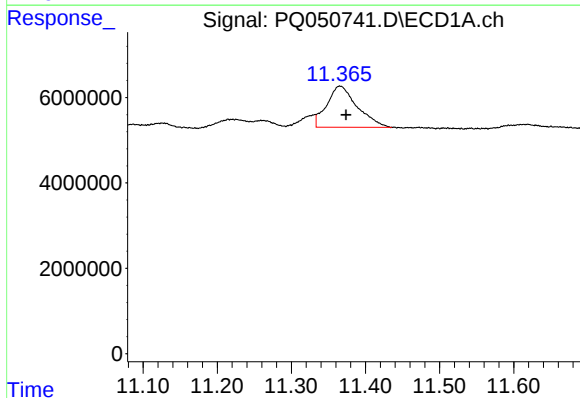

#2 Decachlorobiphenyl

R.T.: 11.365 min
Delta R.T.: -0.009 min
Response: 27348322
Conc: 2.19 ng/ml m

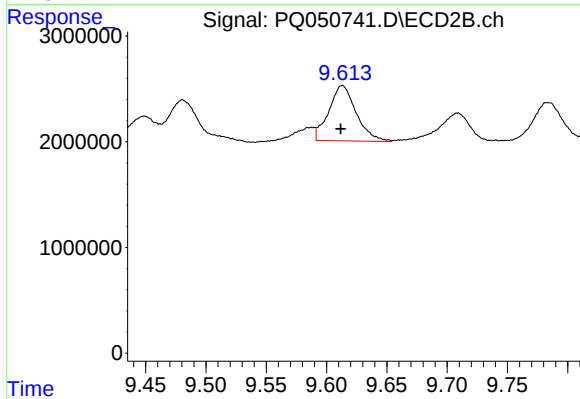

#2 Decachlorobiphenyl

R.T.: 9.613 min
Delta R.T.: 0.001 min
Response: 8199499
Conc: 1.23 ng/ml m