

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102720\
 Data File : PQ050745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 01:52
 Operator : DD\AJ
 Sample : L4515-05 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 OS-5-BLDG-5-ELEVATOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 03:29:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 23 16:18:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.189	4.262	26652641	12360847	1.226	1.973 #
2) SA Decachlor...	11.367	9.614	21645986	7369037	1.731	1.110 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102720\
Data File : PQ050745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 01:52
Operator : DD\AJ
Sample : L4515-05 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
OS-5-BLDG-5-ELEVATOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 03:29:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 23 16:18:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

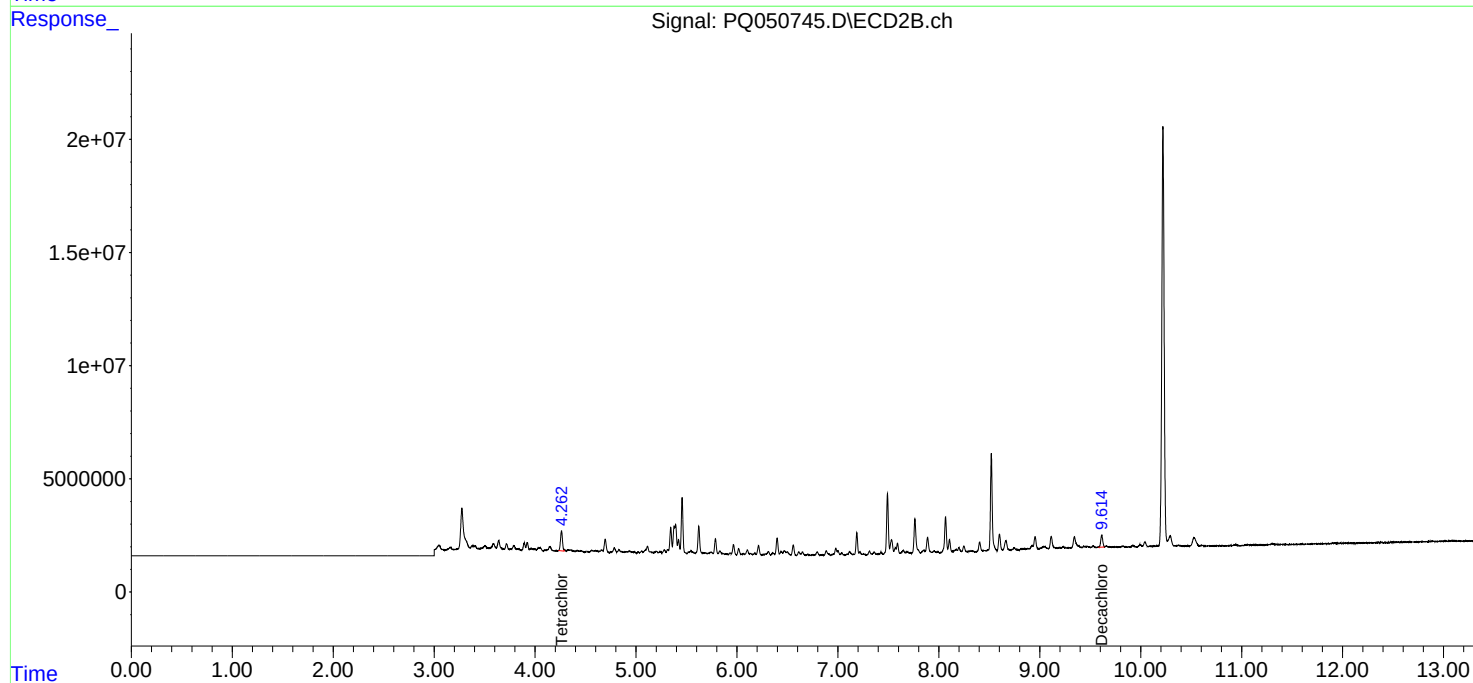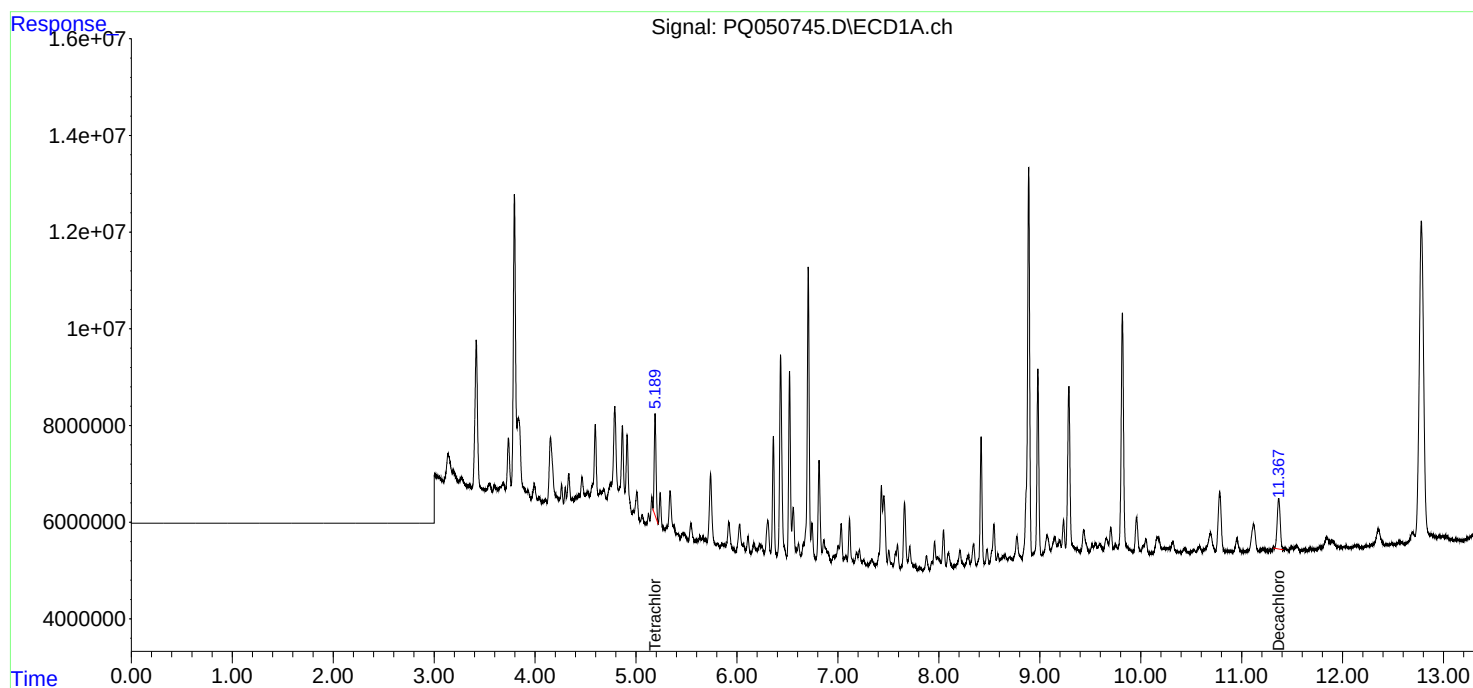


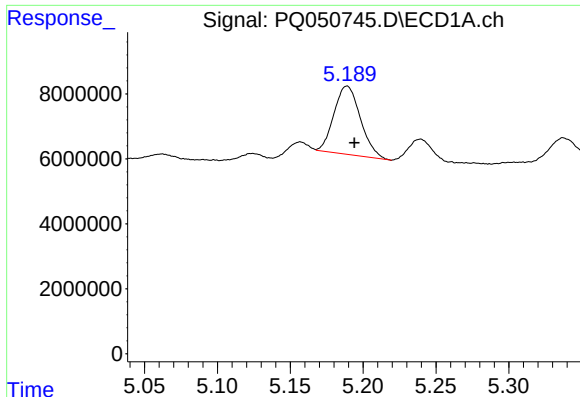

#1 Tetrachloro-m-xylene


R.T.: 5.189 min
Delta R.T.: -0.005 min
Response: 26652641
Conc: 1.23 ng/ml

Instrument :
ECD_Q
ClientSampleId :
OS-5-BLDG-5-ELEVATOR

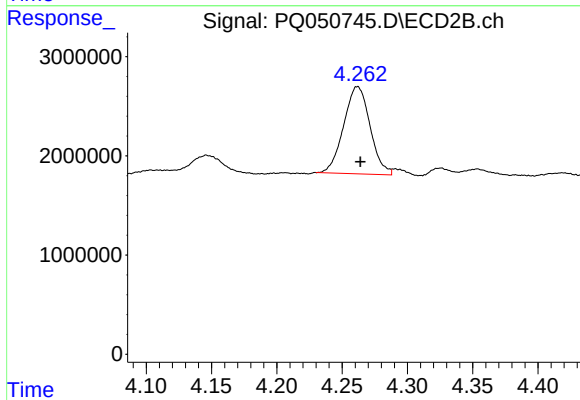


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: -0.002 min
Response: 12360847
Conc: 1.97 ng/ml

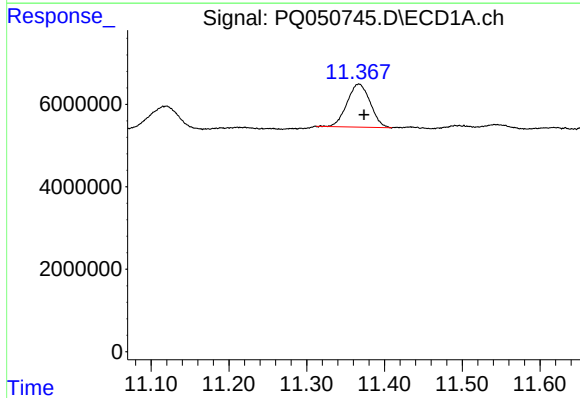

#2 Decachlorobiphenyl

R.T.: 11.367 min
Delta R.T.: -0.007 min
Response: 21645986
Conc: 1.73 ng/ml

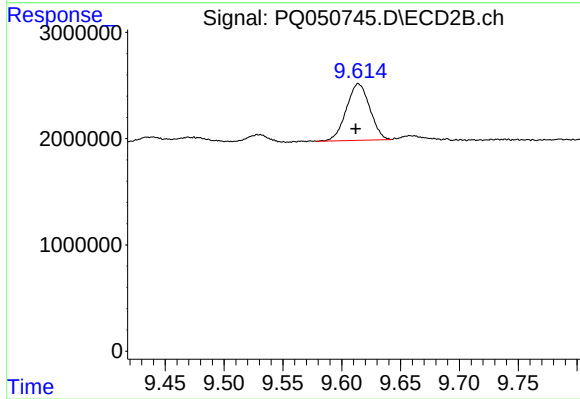

#2 Decachlorobiphenyl

R.T.: 9.614 min
Delta R.T.: 0.002 min
Response: 7369037
Conc: 1.11 ng/ml