

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
 Data File : PS032162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 11:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 04:06:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 28 04:02:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.281	7.745	1645.7E6	594.0E6	380.634	543.197 #
Target Compounds							
1) T	Dalapon	0.000	2.714f	0	80263449	N.D.	21.823
2) T	3,5-DICHL...	6.455	0.000	163801	0	<MDL	N.D. #
6) T	MCP	0.000	8.062f	0	1538128	N.D.	<MDL
7) T	MCPA	7.789	8.236f	111273	25082422	<MDL	7.163 #
8) T	DICHLORPROP	8.169	0.000	1249688	0	<MDL	N.D. #
9) T	2,4-D	8.378f	0.000	211731	0	<MDL	N.D. #
10) T	Pentachlo...	8.712	0.000	3504257	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.303f	9.913	709211	11449604	<MDL	<MDL #
12) T	2,4,5-T	9.581	0.000	591039	0	<MDL	N.D. #
13) T	2,4-DB	10.178	0.000	7027575	0	3.054	N.D. #
14) T	DINOSEB	11.356	0.000	2359899	0	<MDL	N.D. #
15) T	Picloram	11.213	0.000	378260	0	<MDL	N.D. #
16) T	DCPA	11.643	0.000	1896261	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 11:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 04:06:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:02:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

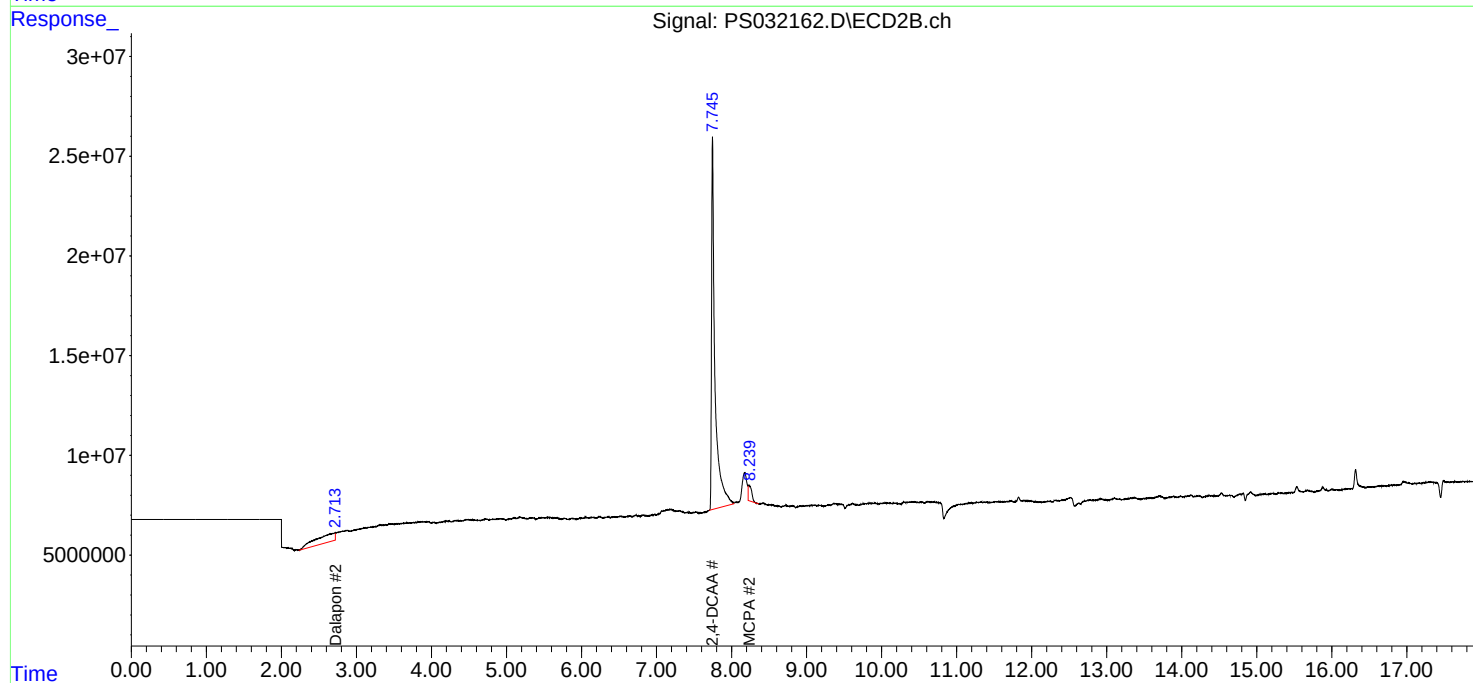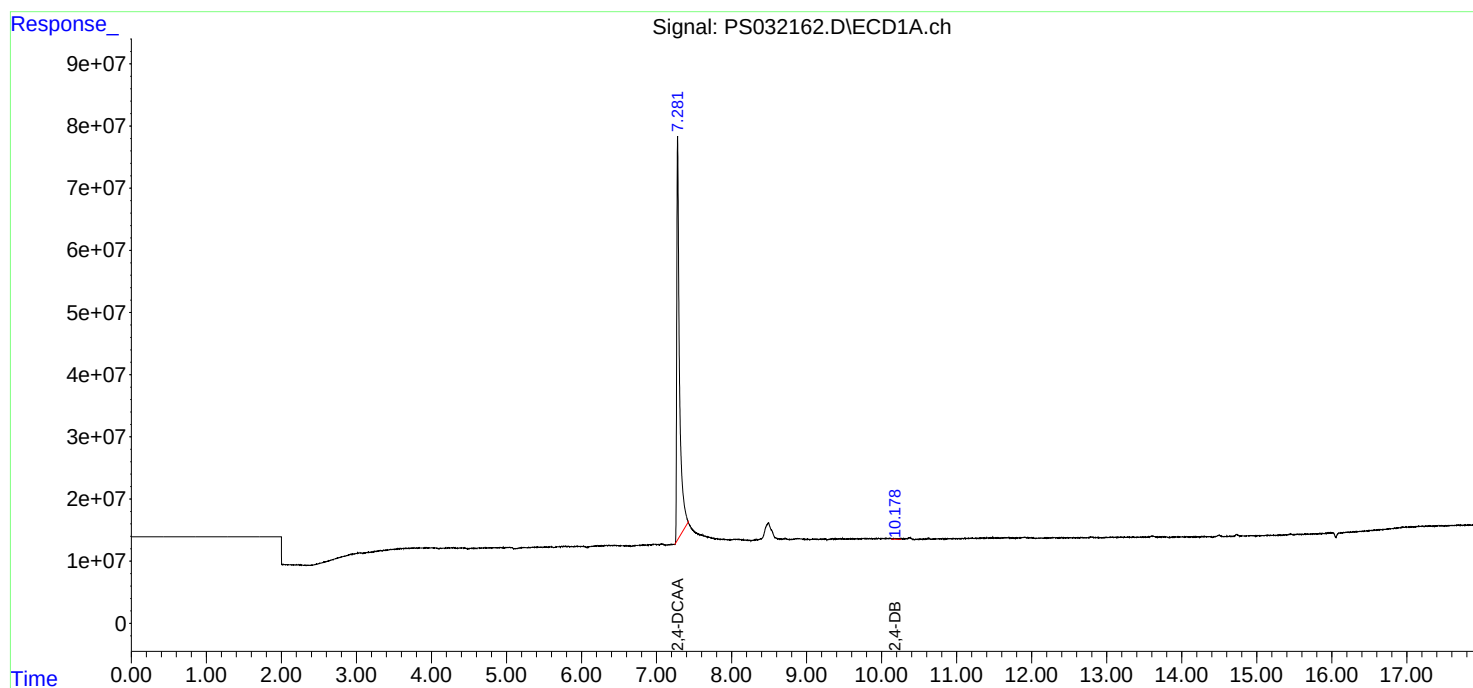


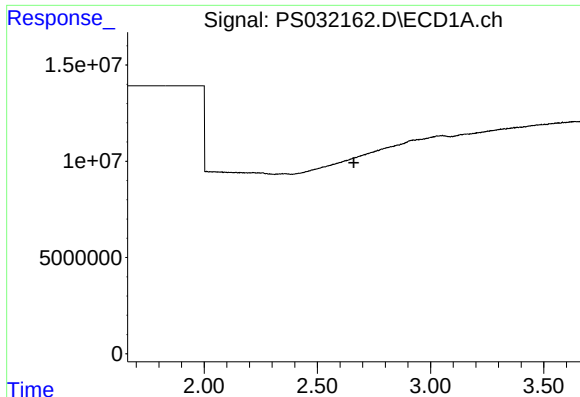

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.661 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
I.BLK

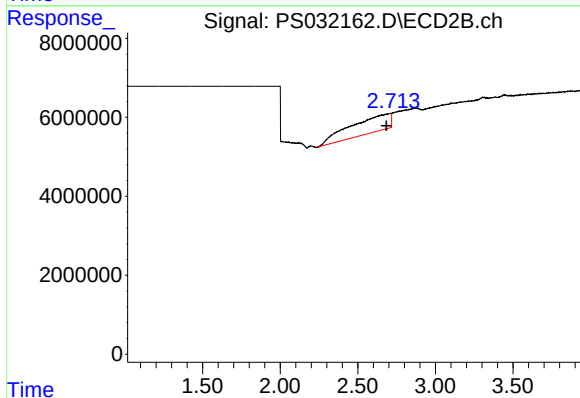


#1 Dalapon

R.T.: 2.714 min
Delta R.T.: 0.029 min
Response: 80263449
Conc: 21.82 ng/ml

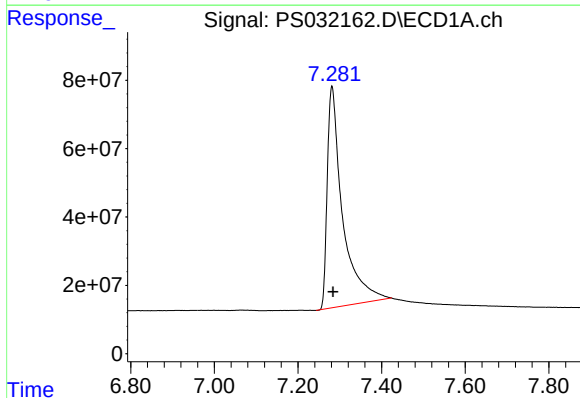


#4 2,4-DCAA

R.T.: 7.281 min
Delta R.T.: -0.003 min
Response: 1645734694
Conc: 380.63 ng/ml

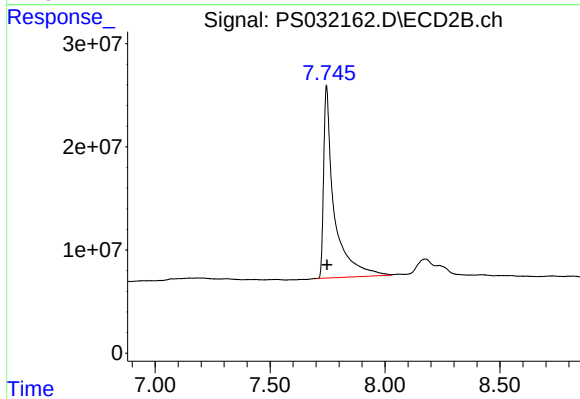

#4 2,4-DCAA


R.T.: 7.745 min
Delta R.T.: -0.002 min
Response: 594004792
Conc: 543.20 ng/ml

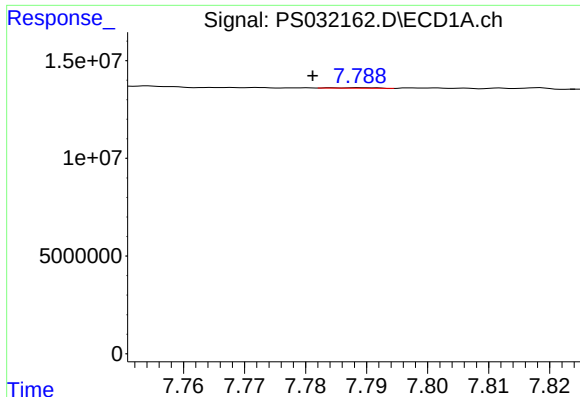

#7 MCPA


R.T.: 7.789 min
Delta R.T.: 0.008 min
Response: 111273
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
I.BLK

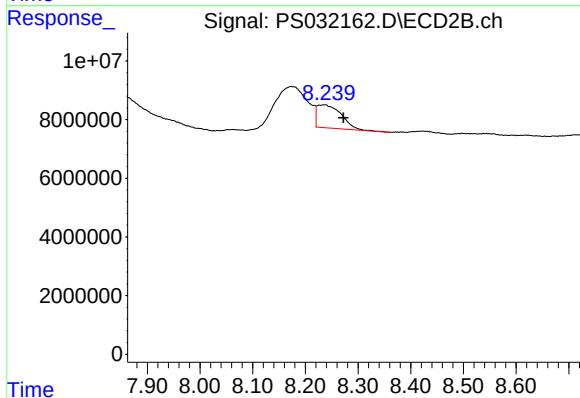


#7 MCPA

R.T.: 8.236 min
Delta R.T.: -0.036 min
Response: 25082422
Conc: 7.16 ug/ml

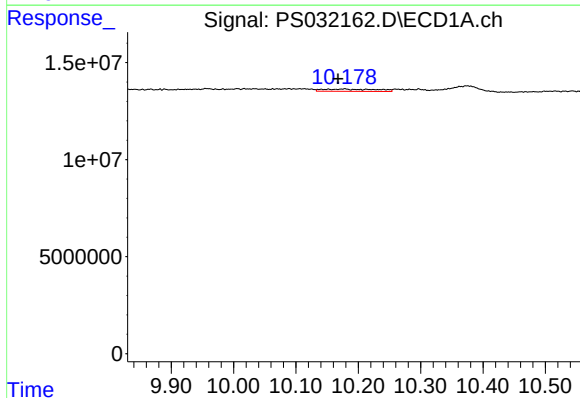

#13 2,4-DB

R.T.: 10.178 min
Delta R.T.: 0.011 min
Response: 7027575
Conc: 3.05 ng/ml

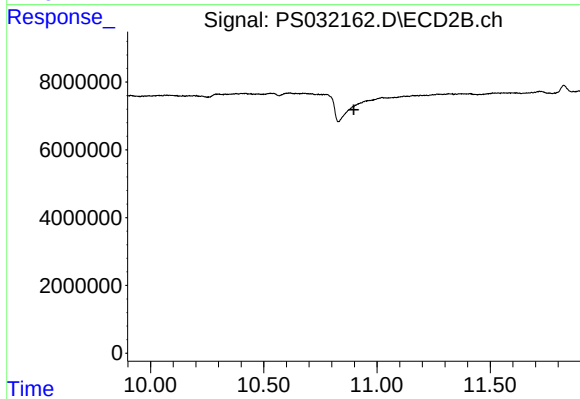

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.898 min
Response: 0
Conc: N.D.