

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102920\
 Data File : PQ050779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 09:45
 Operator : DD\AJ
 Sample : L4528-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 CHRT-24245

Manual Integrations
 APPROVED

Ankita
 10/30/2020 3:58:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:55:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 23 16:18:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.201	4.262	410.7E6	108.5E6	18.883	17.312
2) SA Decachlor...	11.406f	9.634f	199.2E6	69321676	15.926m	10.438m#
Target Compounds						
26) L6 AR-1254-1	7.446	6.402	23627764	9183684	42.569	31.306 #
27) L6 AR-1254-2	7.678	6.562	36398479	7350459	42.961	29.181 #
28) L6 AR-1254-3	8.065	6.984	45636291	13632429	53.716	32.775m#
29) L6 AR-1254-4	8.364	7.227	24532985	7593615	37.417	26.476 #
30) L6 AR-1254-5	8.794f	7.656	48079006	35888981	75.369	94.710 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102920\
Data File : PQ050779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 09:45
Operator : DD\AJ
Sample : L4528-03
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/30/2020 3:58:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:55:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 23 16:18:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

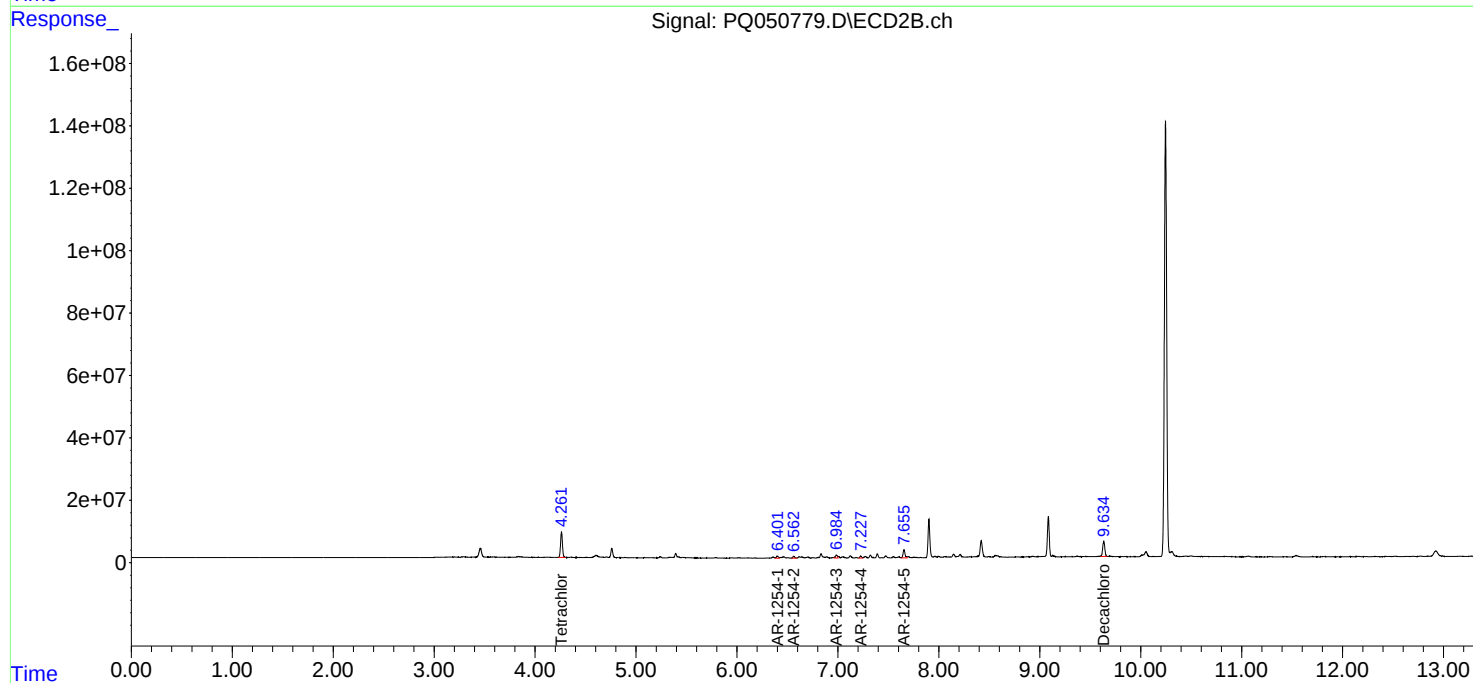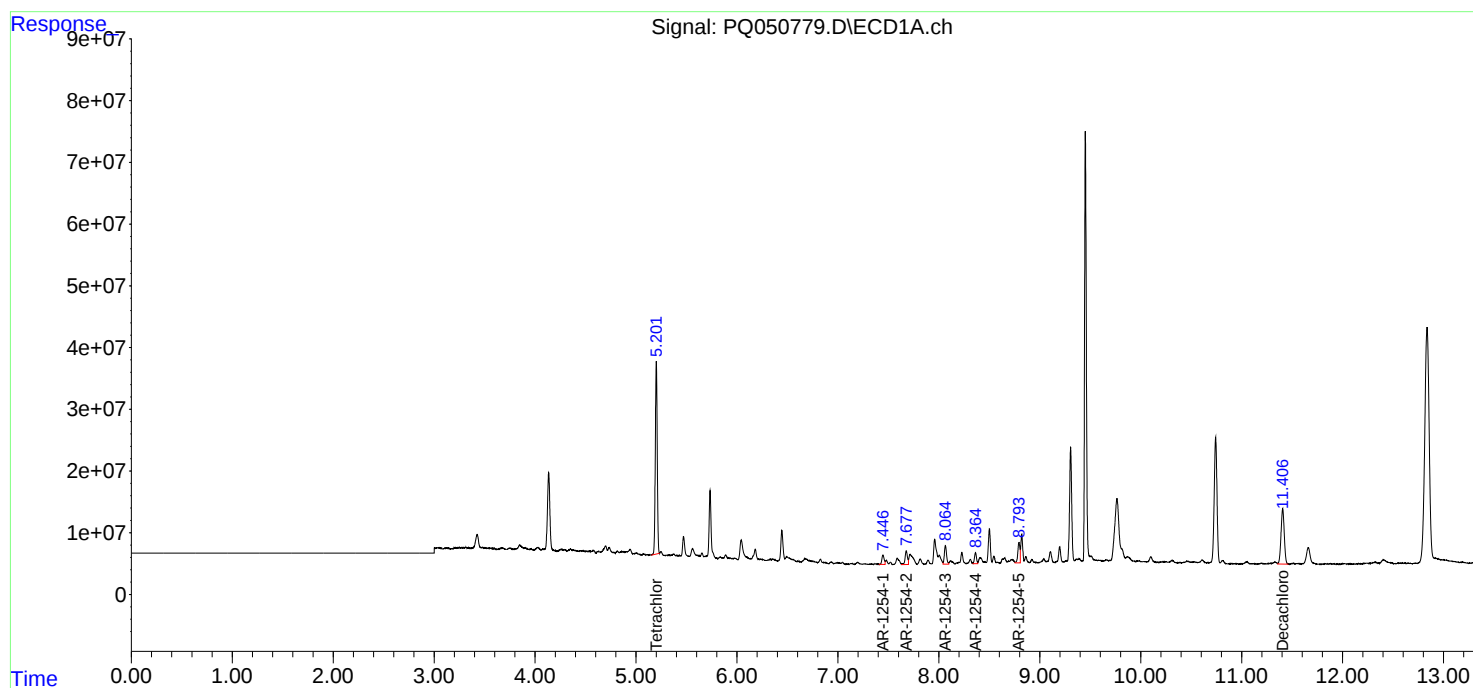

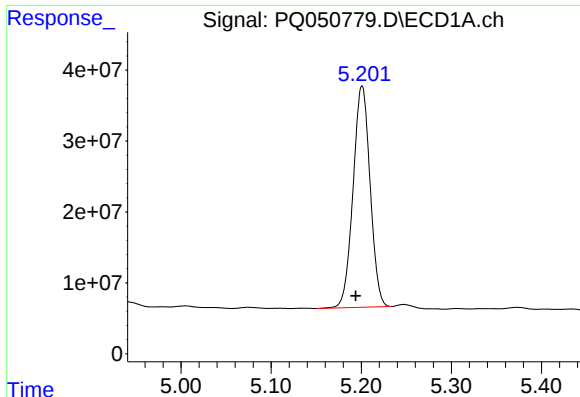


#1 Tetrachloro-m-xylene

R.T.: 5.201 min
Delta R.T.: 0.007 min
Response: 410651463
Conc: 18.88 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/30/2020 3:58:13 PM

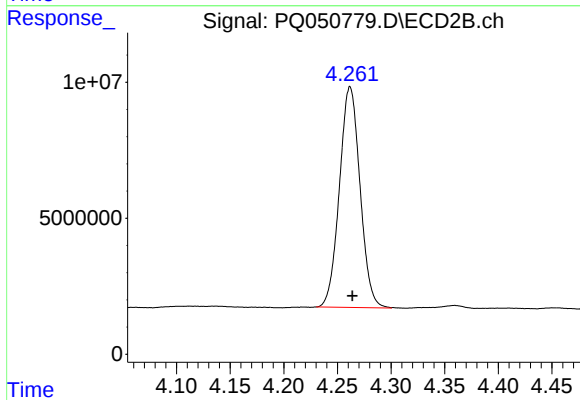


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: -0.002 min
Response: 108455498
Conc: 17.31 ng/ml

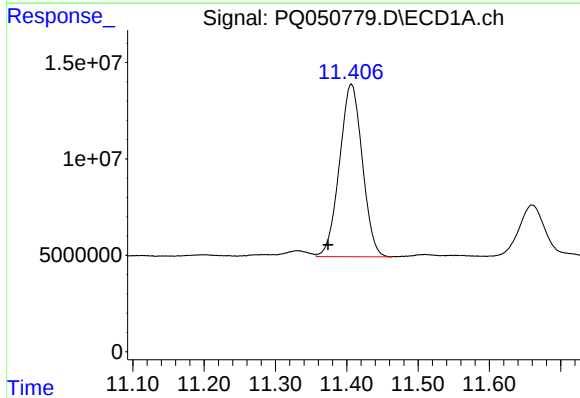


#2 Decachlorobiphenyl

R.T.: 11.406 min
Delta R.T.: 0.032 min
Response: 199201214
Conc: 15.93 ng/ml m

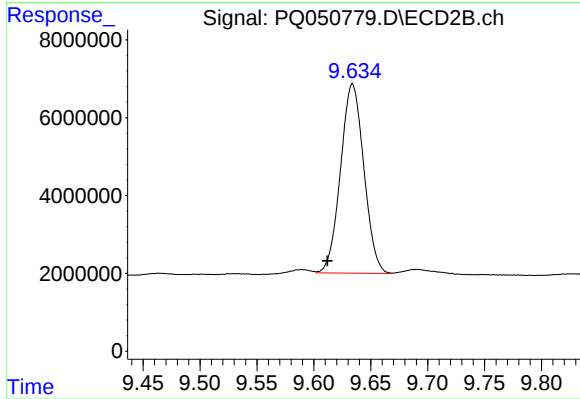

#2 Decachlorobiphenyl

R.T.: 9.634 min
Delta R.T.: 0.022 min
Response: 69321676
Conc: 10.44 ng/ml m

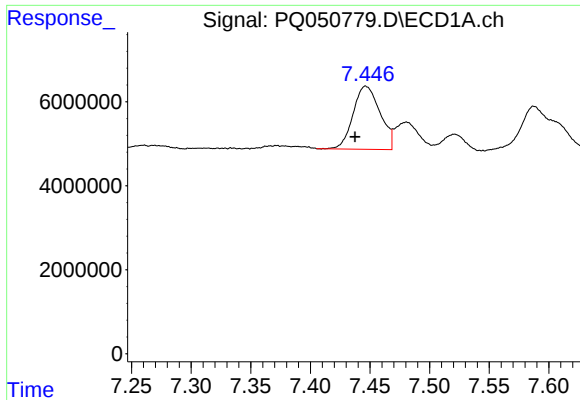


#26 AR-1254-1

R.T.: 7.446 min
Delta R.T.: 0.009 min
Response: 23627764
Conc: 42.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/30/2020 3:58:13 PM

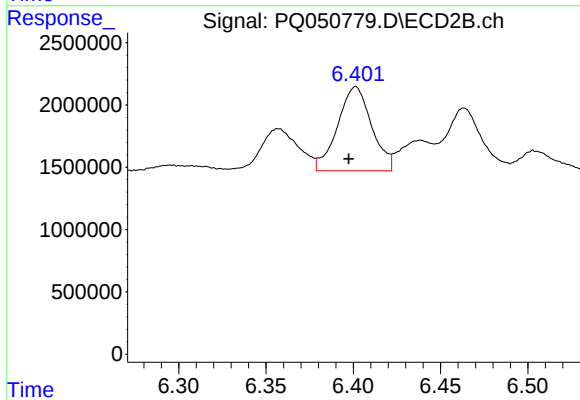


#26 AR-1254-1

R.T.: 6.402 min
Delta R.T.: 0.004 min
Response: 9183684
Conc: 31.31 ng/ml

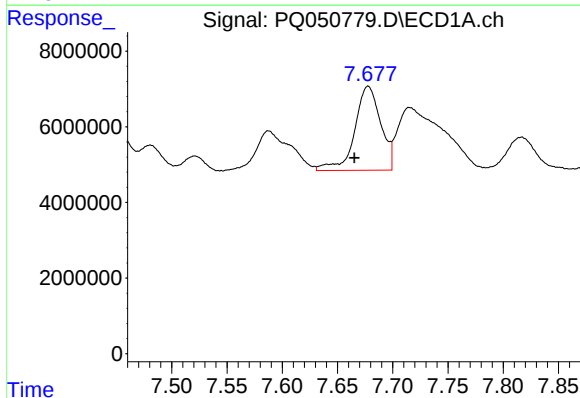


#27 AR-1254-2

R.T.: 7.678 min
Delta R.T.: 0.013 min
Response: 36398479
Conc: 42.96 ng/ml

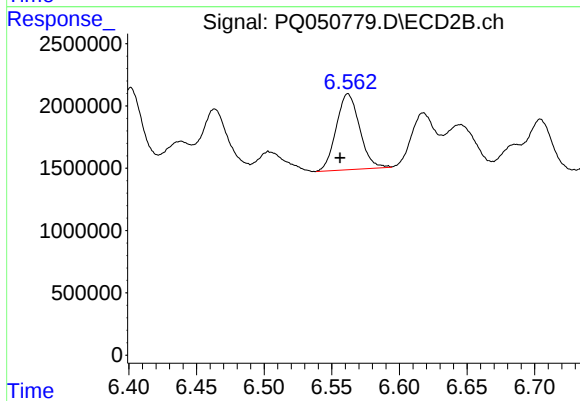

#27 AR-1254-2

R.T.: 6.562 min
Delta R.T.: 0.006 min
Response: 7350459
Conc: 29.18 ng/ml

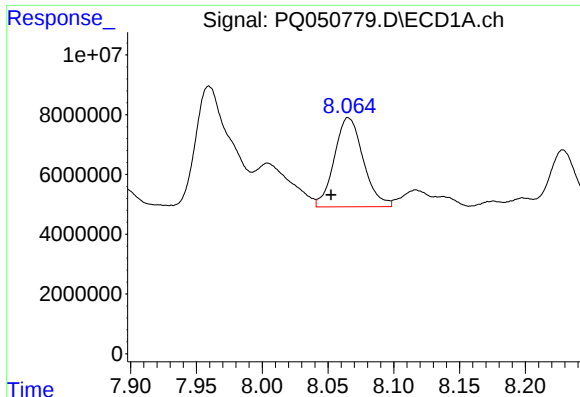


#28 AR-1254-3

R.T.: 8.065 min
Delta R.T.: 0.013 min
Response: 45636291
Conc: 53.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/30/2020 3:58:13 PM

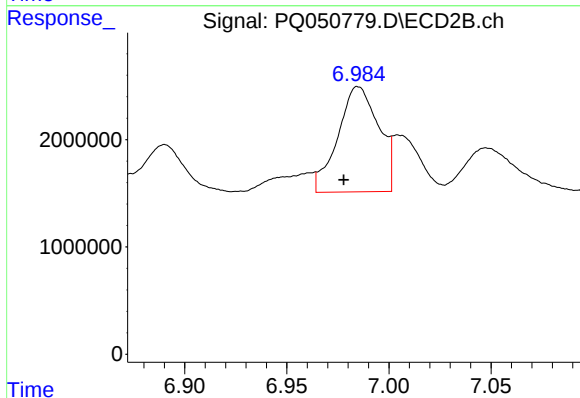


#28 AR-1254-3

R.T.: 6.984 min
Delta R.T.: 0.006 min
Response: 13632429
Conc: 32.77 ng/ml m

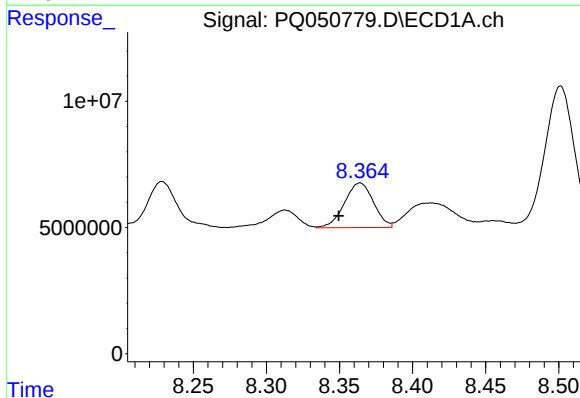


#29 AR-1254-4

R.T.: 8.364 min
Delta R.T.: 0.015 min
Response: 24532985
Conc: 37.42 ng/ml

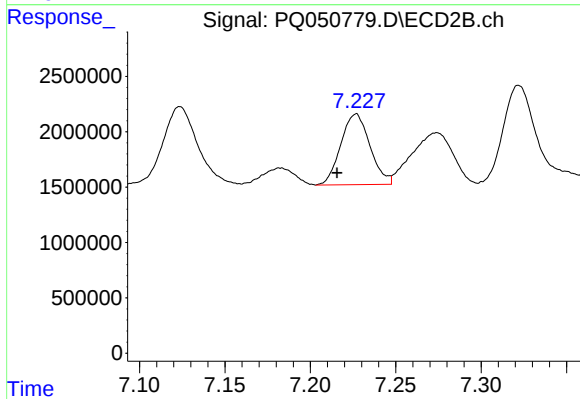

#29 AR-1254-4

R.T.: 7.227 min
Delta R.T.: 0.011 min
Response: 7593615
Conc: 26.48 ng/ml

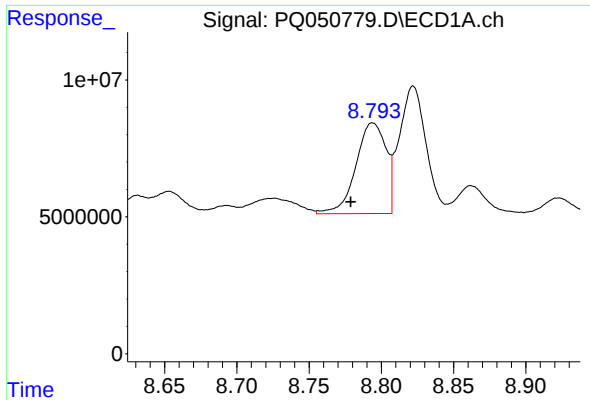


#30 AR-1254-5

R.T.: 8.794 min
Delta R.T.: 0.015 min
Response: 48079006
Conc: 75.37 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CHRT-24245

Manual Integrations
APPROVED

Ankita
10/30/2020 3:58:13 PM

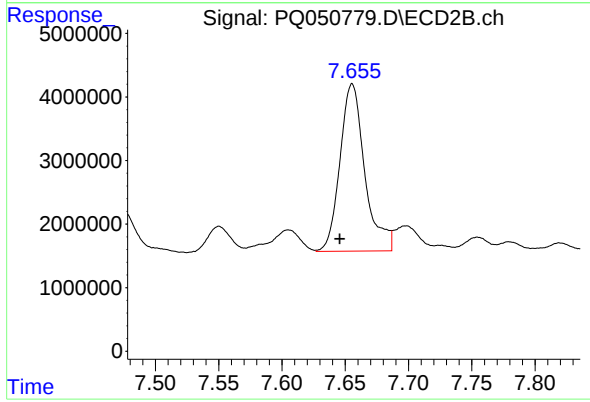

#30 AR-1254-5

R.T.: 7.656 min
Delta R.T.: 0.010 min
Response: 35888981
Conc: 94.71 ng/ml