

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ103019\
Data File : PQ044622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 15:09
Operator : HP\AJ
Sample : K5111-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/31/2019 9:55:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 15:34:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ103019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 15:29:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

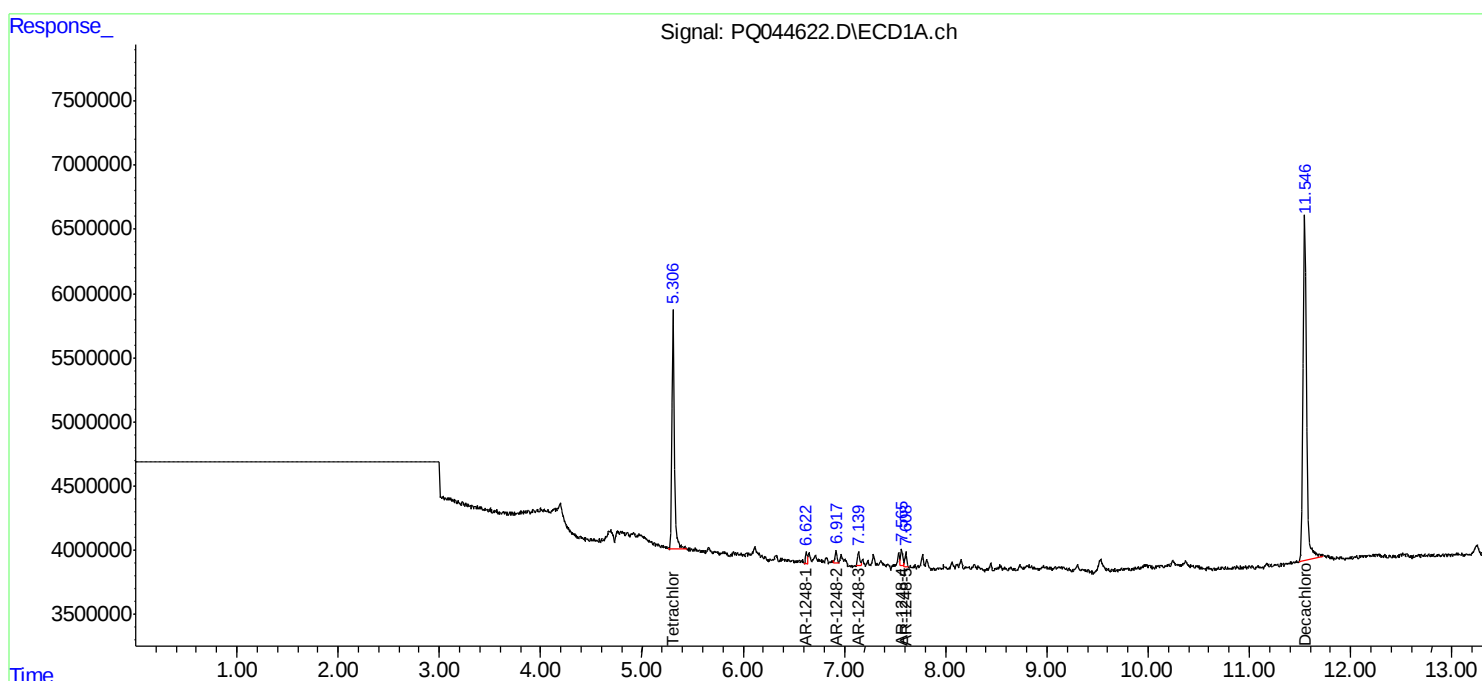

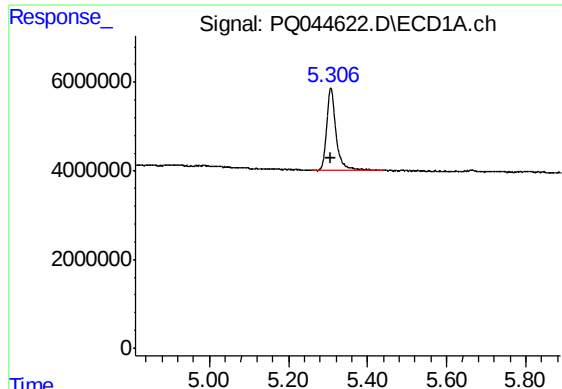


#1 Tetrachloro-m-xylene

R.T.: 5.307 min
Delta R.T.: 0.001 min
Response: 30496973
Conc: 14.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED


Ankita
10/31/2019 9:55:18 AM

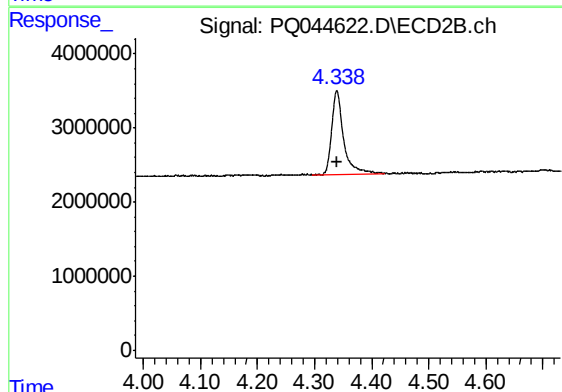

#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.001 min
Response: 16192917
Conc: 13.31 ng/ml

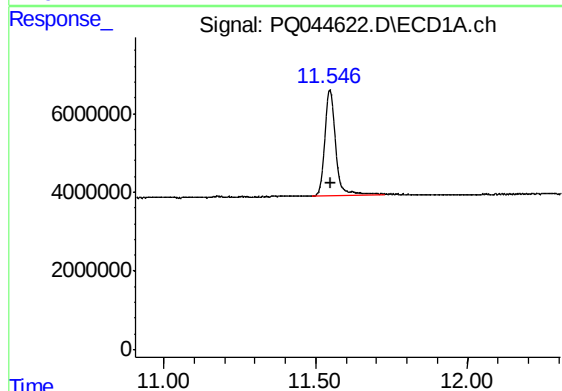

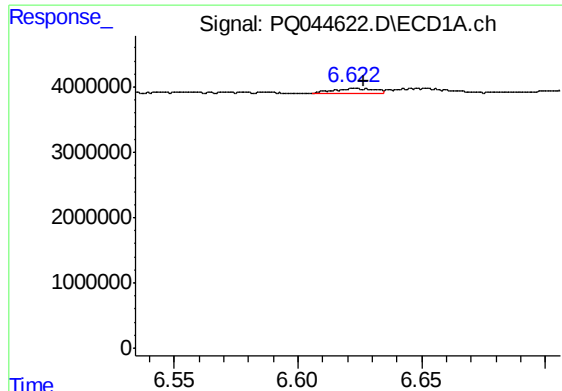


#21 AR-1248-1

R.T.: 6.622 min
Delta R.T.: -0.005 min
Response: 989978
Conc: 22.76 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED


Ankita
10/31/2019 9:55:18 AM

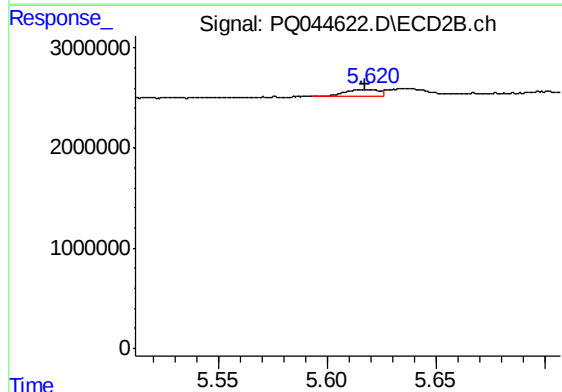

#21 AR-1248-1

R.T.: 5.620 min
Delta R.T.: 0.002 min
Response: 776883
Conc: 22.53 ng/ml m

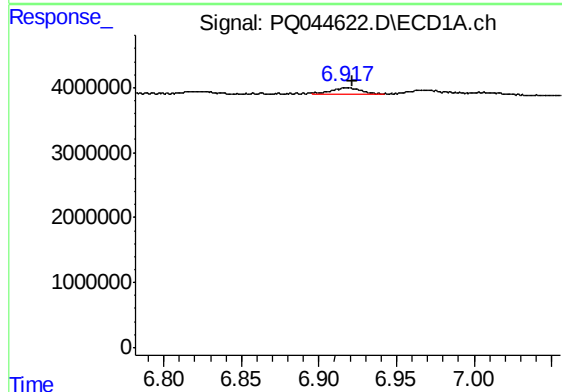

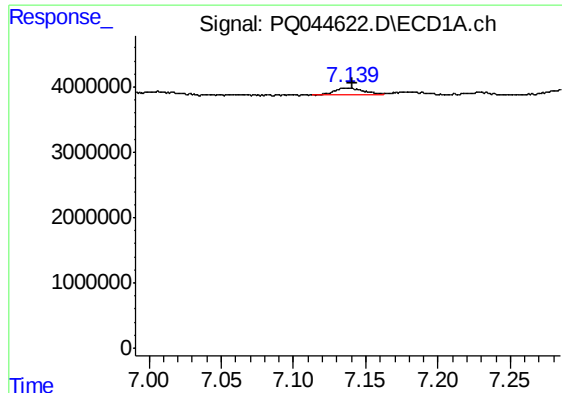


#23 AR-1248-3

R.T.: 7.139 min
Delta R.T.: -0.001 min
Response: 1567927
Conc: 21.02 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED


Ankita
10/31/2019 9:55:18 AM

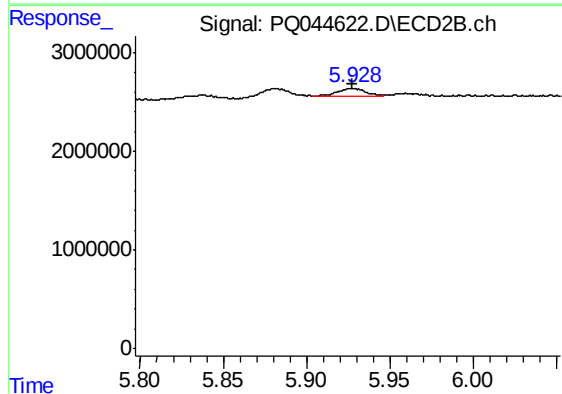

#23 AR-1248-3

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 985737
Conc: 18.10 ng/ml m

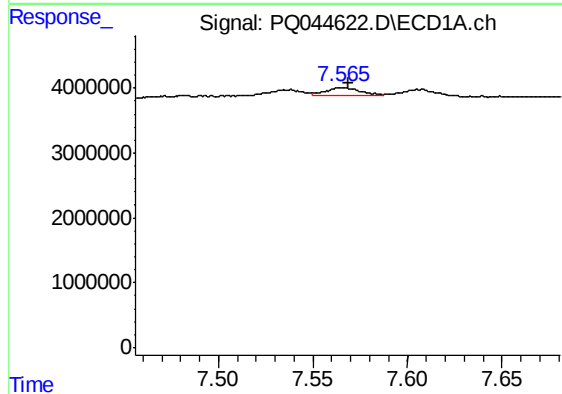

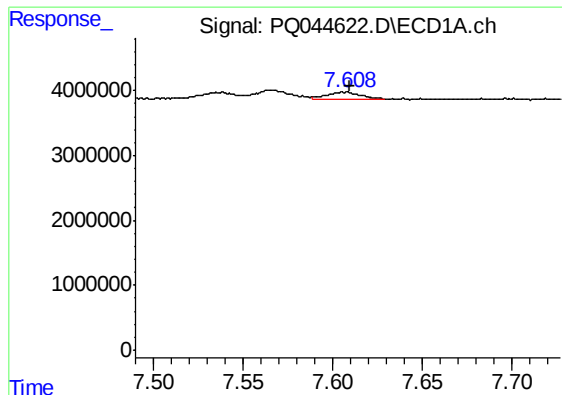


#25 AR-1248-5

R.T.: 7.608 min
Delta R.T.: -0.002 min
Response: 1335605
Conc: 16.12 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019

Manual Integrations
APPROVED

Ankita
10/31/2019 9:55:18 AM

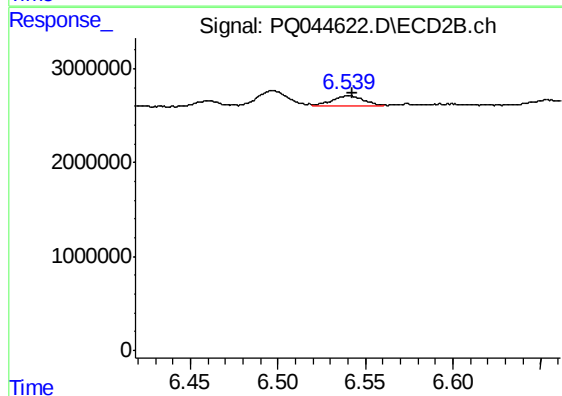

#25 AR-1248-5

R.T.: 6.539 min
Delta R.T.: -0.003 min
Response: 1307012
Conc: 18.24 ng/ml m