

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ103119\
 Data File : PQ044654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 09:13
 Operator : HP\AJ
 Sample : K5111-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT4-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 06:51:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ103019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 15:29:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.303	4.338	29537810	14482825	13.644	11.906
2) SA Decachlor...	11.537	9.750	78989446	91357636	16.645	21.400 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ103119\
Data File : PQ044654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 09:13
Operator : HP\AJ
Sample : K5111-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 06:51:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ103019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 15:29:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

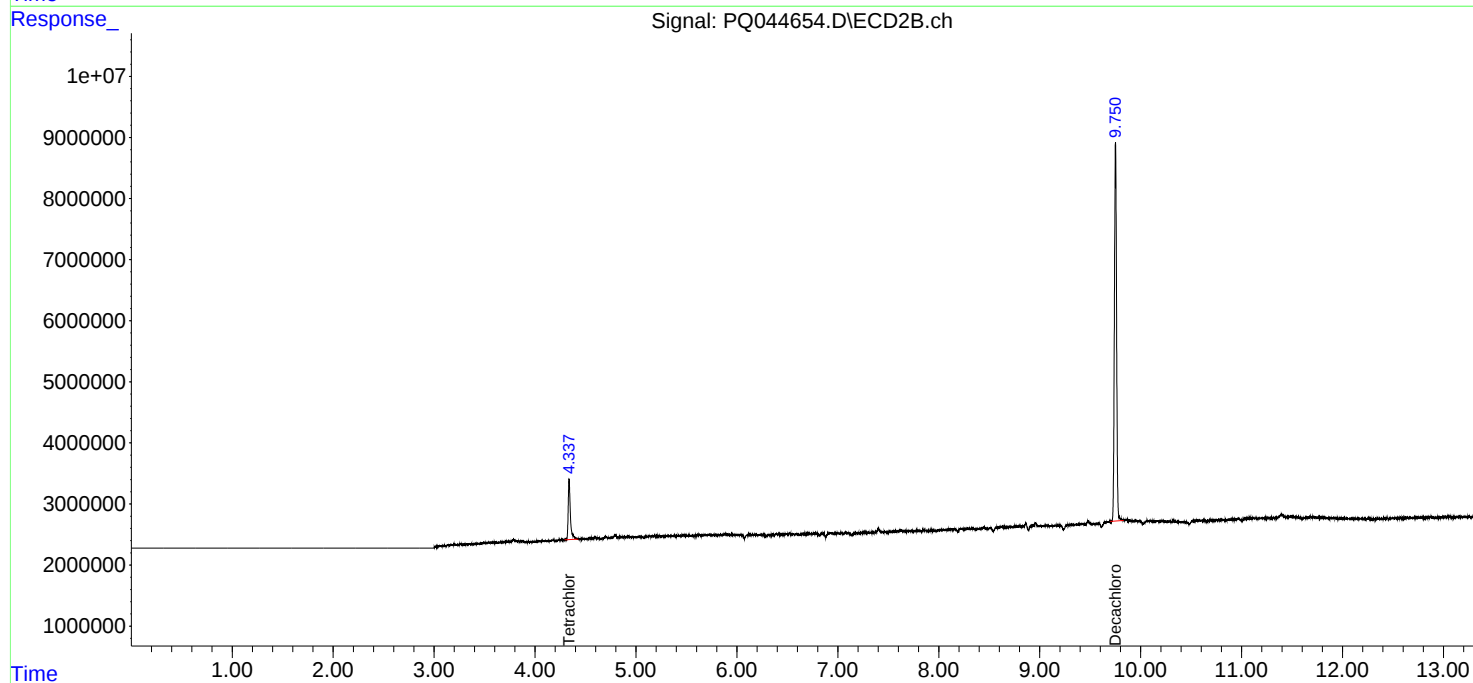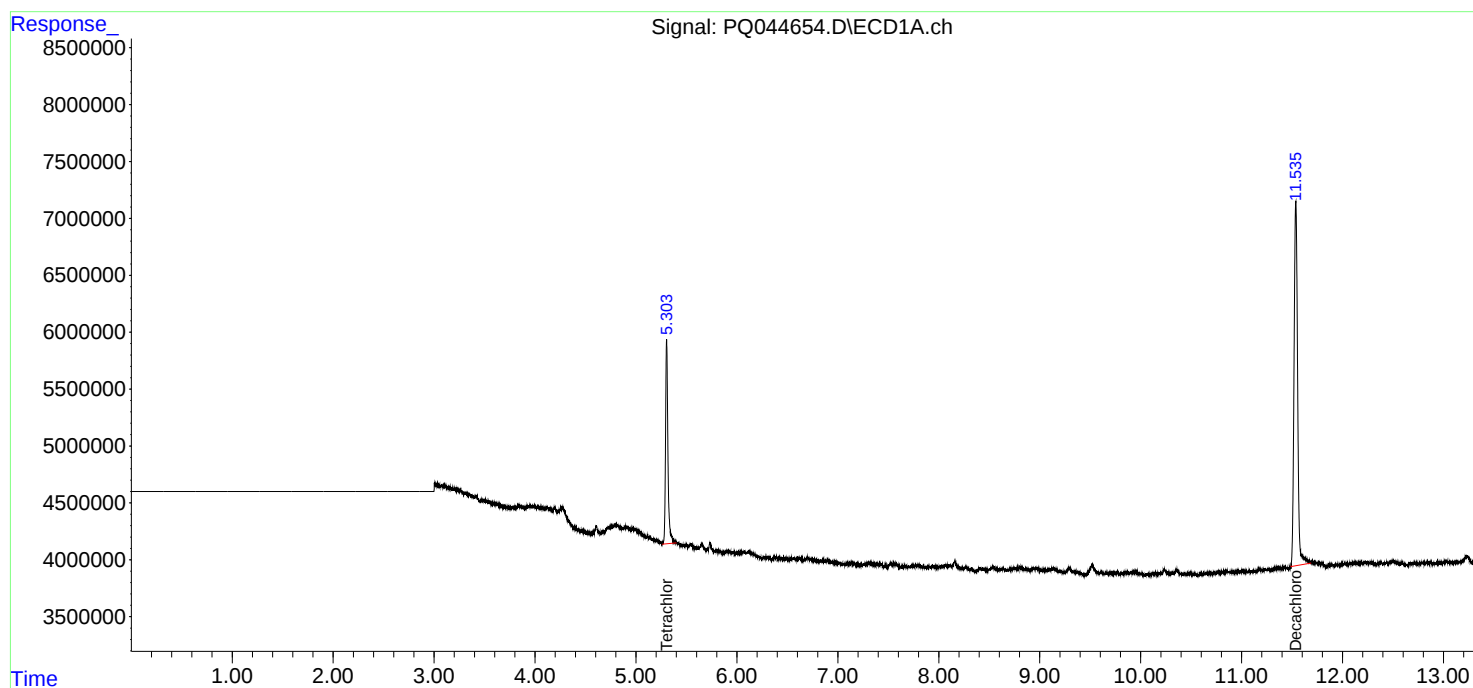


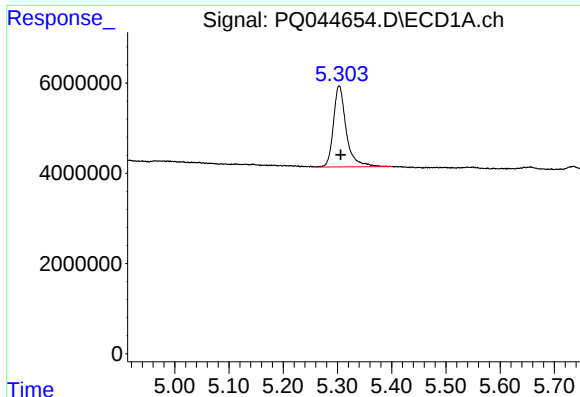

#1 Tetrachloro-m-xylene


R.T.: 5.303 min
Delta R.T.: -0.003 min
Response: 29537810
Conc: 13.64 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

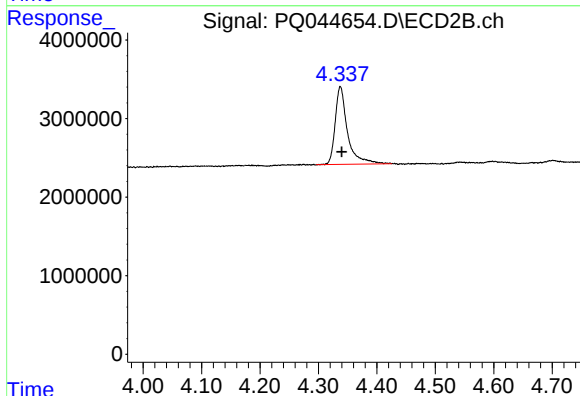


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.003 min
Response: 14482825
Conc: 11.91 ng/ml

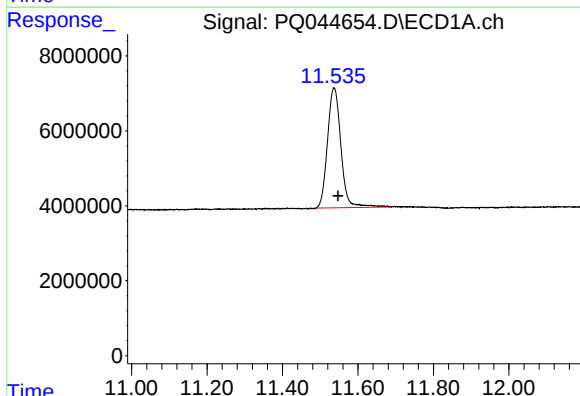

#2 Decachlorobiphenyl

R.T.: 11.537 min
Delta R.T.: -0.011 min
Response: 78989446
Conc: 16.64 ng/ml

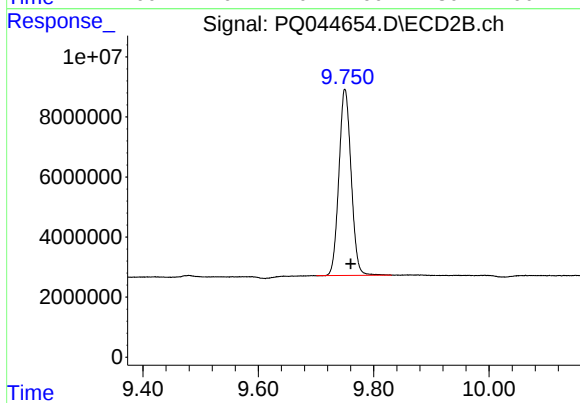

#2 Decachlorobiphenyl

R.T.: 9.750 min
Delta R.T.: -0.010 min
Response: 91357636
Conc: 21.40 ng/ml