

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ103119\
 Data File : PQ044655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 09:29
 Operator : HP\AJ
 Sample : K5111-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT4-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 06:51:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ103019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 15:29:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.304	4.338	25439276	12075311	11.751	9.927
2) SA Decachlor...	11.536	9.750	67565462	80384503	14.237	18.830 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ103119\
Data File : PQ044655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 09:29
Operator : HP\AJ
Sample : K5111-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 06:51:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ103019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 15:29:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

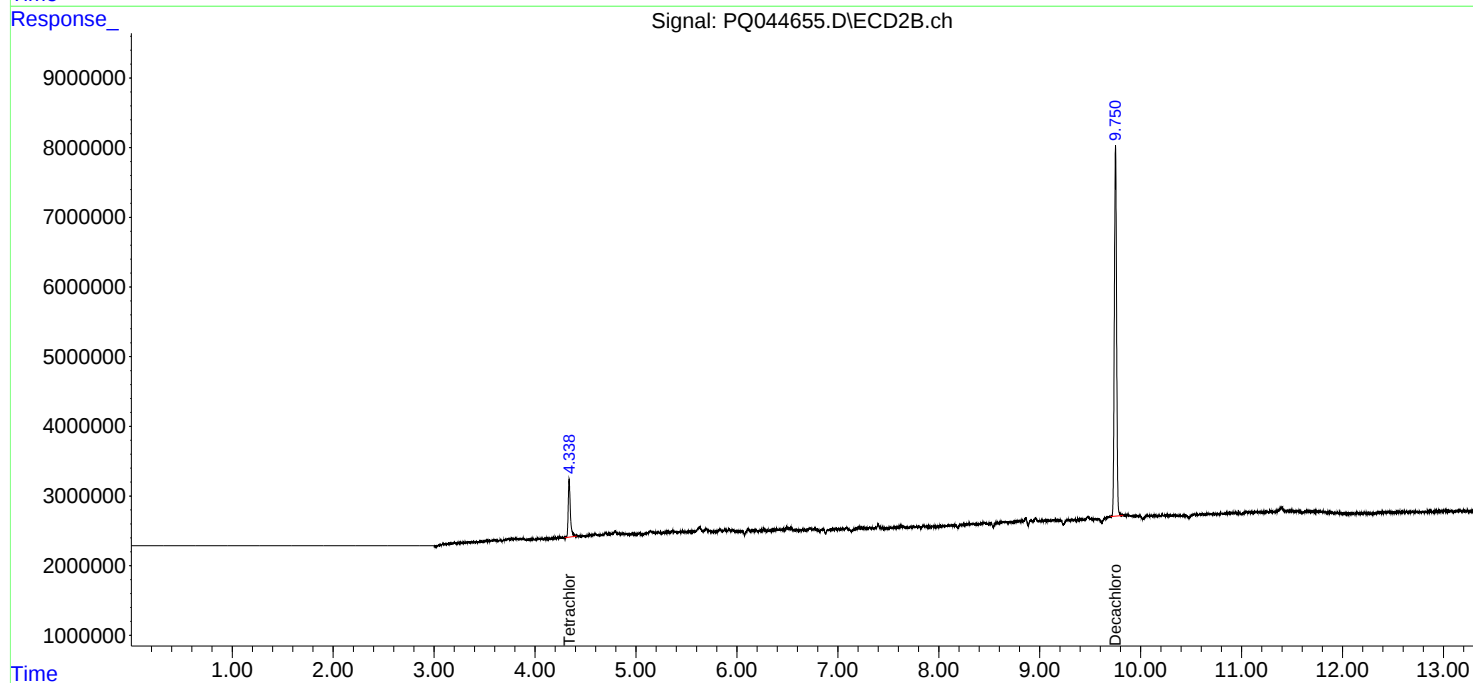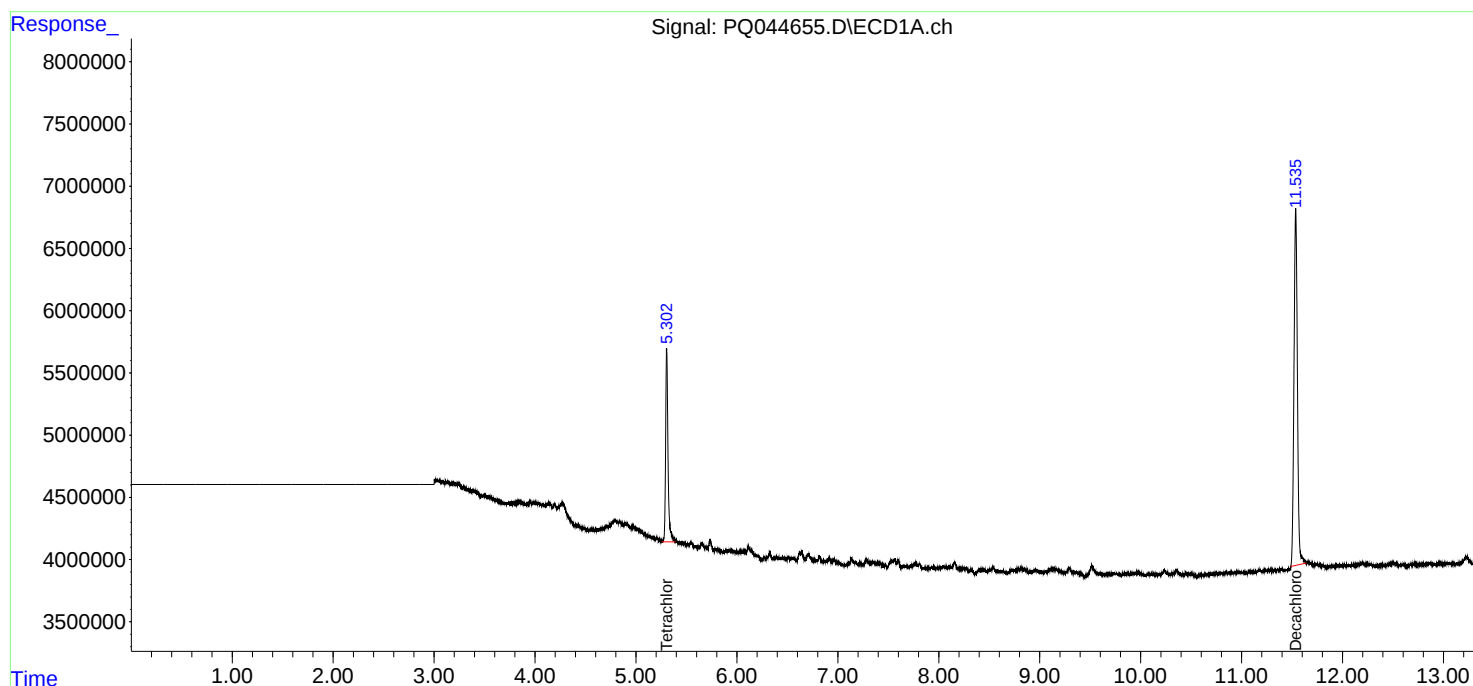


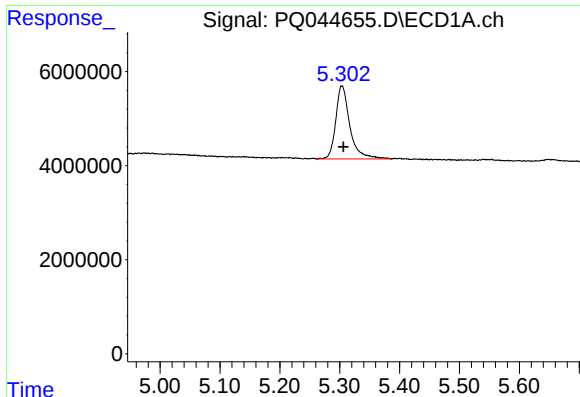

#1 Tetrachloro-m-xylene


R.T.: 5.304 min
Delta R.T.: -0.002 min
Response: 25439276
Conc: 11.75 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT4-2019

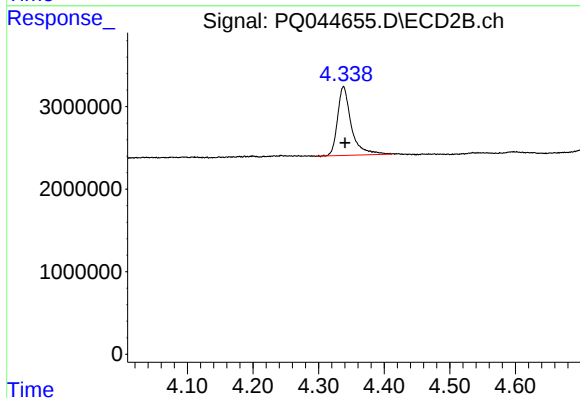


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.002 min
Response: 12075311
Conc: 9.93 ng/ml

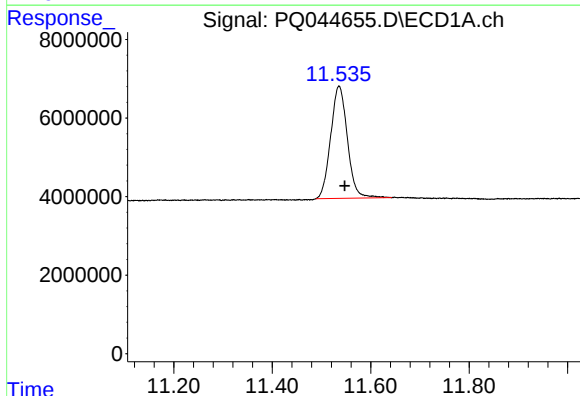

#2 Decachlorobiphenyl

R.T.: 11.536 min
Delta R.T.: -0.011 min
Response: 67565462
Conc: 14.24 ng/ml

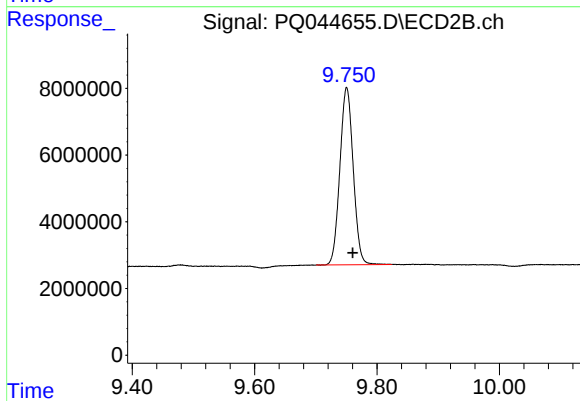

#2 Decachlorobiphenyl

R.T.: 9.750 min
Delta R.T.: -0.010 min
Response: 80384503
Conc: 18.83 ng/ml