

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110525\
 Data File : PQ071225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2025 20:34
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 04:21:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 06 04:20:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30) L6 AR-1254-5	6.592	5.811	2476.1E6	3483.3E6	8637.152	6624.292



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110525\
Data File : PQ071225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2025 20:34
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 04:21:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 06 04:20:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

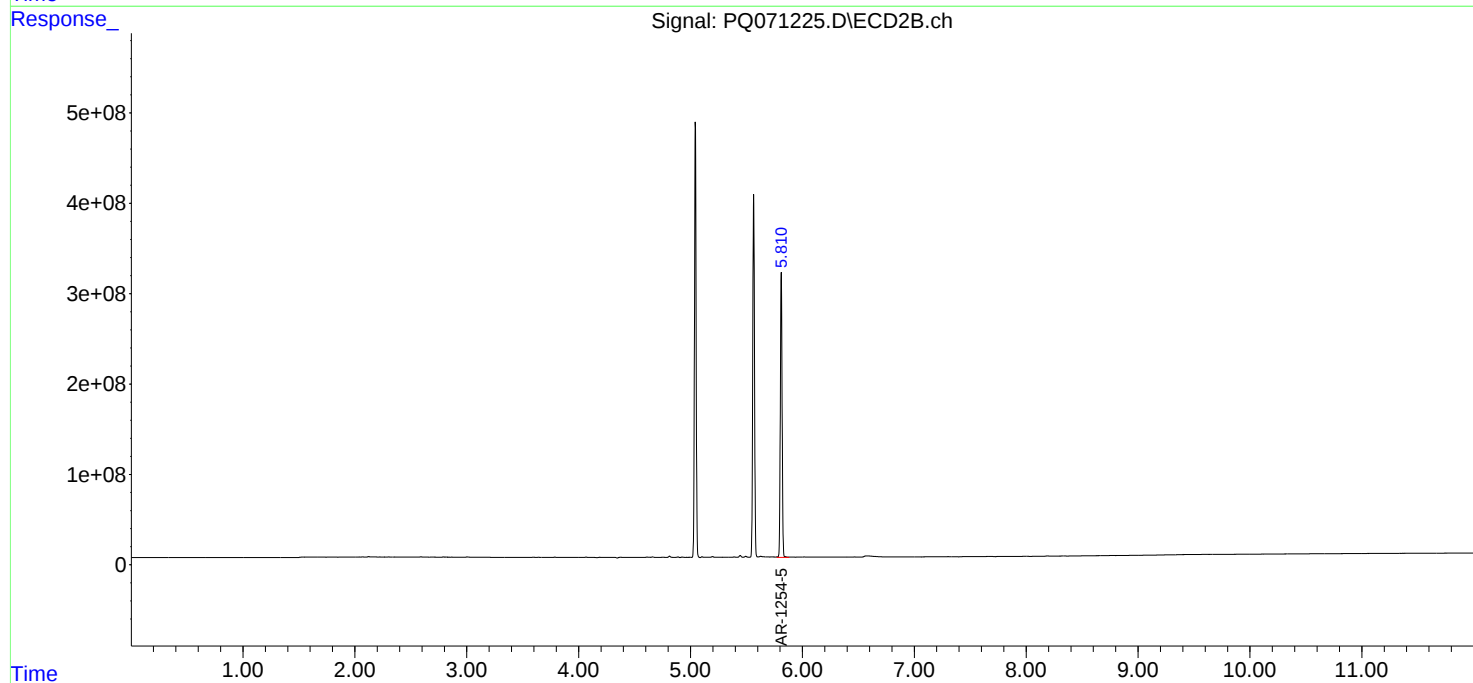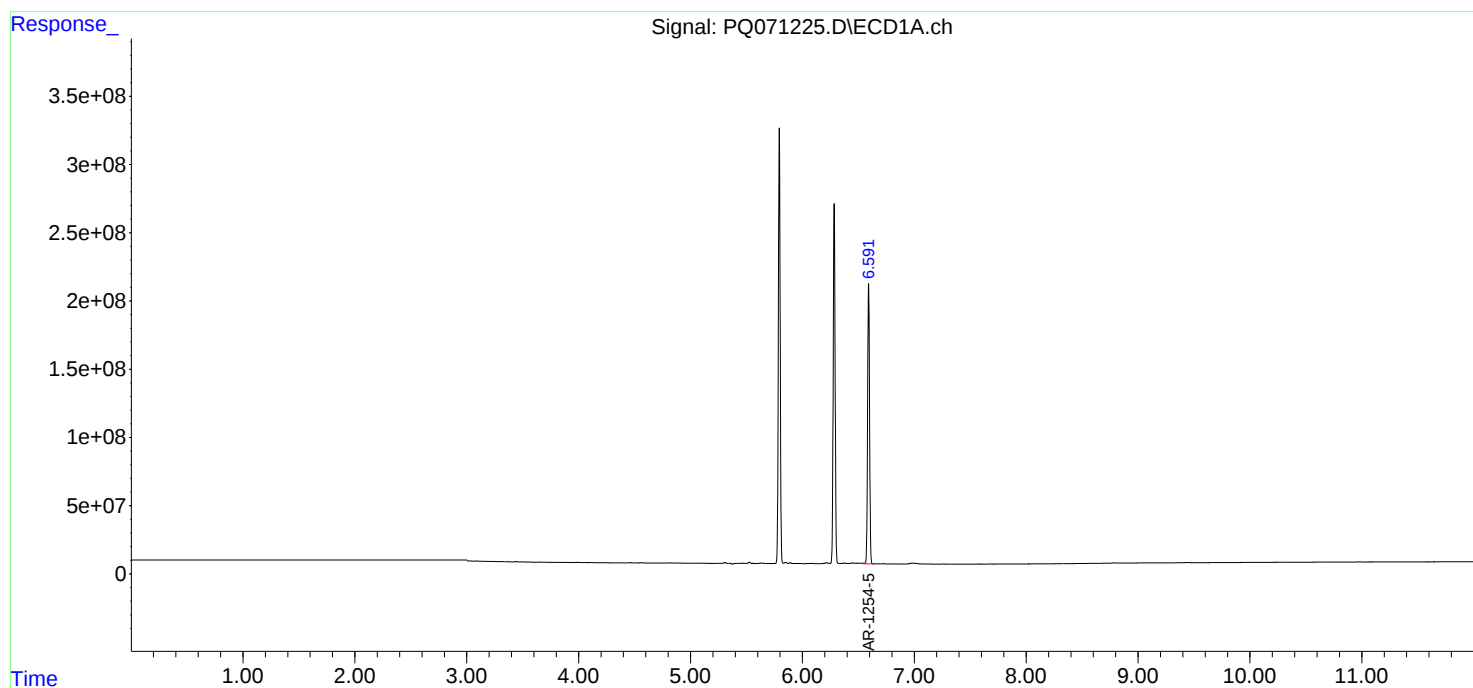


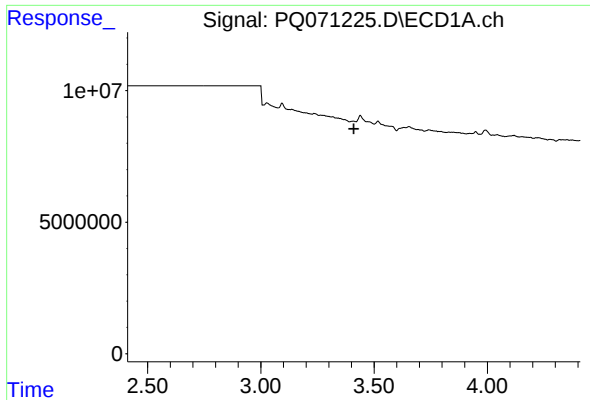

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

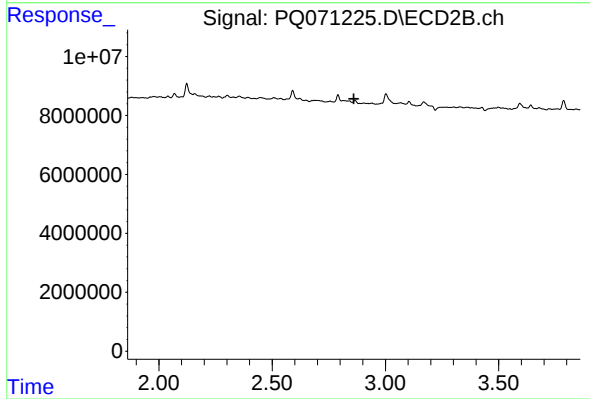


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.860 min
Response: 0
Conc: N.D.

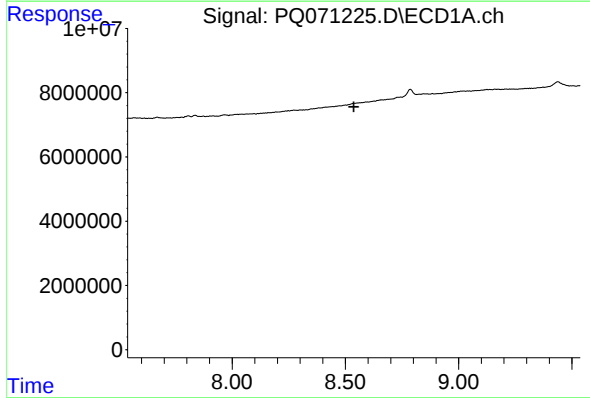


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.537 min
Response: 0
Conc: N.D.

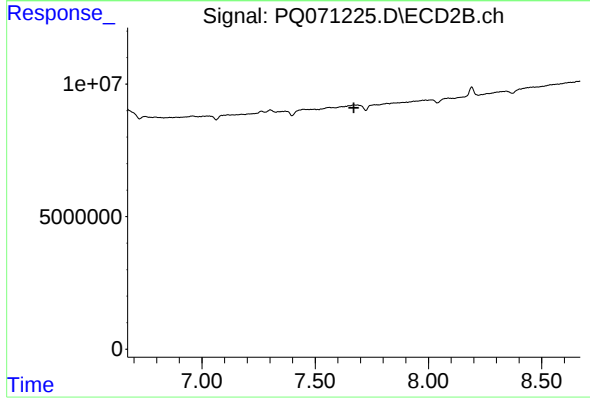

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 7.670 min
Response: 0
Conc: N.D.

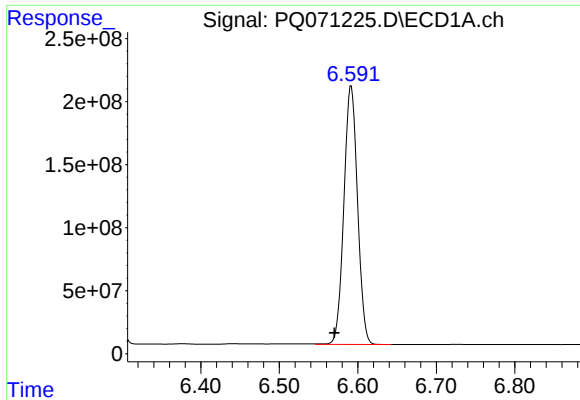

#30 AR-1254-5

R.T.: 6.592 min
Delta R.T.: 0.021 min
Response: 2476053546
Conc: 8637.15 ng/m

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

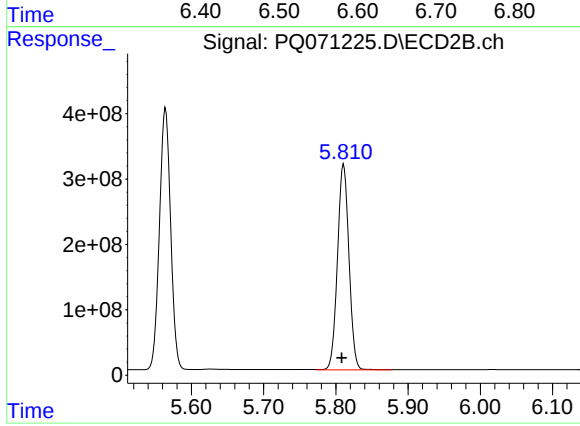

#30 AR-1254-5

R.T.: 5.811 min
Delta R.T.: 0.003 min
Response: 3483276494
Conc: 6624.29 ng/ml