

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110718\
 Data File : PQ034195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2018 15:34
 Operator : SM\SJ
 Sample : J5819-08RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 BES48_SB03_3.5-4.0RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 15:48:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 06 13:07:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.551	3.832	58271936	41336478	20.279	22.070
2) SA Decachlor...	10.361	8.865	19185573	14554033	6.310	6.321

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110718\
Data File : PQ034195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2018 15:34
Operator : SM\SJ
Sample : J5819-08RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
BES48_SB03_3.5-4.0RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 15:48:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 13:07:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

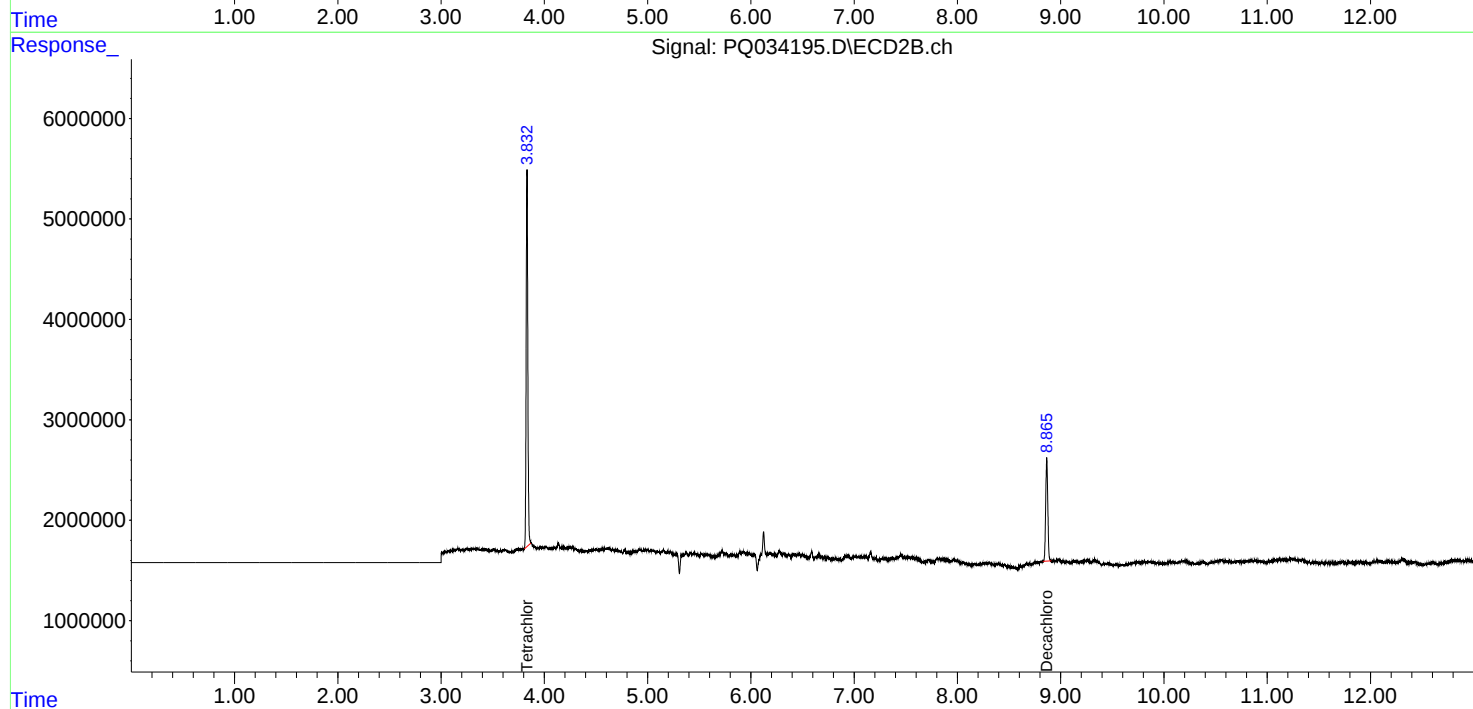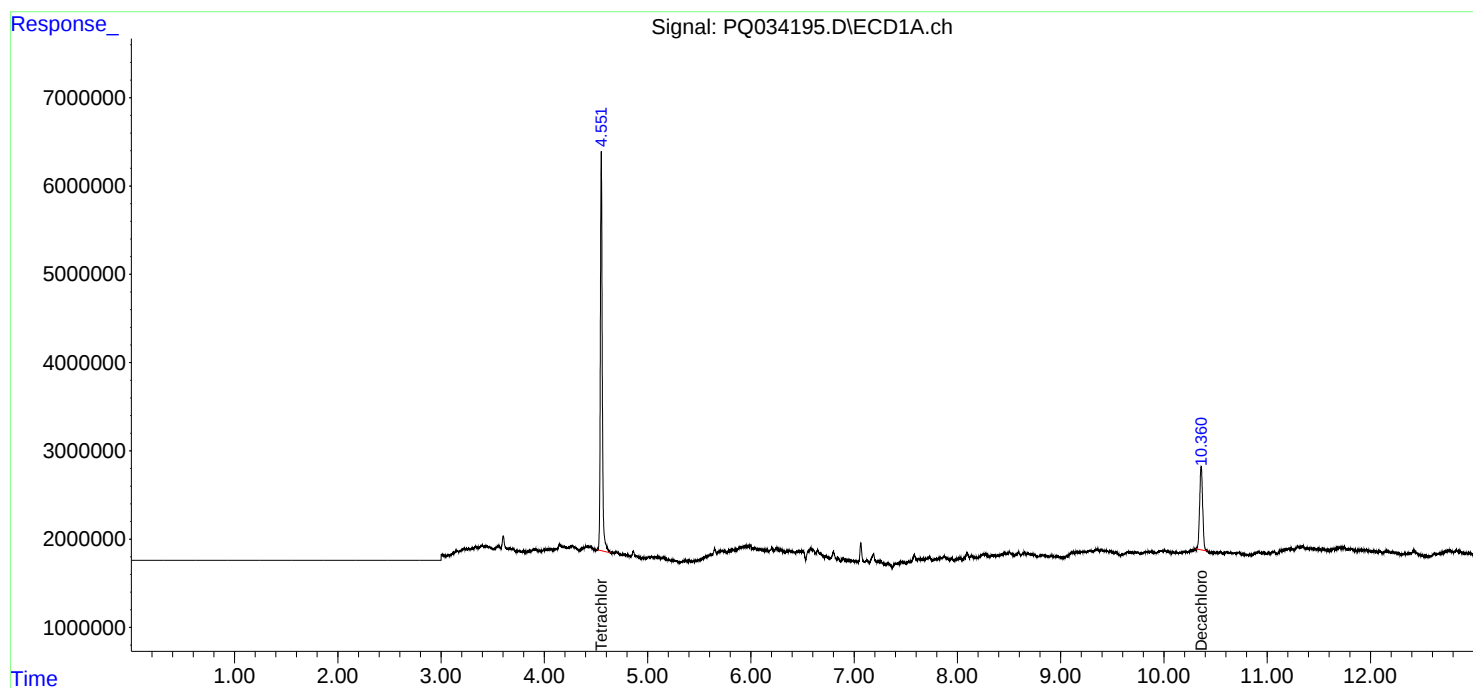


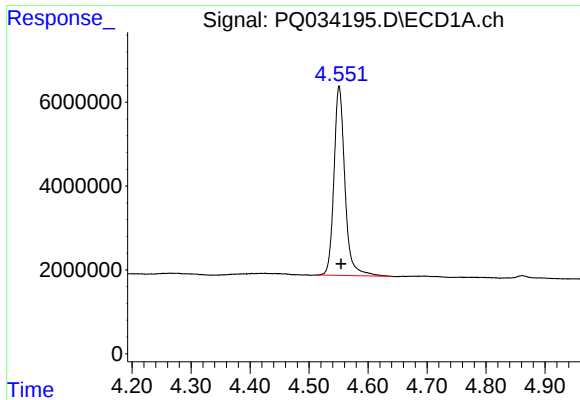

#1 Tetrachloro-m-xylene


R.T.: 4.551 min
Delta R.T.: -0.003 min
Response: 58271936
Conc: 20.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
BES48_SB03_3.5-4.0RE

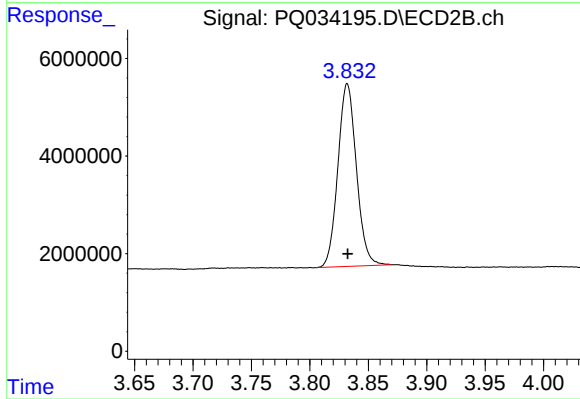


#1 Tetrachloro-m-xylene

R.T.: 3.832 min
Delta R.T.: 0.000 min
Response: 41336478
Conc: 22.07 ng/ml

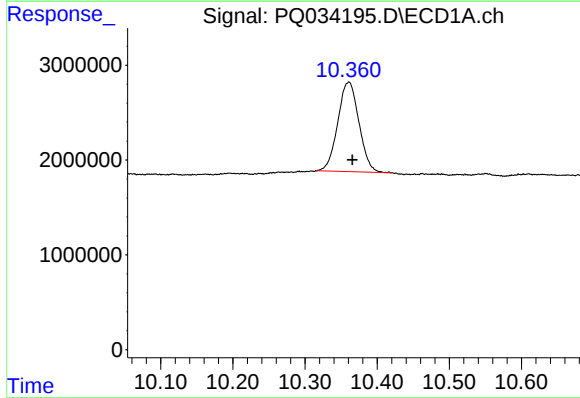

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.005 min
Response: 19185573
Conc: 6.31 ng/ml

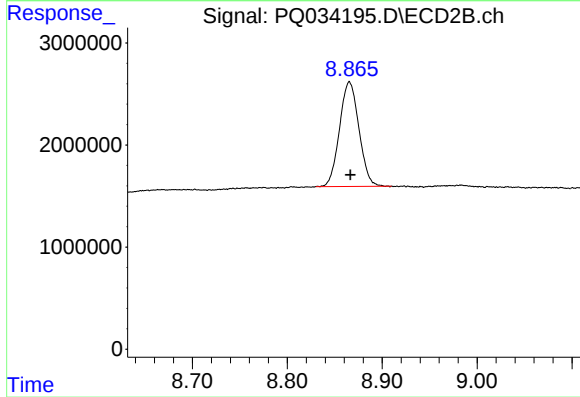

#2 Decachlorobiphenyl

R.T.: 8.865 min
Delta R.T.: -0.001 min
Response: 14554033
Conc: 6.32 ng/ml