

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
 Data File : PQ063838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2023 13:34
 Operator : YP\AJ
 Sample : 05284-05 10X
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 50167

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2023
 Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 14:21:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 18:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.461	2.768	2578166	5449572	0.605m	1.482m#
2) SA Decachlor...	8.696	7.565	485449	4312490	0.150m	0.920m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
Data File : PQ063838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2023 13:34
Operator : YP\AJ
Sample : 05284-05 10X
Misc :
ALS Vial : 75 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
50167


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 14:21:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 18:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

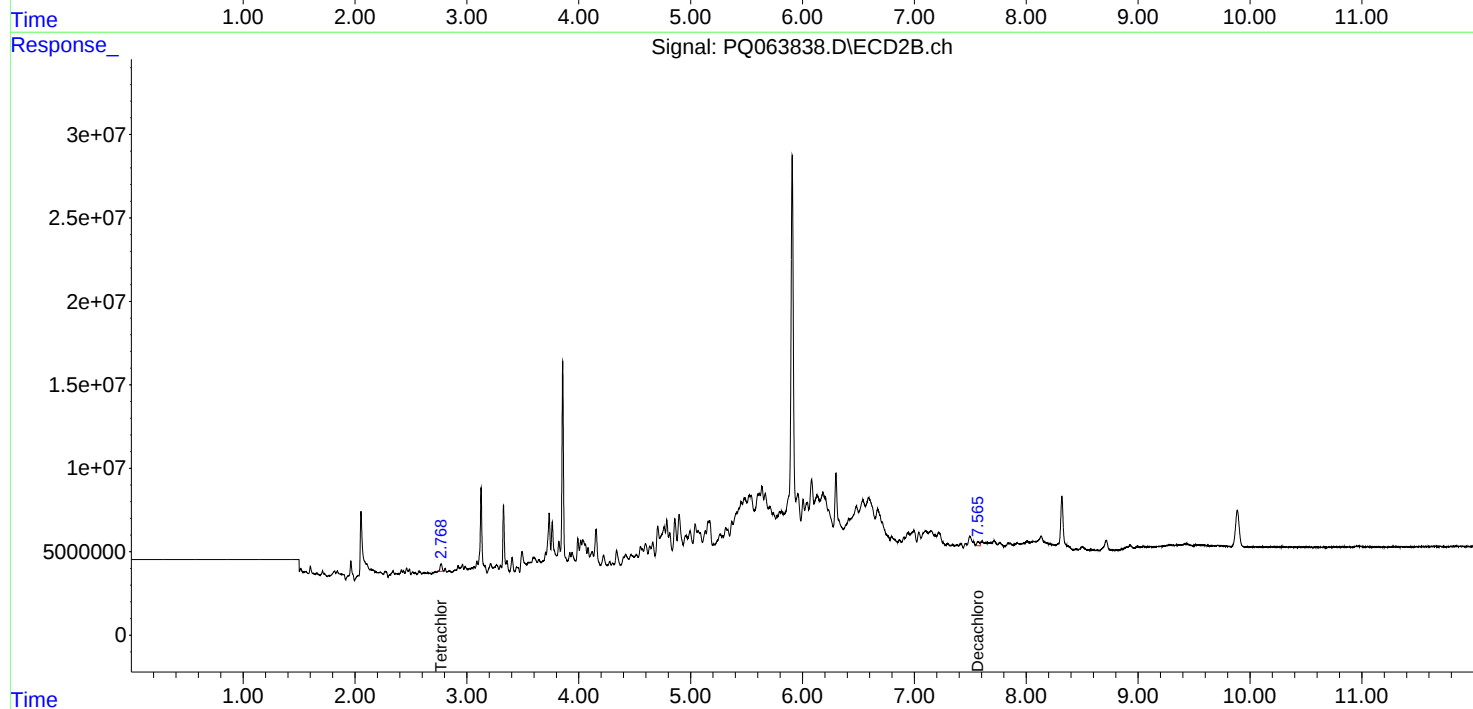

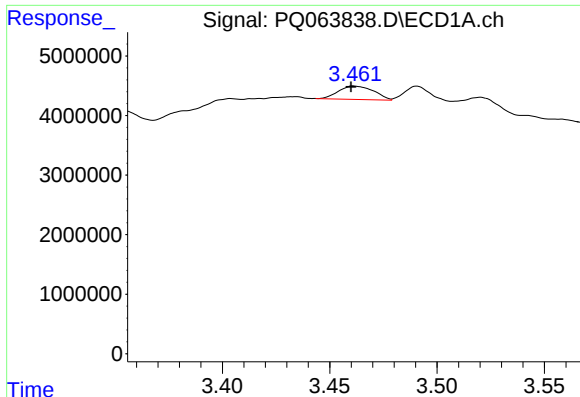


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 2578166
Conc: 0.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
50167


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

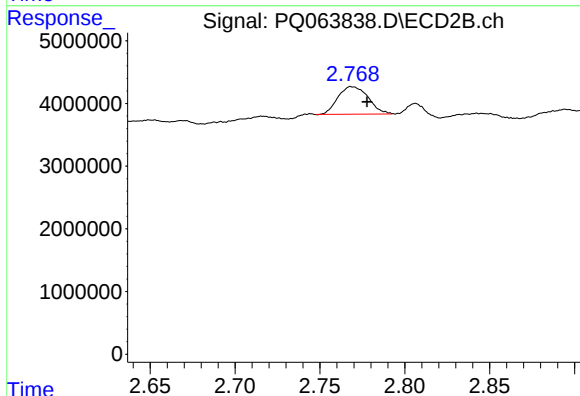


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.010 min
Response: 5449572
Conc: 1.48 ng/ml m

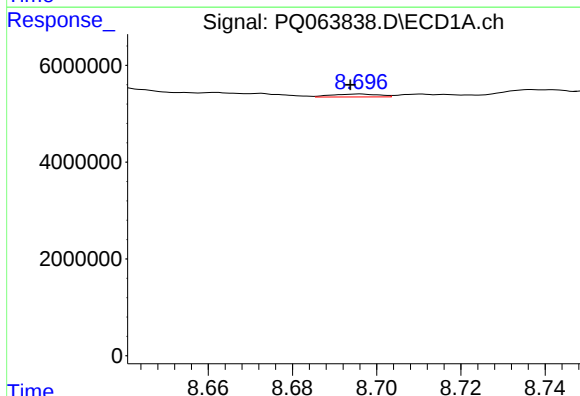

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: 0.002 min
Response: 485449
Conc: 0.15 ng/ml m

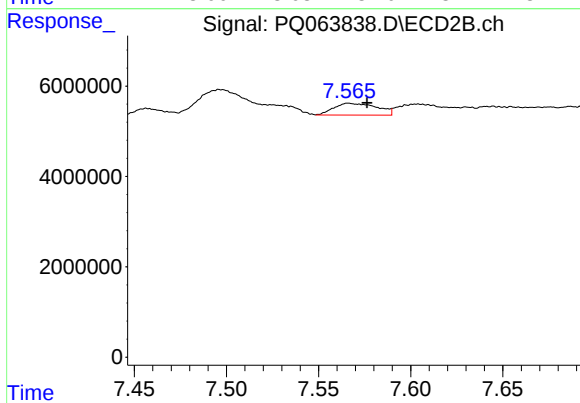

#2 Decachlorobiphenyl

R.T.: 7.565 min
Delta R.T.: -0.011 min
Response: 4312490
Conc: 0.92 ng/ml m