

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
 Data File : PQ063853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2023 17:15
 Operator : YP\AJ
 Sample : 05312-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 P-4(170FT)(5-10)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2023
 Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 08:29:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 18:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	2.777	66739224	66051820	15.657m	17.960
2) SA Decachlor...	8.694	7.576	59671677	68208022	18.482m	14.558

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
Data File : PQ063853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2023 17:15
Operator : YP\AJ
Sample : 05312-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
P-4(170FT)(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 08:29:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 18:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

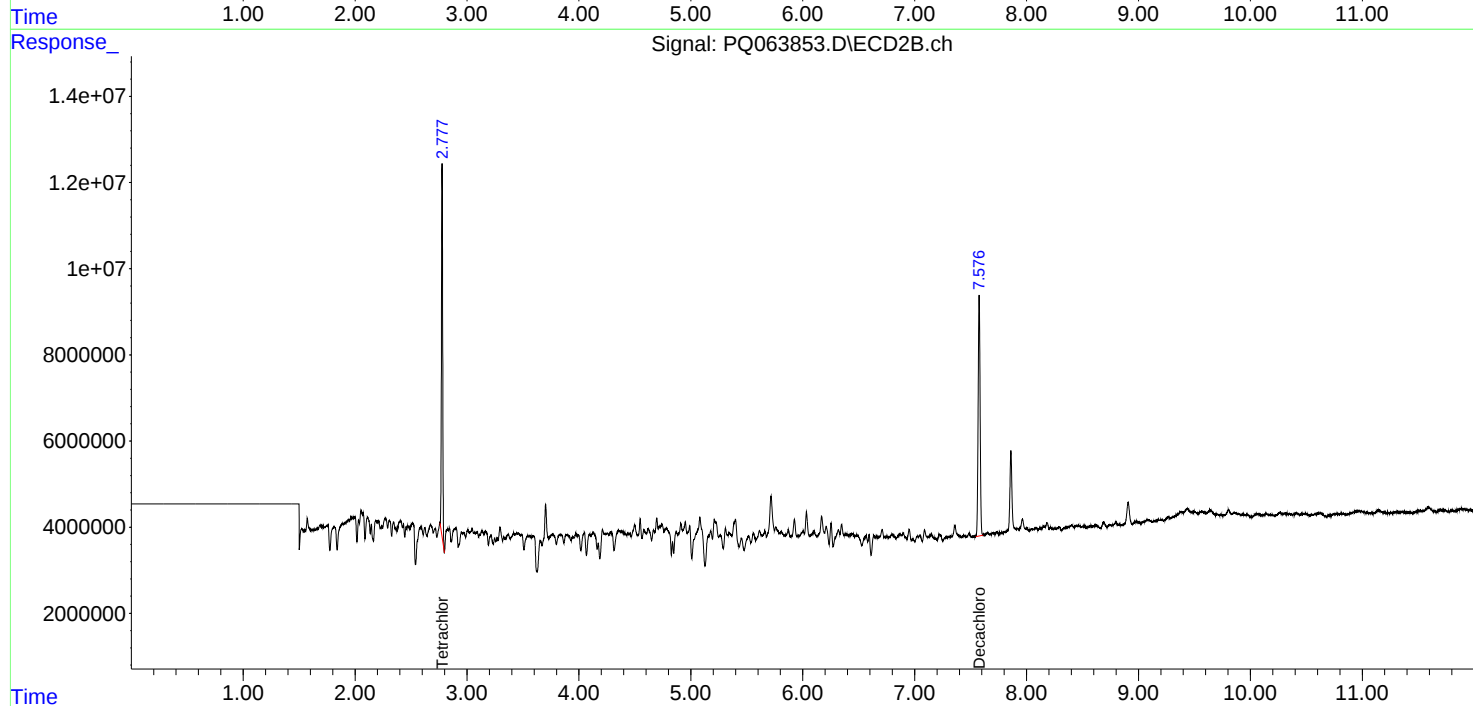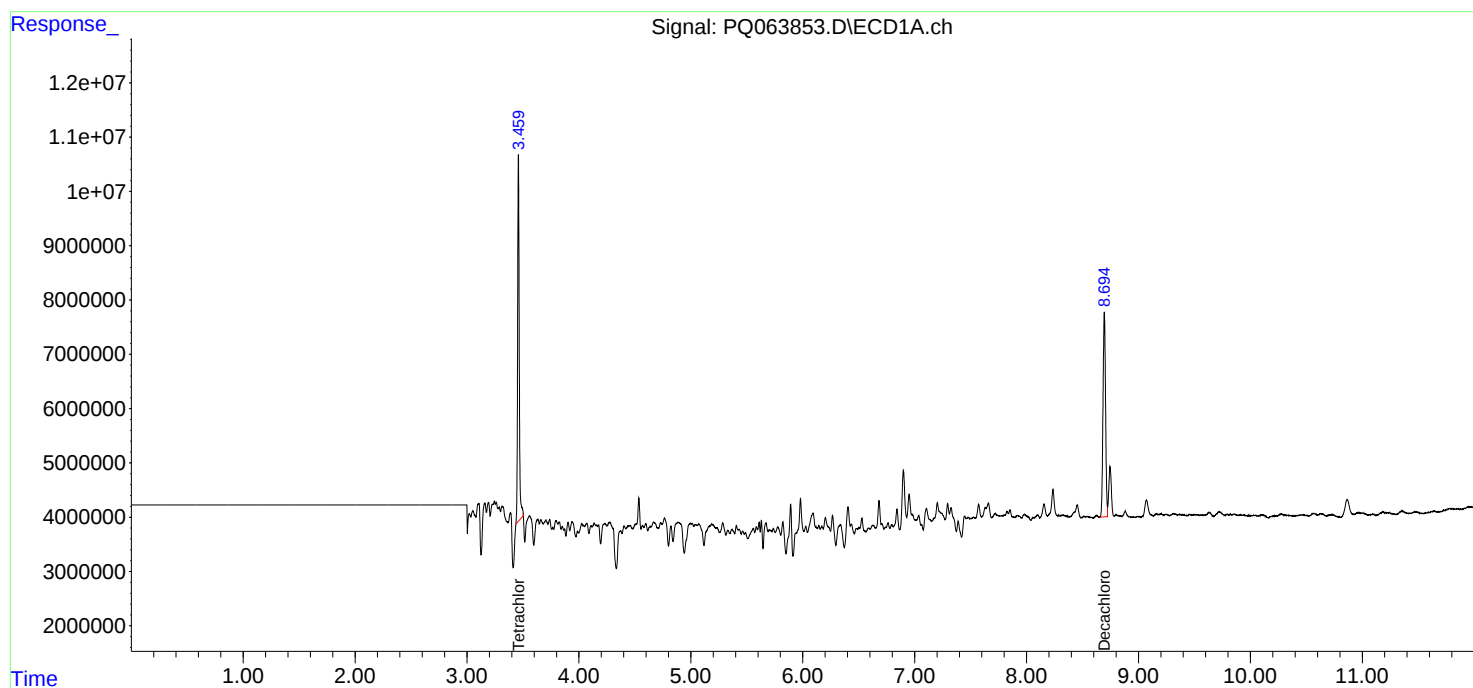

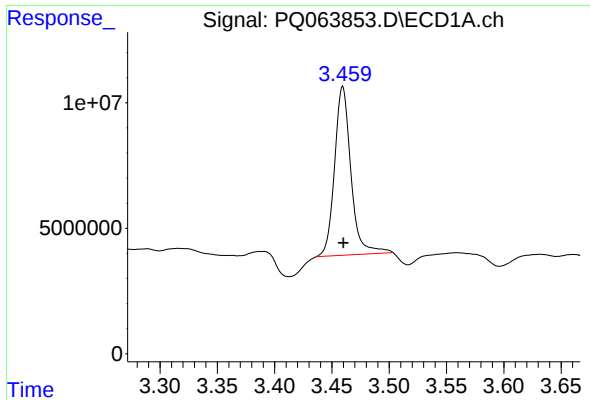


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 66739224
Conc: 15.66 ng/ml

Instrument :
ECD_Q
ClientSampleId :
P-4(170FT)(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

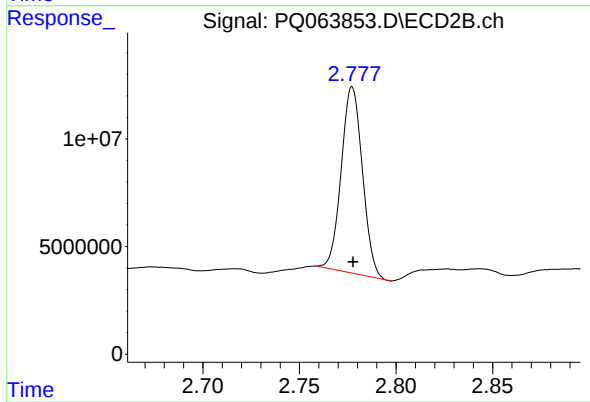


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 66051820
Conc: 17.96 ng/ml

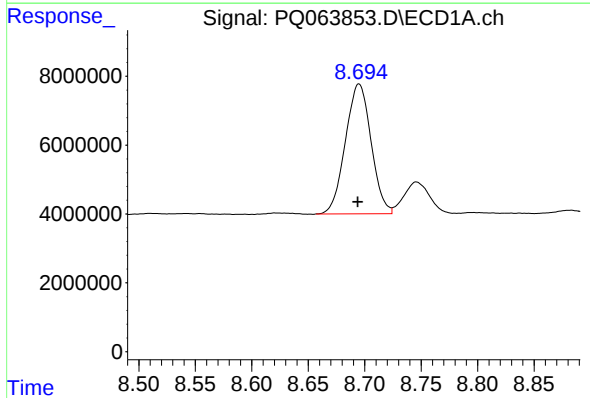

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 59671677
Conc: 18.48 ng/ml m

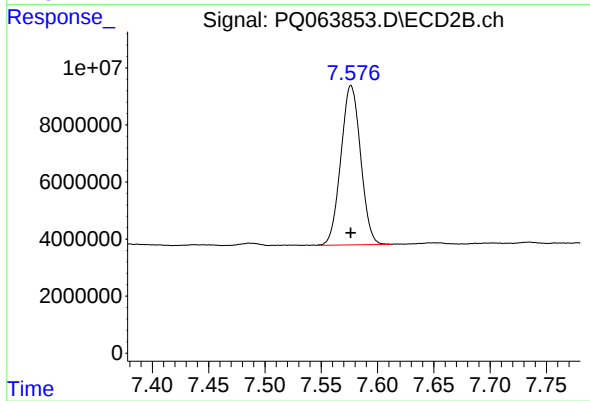

#2 Decachlorobiphenyl

R.T.: 7.576 min
Delta R.T.: 0.000 min
Response: 68208022
Conc: 14.56 ng/ml