

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
 Data File : PQ063876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2023 23:08
 Operator : YP\AJ
 Sample : 05322-07 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 HEF218I-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2023
 Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 00:41:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 18:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	2.778	6610884	7092638	1.551m	1.929
2) SA Decachlor...	8.692	7.575	5225591	7502108	1.619	1.601

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
Data File : PQ063876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2023 23:08
Operator : YP\AJ
Sample : 05322-07 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
HEF218I-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 00:41:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 18:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

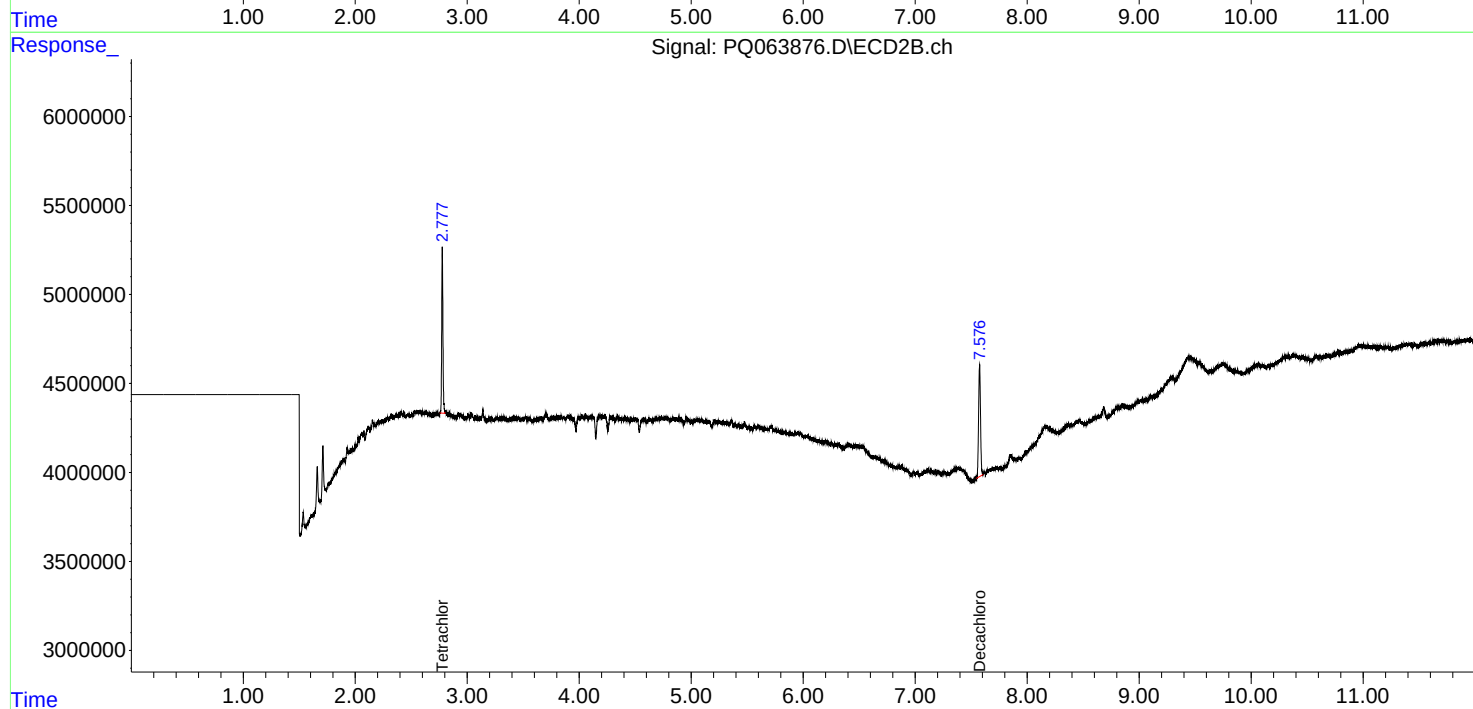

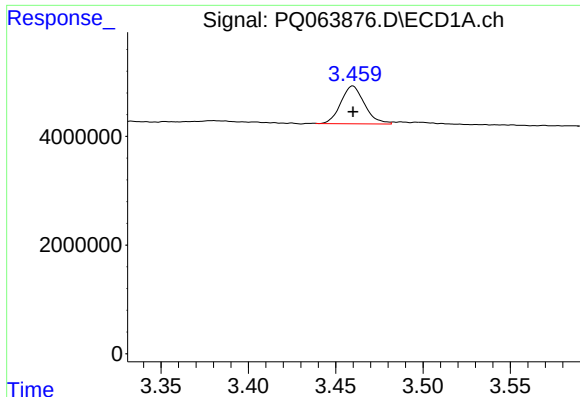


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 6610884
Conc: 1.55 ng/ml

Instrument :
ECD_Q
ClientSampleId :
HEF218I-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

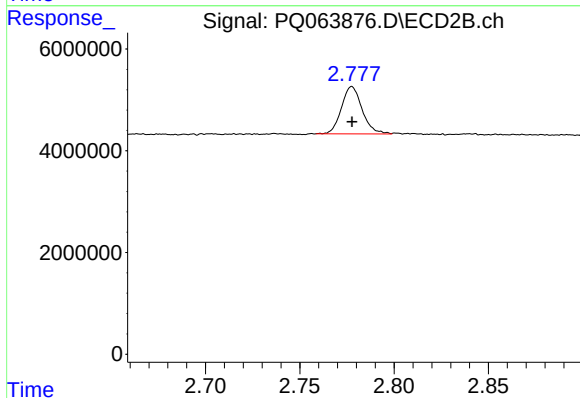


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 7092638
Conc: 1.93 ng/ml

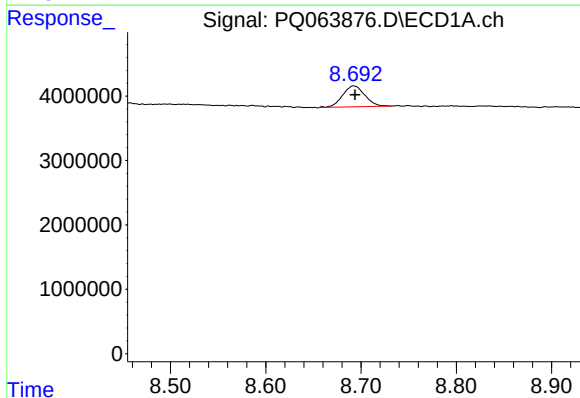

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.001 min
Response: 5225591
Conc: 1.62 ng/ml

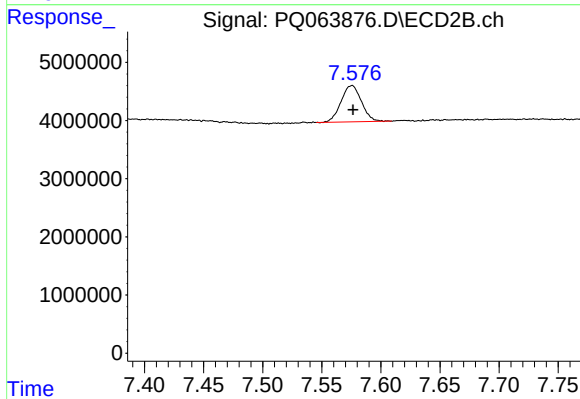

#2 Decachlorobiphenyl

R.T.: 7.575 min
Delta R.T.: 0.000 min
Response: 7502108
Conc: 1.60 ng/ml