

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
 Data File : PQ063904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2023 06:58
 Operator : YP\AJ
 Sample : 05311-13
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2023
 Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 07:42:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 18:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.460	2.777	70830839	68941247	16.617	18.746
2) SA Decachlor...	8.690	7.573	35217916	53354378	10.908m	11.387

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ110923\
Data File : PQ063904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2023 06:58
Operator : YP\AJ
Sample : 05311-13
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 07:42:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 18:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

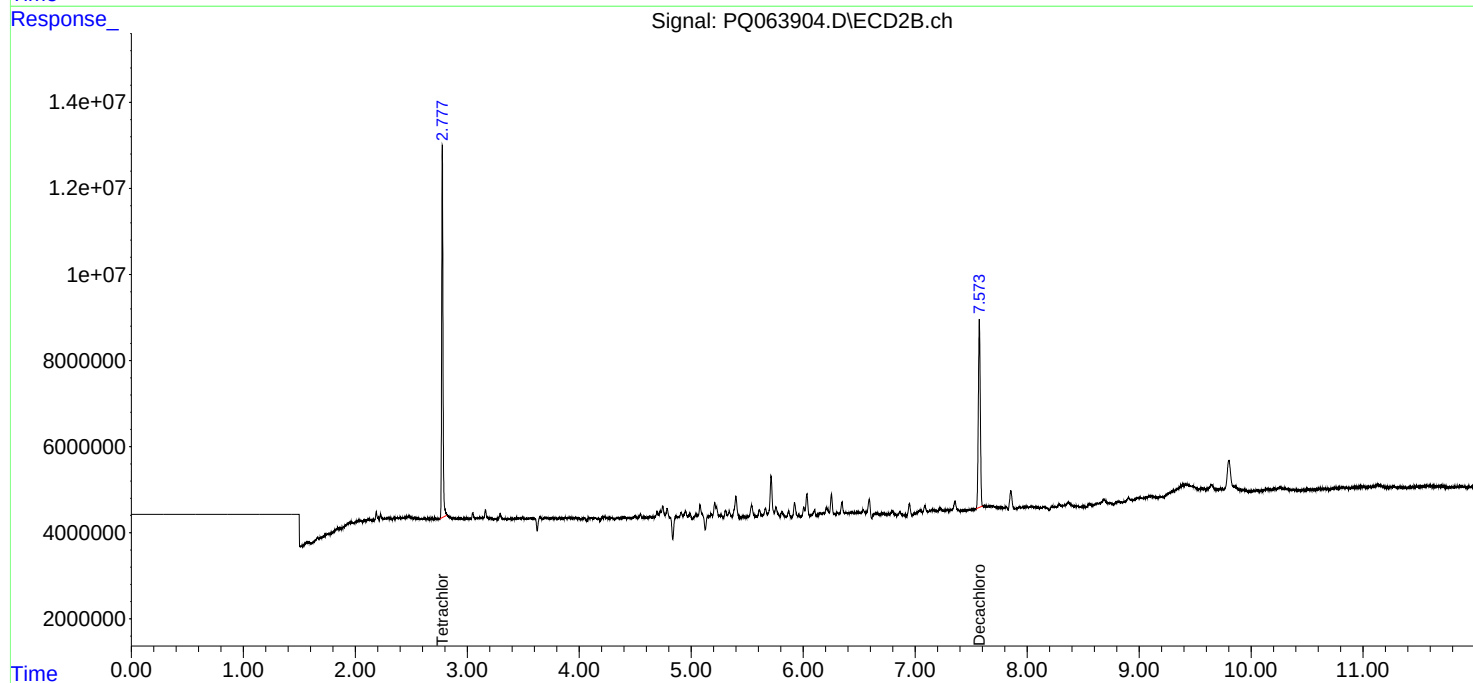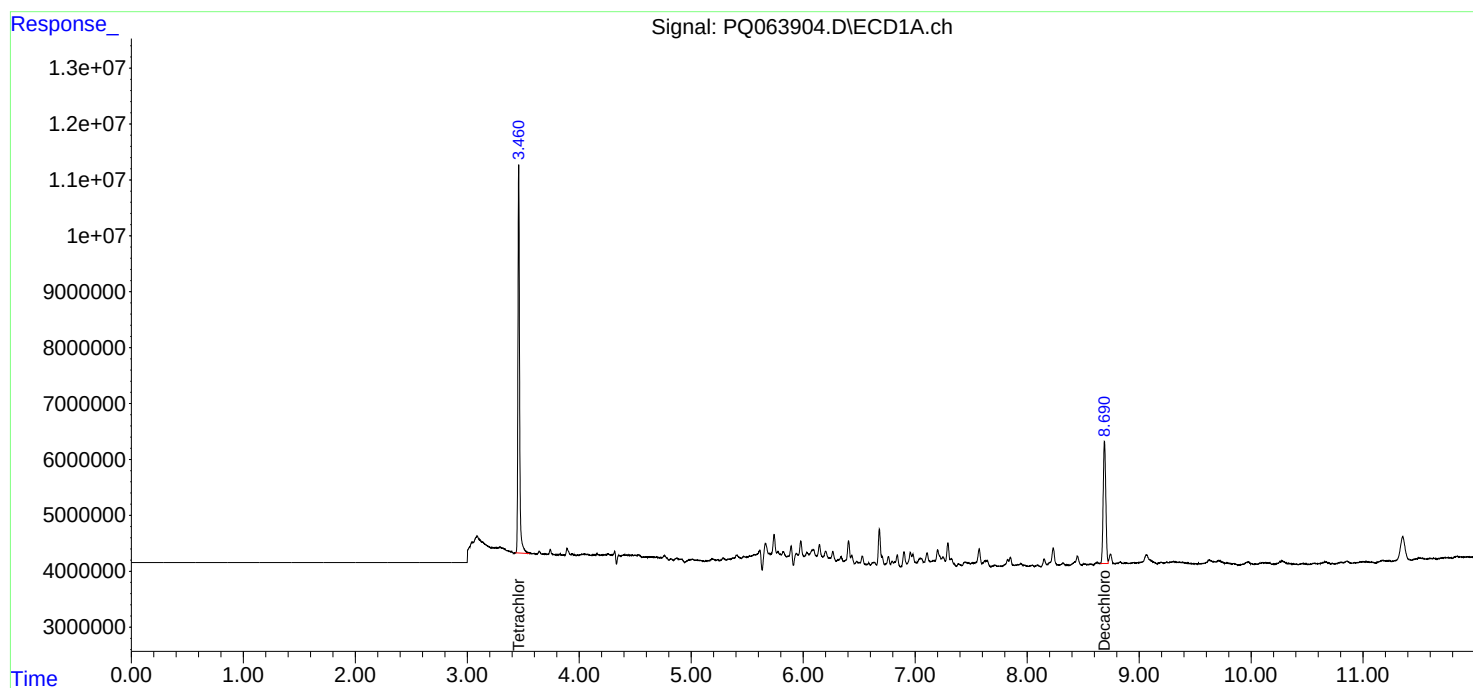

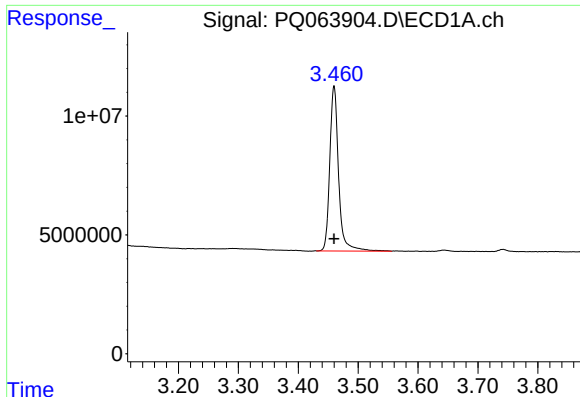


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 70830839
Conc: 16.62 ng/ml

Instrument :
ECD_Q
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

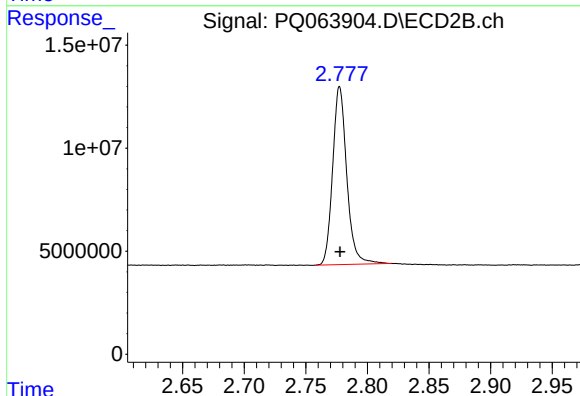


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 68941247
Conc: 18.75 ng/ml

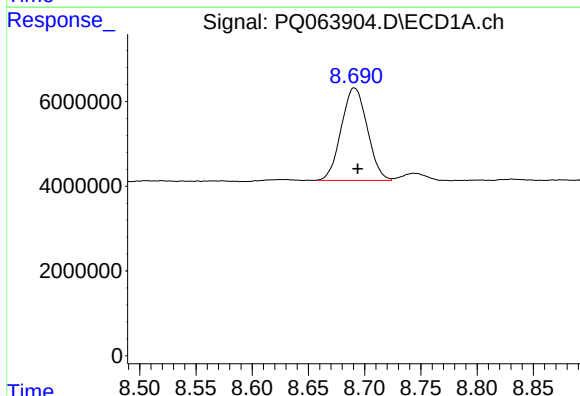

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.004 min
Response: 35217916
Conc: 10.91 ng/ml m

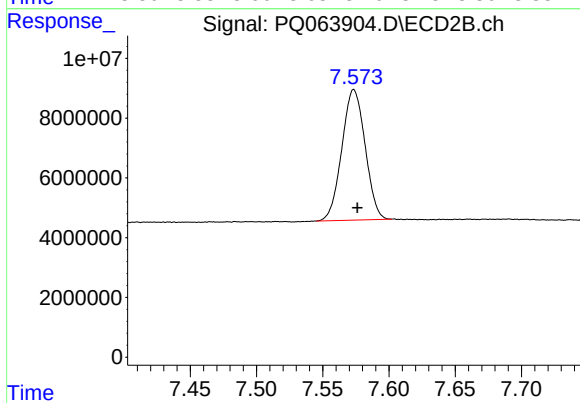

#2 Decachlorobiphenyl

R.T.: 7.573 min
Delta R.T.: -0.003 min
Response: 53354378
Conc: 11.39 ng/ml