

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ111323\
 Data File : PQ064012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2023 13:10
 Operator : YP\AJ
 Sample : 05310-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATERE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :Ankita Jodhani 11/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 13:58:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 18:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.463	2.777	40347568	40023652	9.466	10.883m
2) SA Decachlor...	8.696	7.574	50678078	76323541	15.696	16.290

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ111323\
Data File : PQ064012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2023 13:10
Operator : YP\AJ
Sample : 05310-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SEMI-ANNUAL-CONDENSATERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :Ankita Jodhani 11/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 13:58:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 18:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

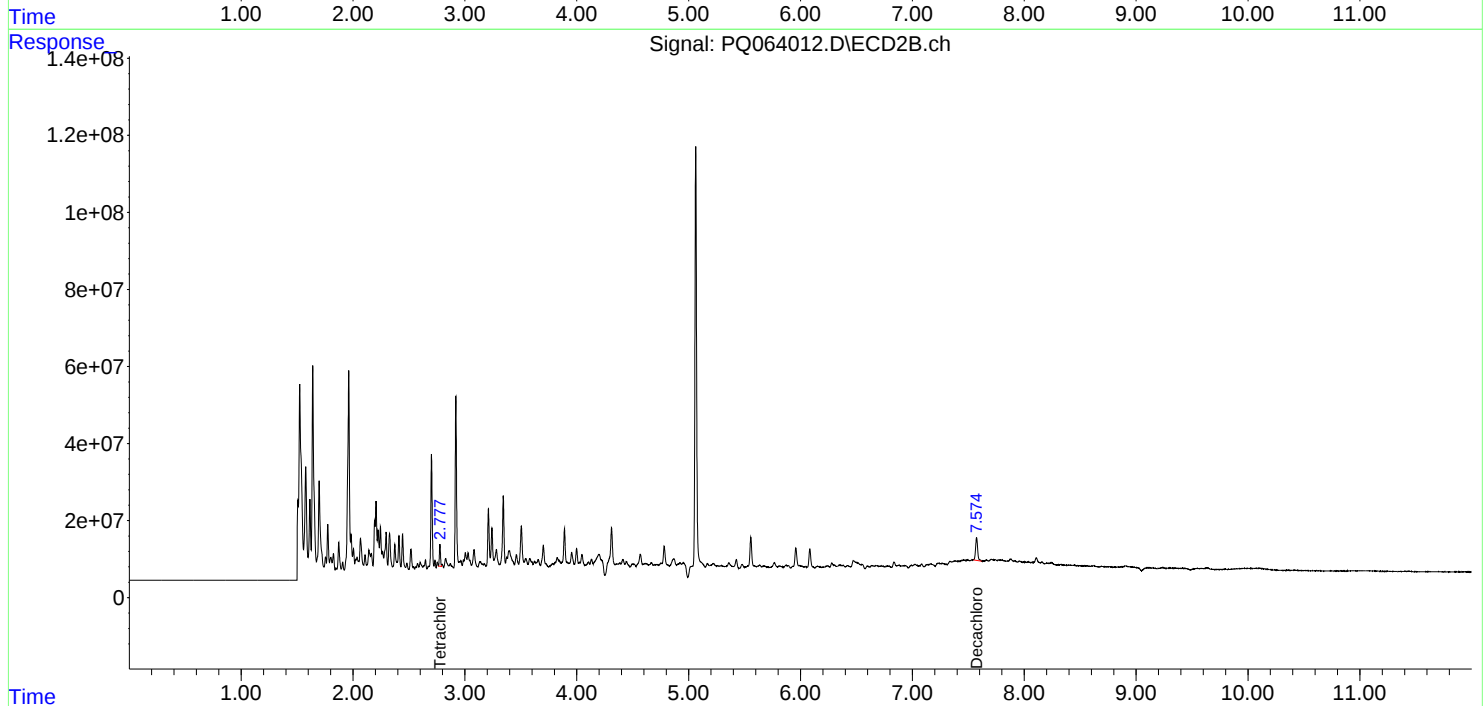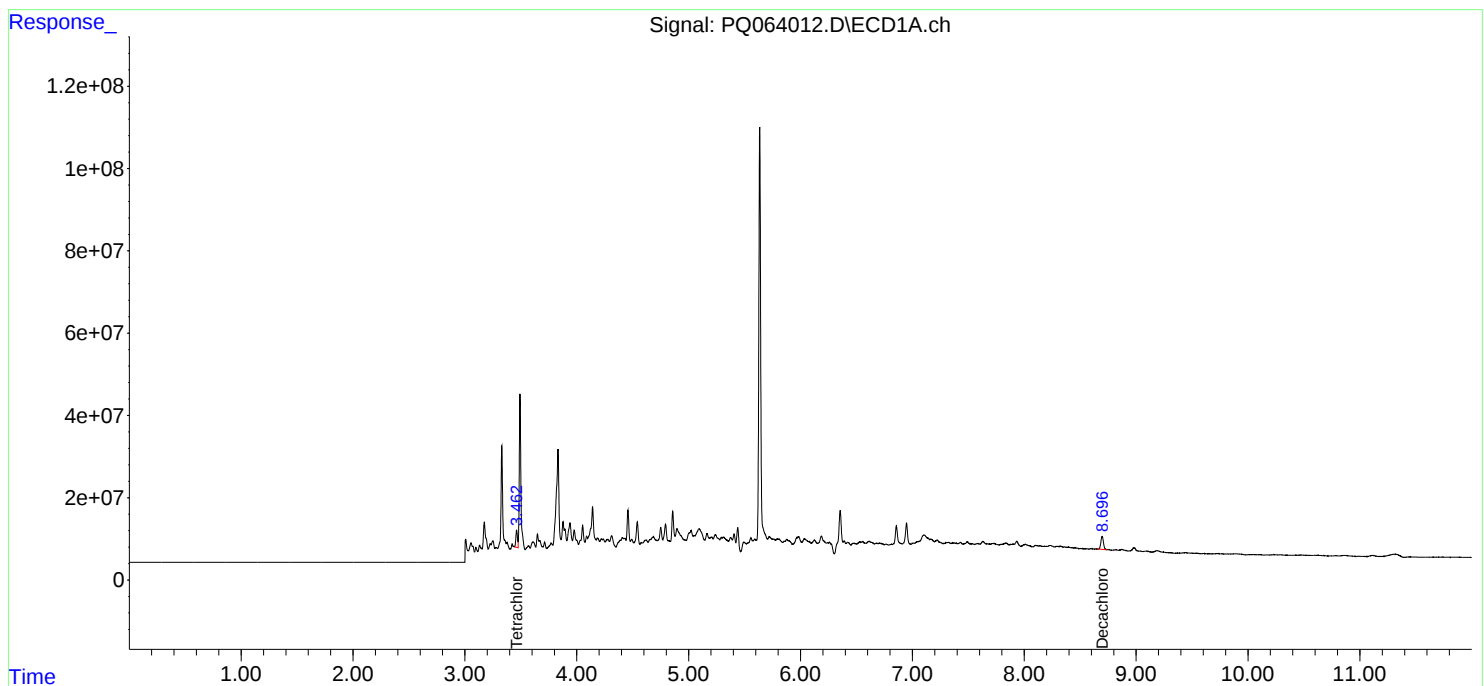

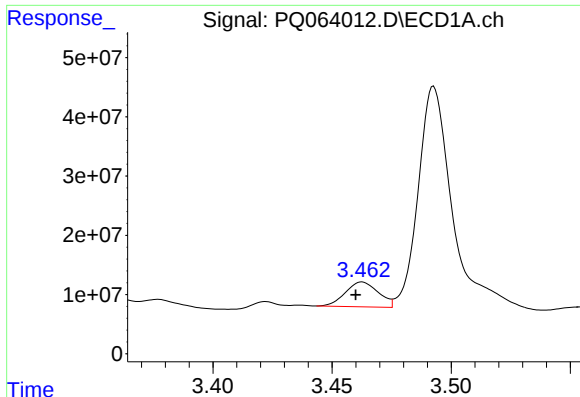


#1 Tetrachloro-m-xylene

R.T.: 3.463 min
Delta R.T.: 0.003 min
Response: 40347568
Conc: 9.47 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SEMI-ANNUAL-CONDENSATERE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :Ankita Jodhani 11/14/2023

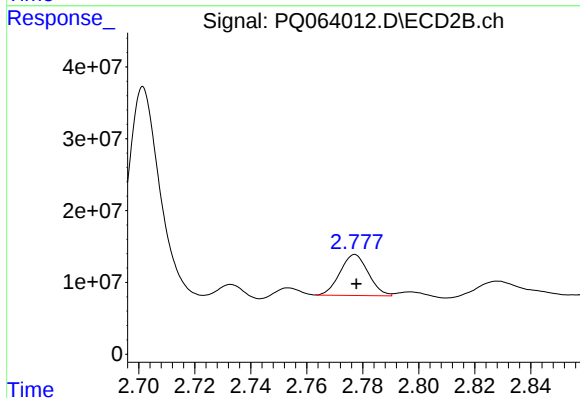


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 40023652
Conc: 10.88 ng/ml m

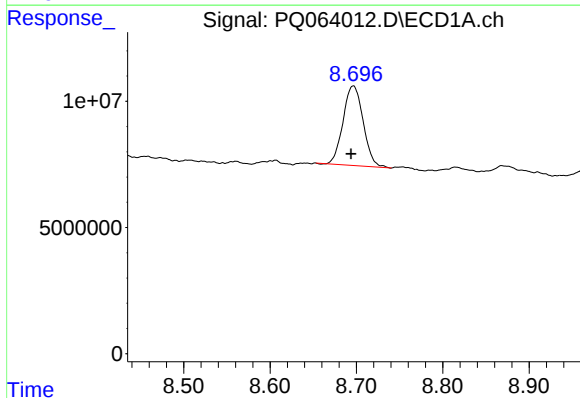

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: 0.003 min
Response: 50678078
Conc: 15.70 ng/ml

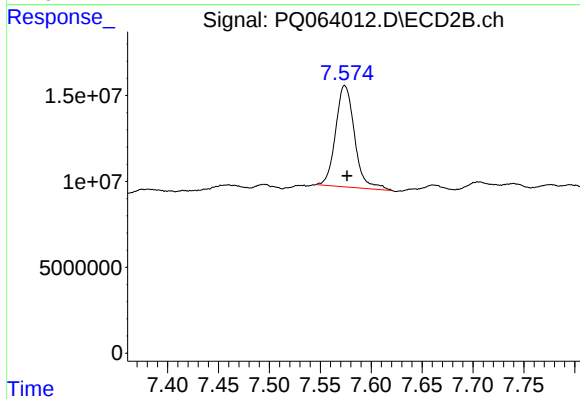

#2 Decachlorobiphenyl

R.T.: 7.574 min
Delta R.T.: -0.002 min
Response: 76323541
Conc: 16.29 ng/ml