

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111925AL\
Data File : FE056923.D
Signal(s) : FID1B.ch
Acq On : 19 Nov 2025 07:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 14:21:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Tue Nov 18 13:37:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.942	112072	0.570 ug/ml
19) T	n-Tetratriacontane (C34)	19.728	97436	0.564 ug/ml
20) T	n-Hexatriacontane (C36)	20.469	61938	0.428 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111925AL\
Data File : FE056923.D
Signal(s) : FID1B.ch
Acq On : 19 Nov 2025 07:04
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 14:21:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Tue Nov 18 13:37:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

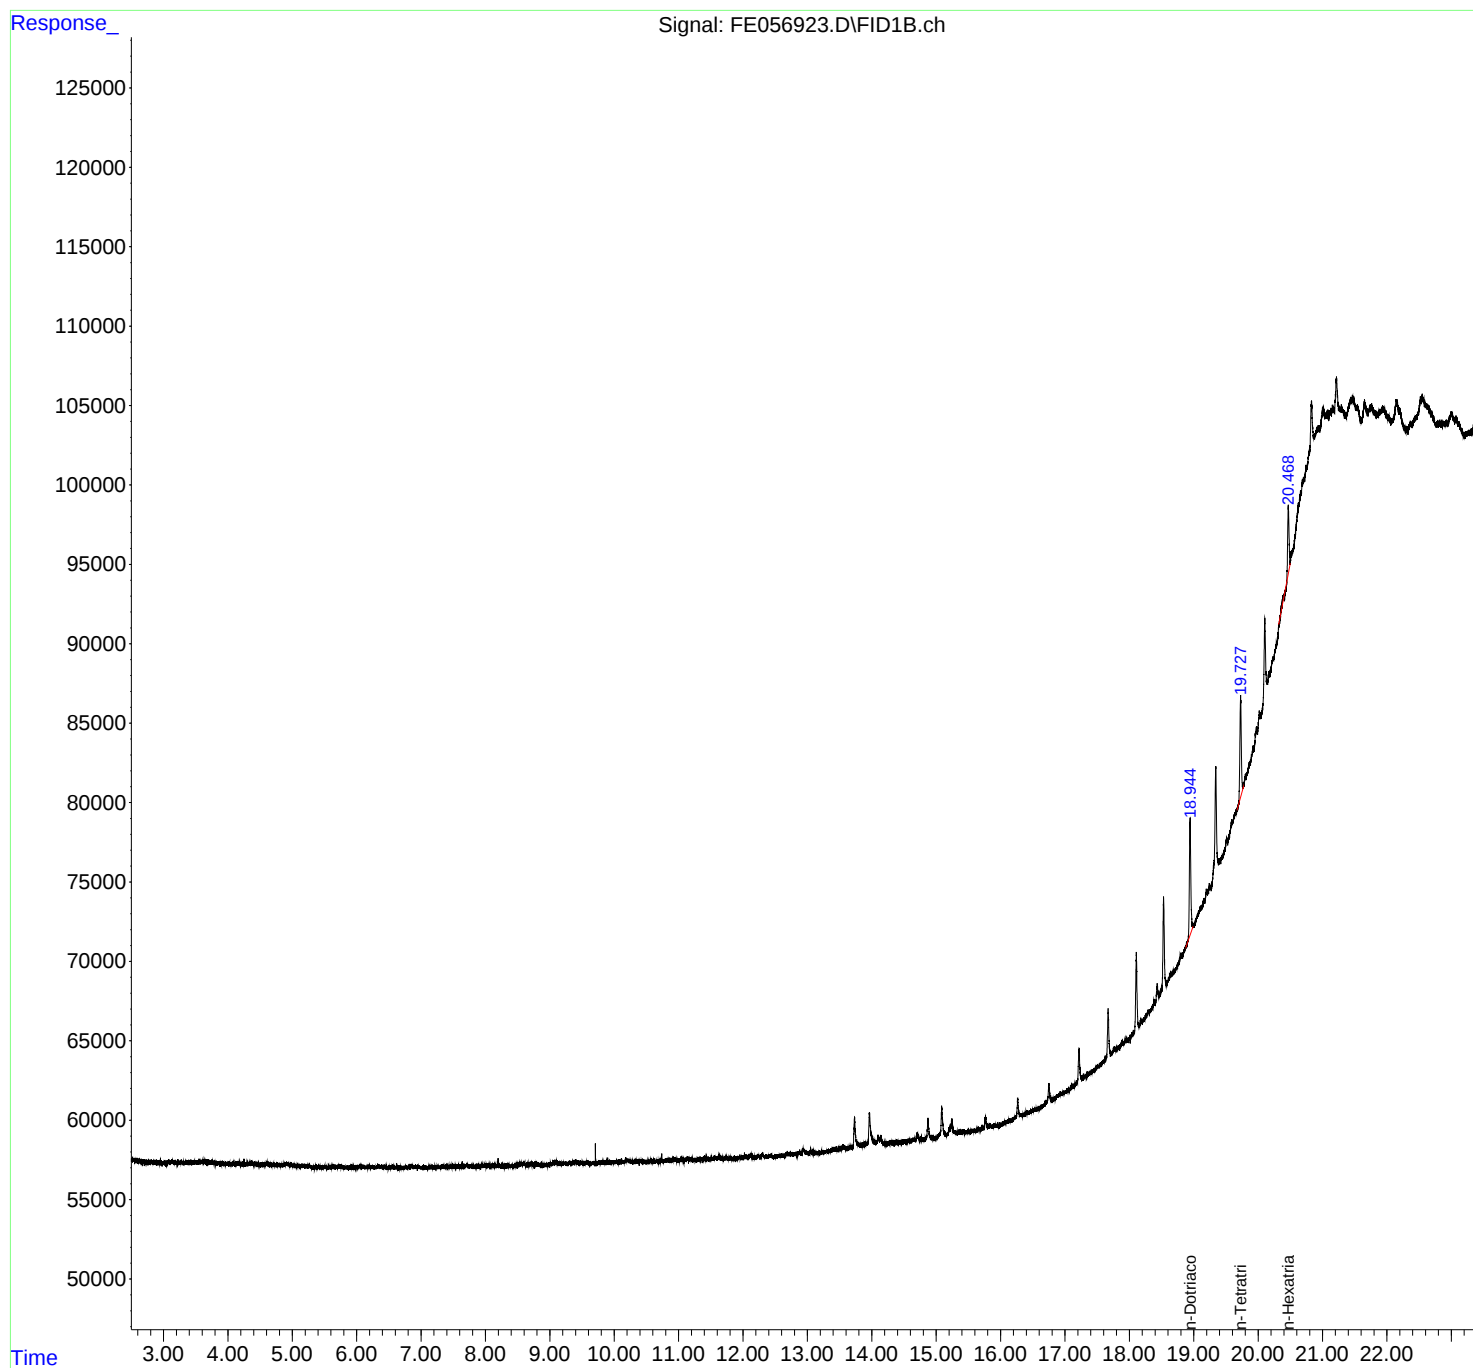


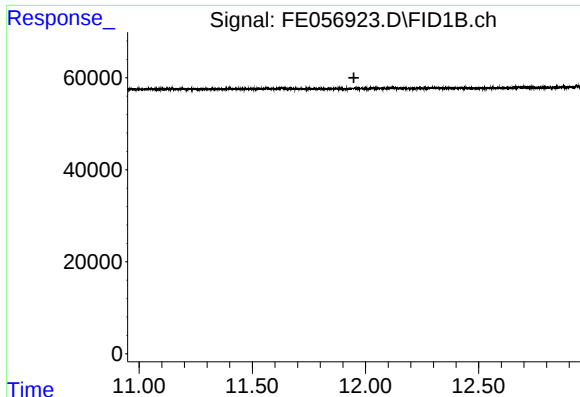

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

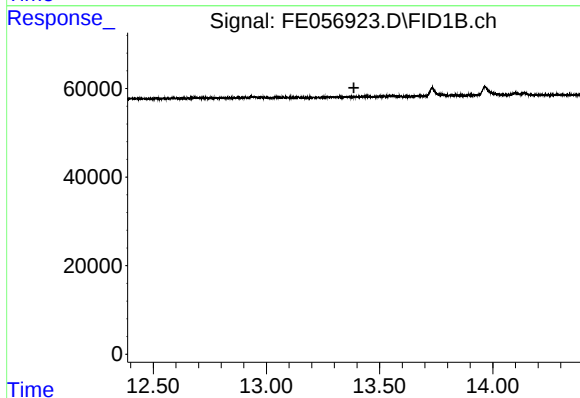


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.386 min
Response: 0
Conc: N.D.

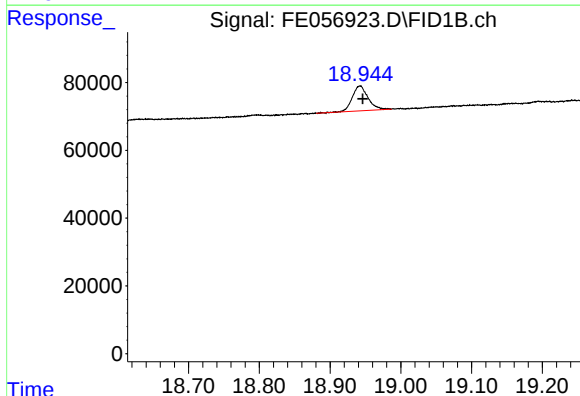


#18 n-Dotriacontane (C32)

R.T.: 18.942 min
Delta R.T.: -0.004 min
Response: 112072
Conc: 0.57 ug/ml

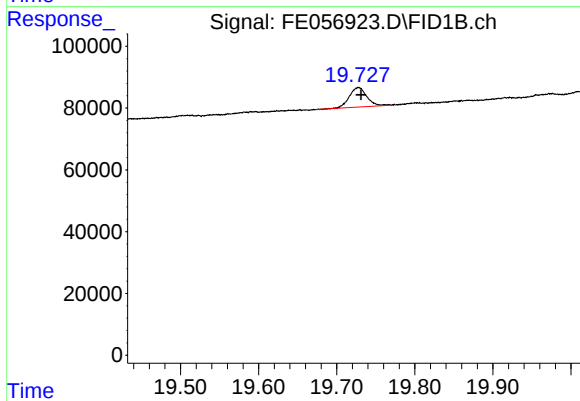

#19 n-Tetratriacontane (C34)

R.T.: 19.728 min
Delta R.T.: -0.003 min
Response: 97436
Conc: 0.56 ug/ml

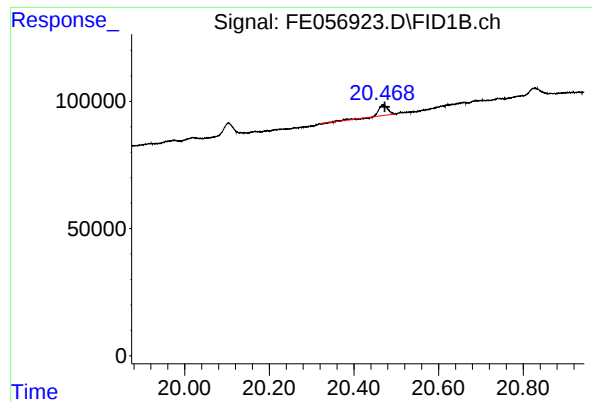

#20 n-Hexatriacontane (C36)

R.T.: 20.469 min
Delta R.T.: -0.003 min
Response: 61938
Conc: 0.43 ug/ml

Instrument :
ECD_Q
ClientSampleId :