

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ111825\
 Data File : PQ071330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2025 11:33
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 06:45:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 19 04:02:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30) L6 AR-1254-5	6.591	5.803	3581.9E6	4964.7E6	7793.055	7172.087



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ111825\
Data File : PQ071330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2025 11:33
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 06:45:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 19 04:02:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

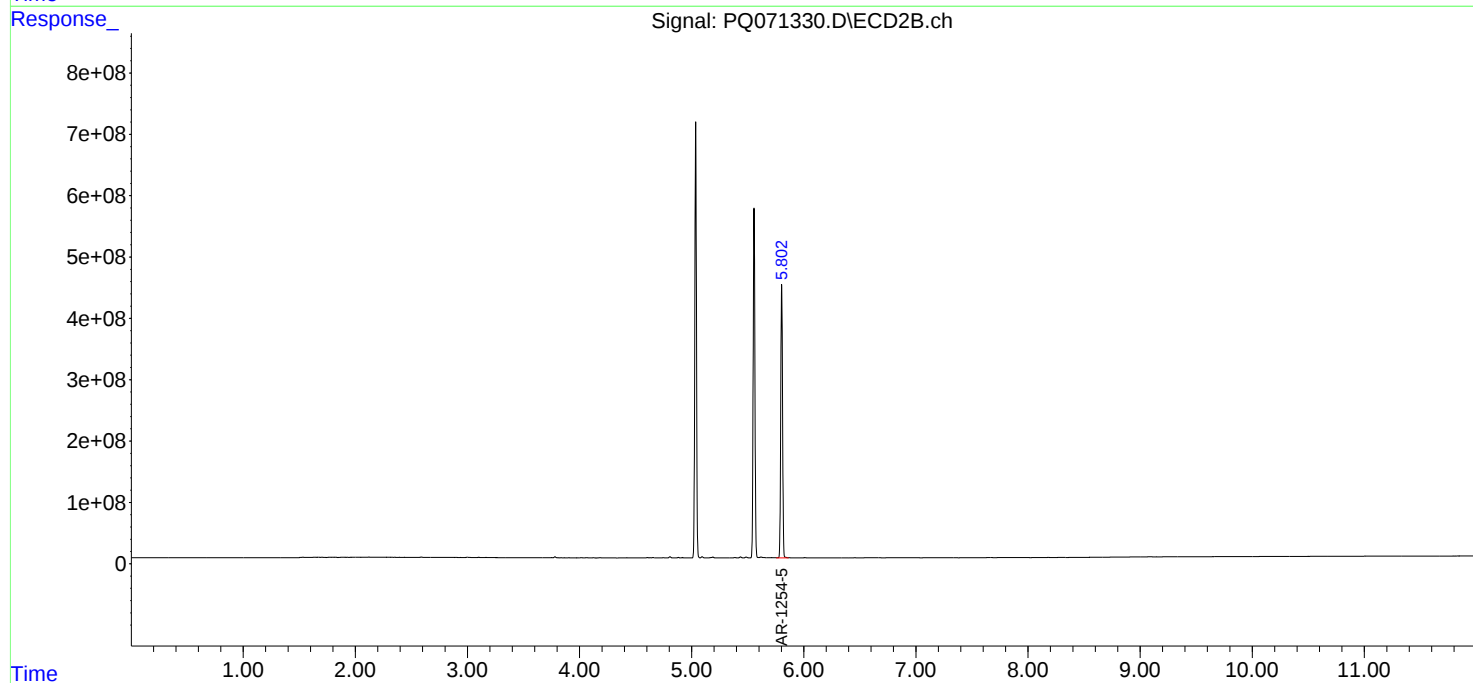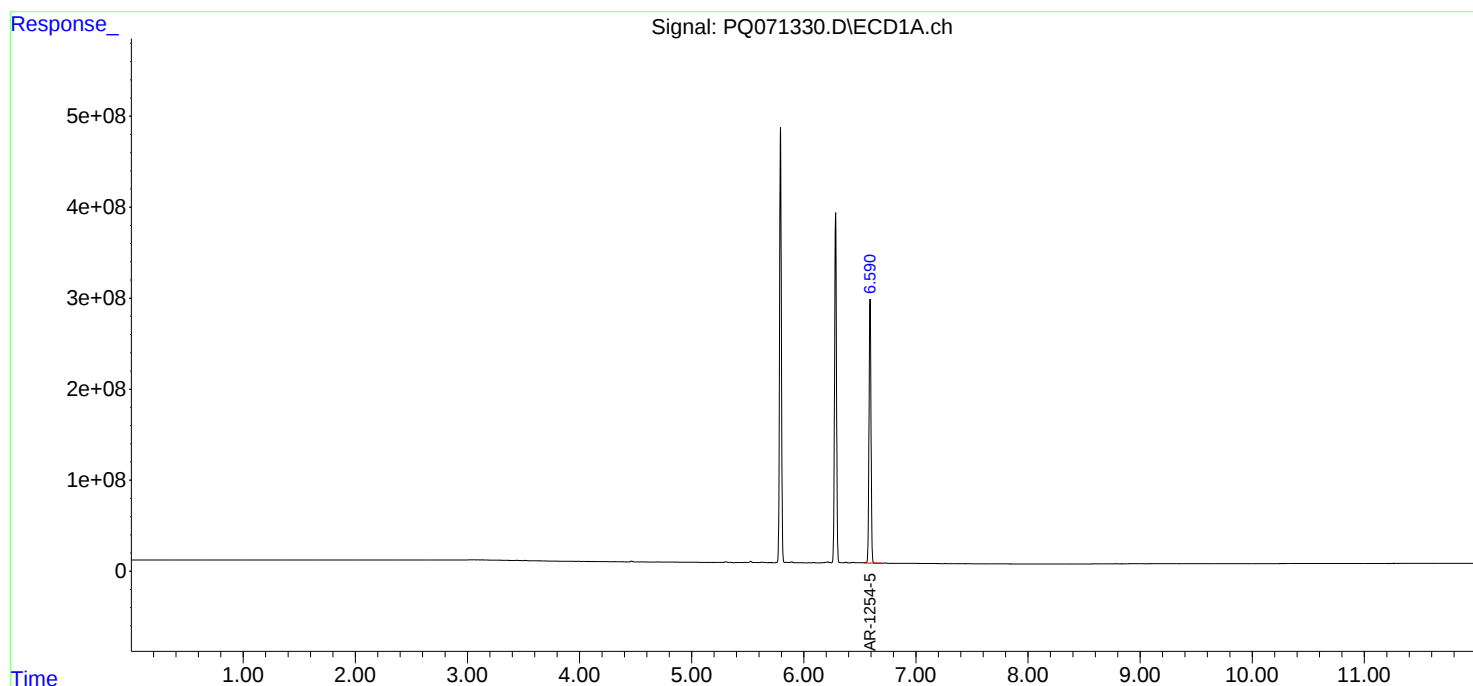


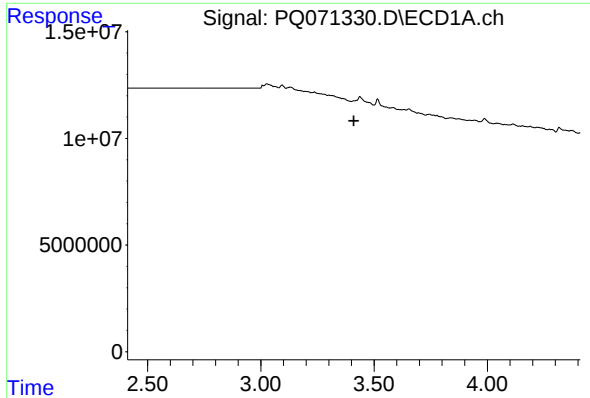

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

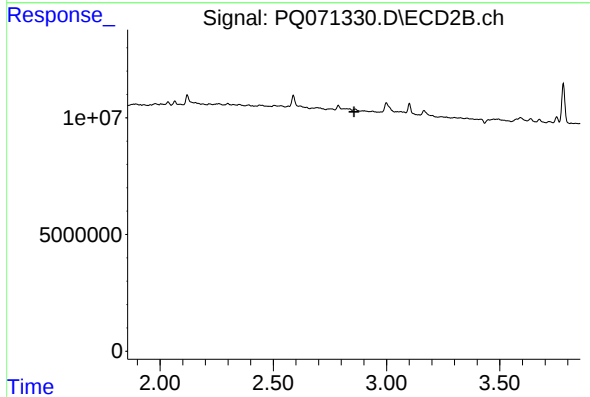


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.856 min
Response: 0
Conc: N.D.

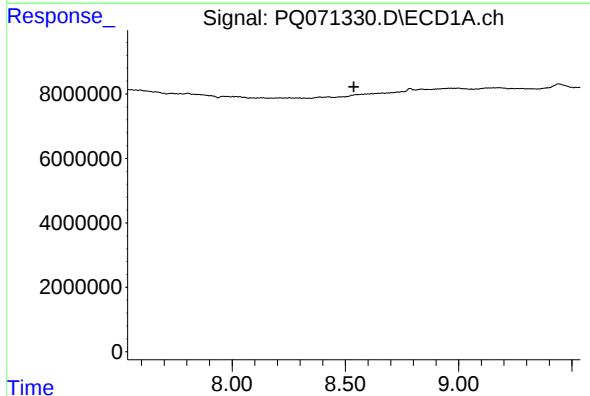


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.537 min
Response: 0
Conc: N.D.

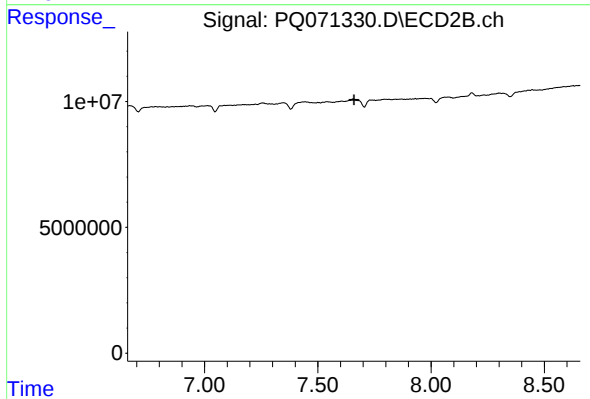

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 7.660 min
Response: 0
Conc: N.D.

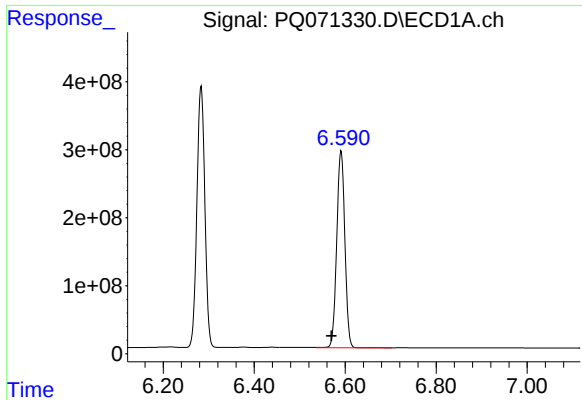

#30 AR-1254-5

R.T.: 6.591 min
Delta R.T.: 0.022 min
Response: 3581938961
Conc: 7793.06 ng/m

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

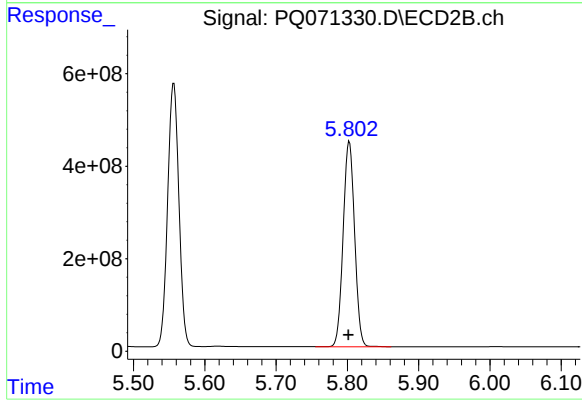

#30 AR-1254-5

R.T.: 5.803 min
Delta R.T.: 0.001 min
Response: 4964735017
Conc: 7172.09 ng/ml