

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ111920\
Data File : PQ051109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2020 03:43
Operator : DD\AJ
Sample : L4751-07
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
C0BG0

Manual Integrations
APPROVED

mohammad
11/20/2020 1:51:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 07:20:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111820CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 19 05:59:02 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

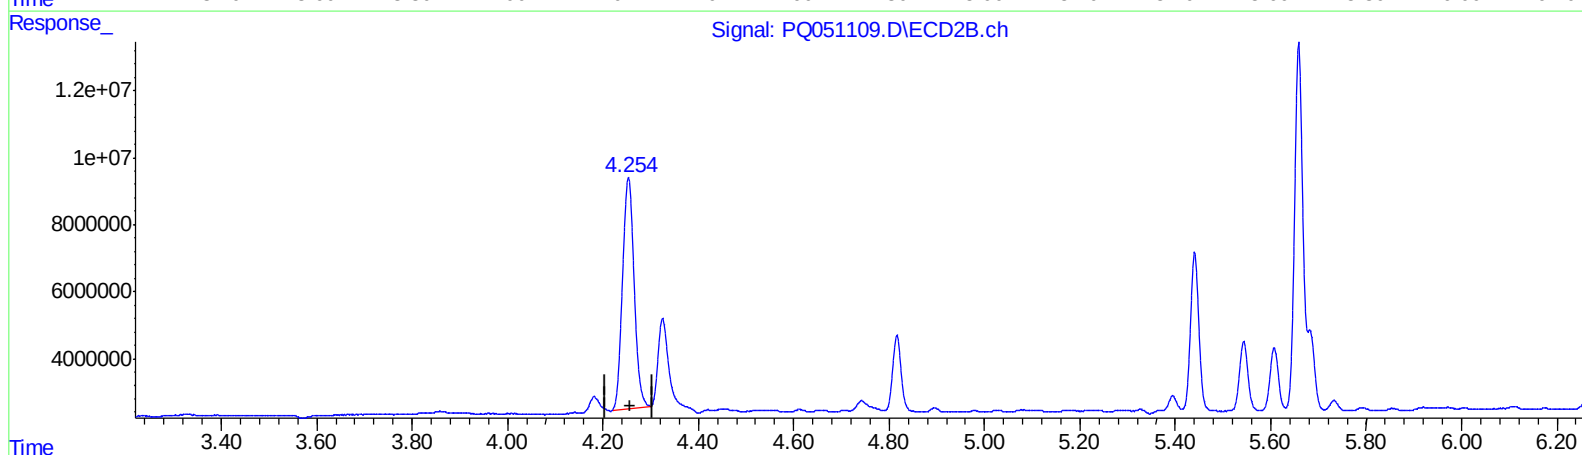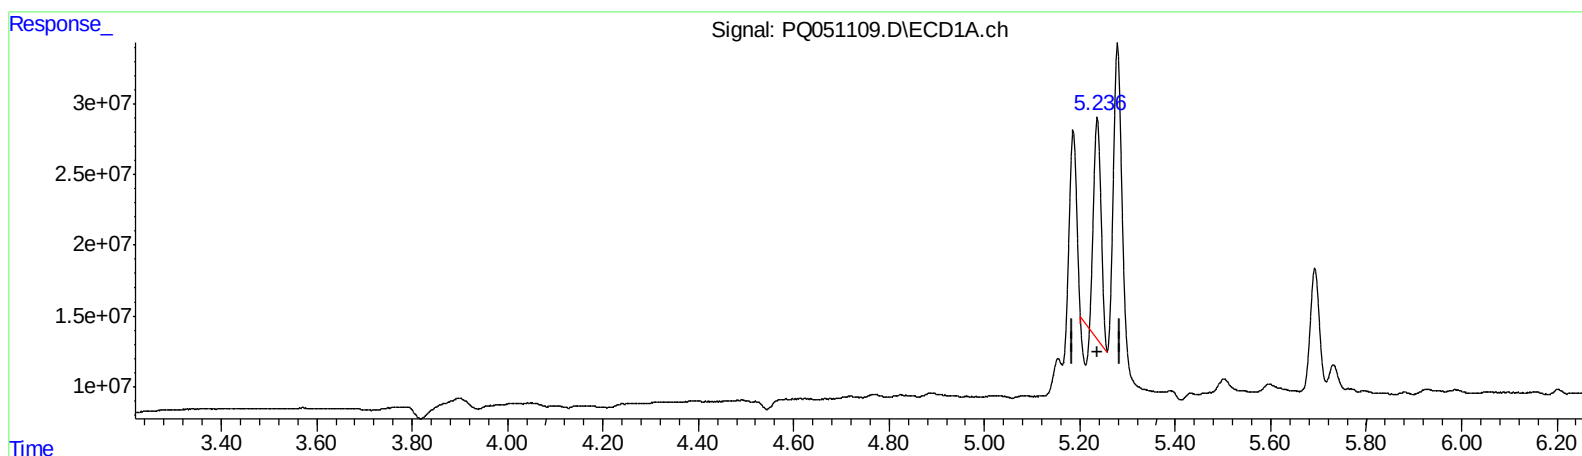

QEdit

(1) Tetrachloro-m-xylene (SA)

5.236min 6.891 ng/ml

response 156035172

(1) Tetrachloro-m-xylene #2 (SA)

4.254min 19.437 ng/ml

response 115885560

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ111920\
 Data File : PQ051109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2020 03:43
 Operator : DD\AJ
 Sample : L4751-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 C0BG0

Manual Integrations
 APPROVED

mohammad
 11/20/2020 1:51:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 07:20:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111820CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 19 05:59:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.236	4.254	213.0E6	115.9E6	9.405m	19.437 #
2) SA Decachlor...	11.430	9.612	278.3E6	80119303	16.962	15.689

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 11/25/20