

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112123\
 Data File : PQ064290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 20:20
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2023
 Supervised By :Ankita Jodhani 11/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:01:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 08 18:43:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.458	2.775	81931065	88619421	19.222	24.097 #
2) SA Decachlor...	8.689	7.569	63967208	83711159	19.812	17.866m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112123\
Data File : PQ064290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 20:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2023
Supervised By :Ankita Jodhani 11/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:01:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 08 18:43:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

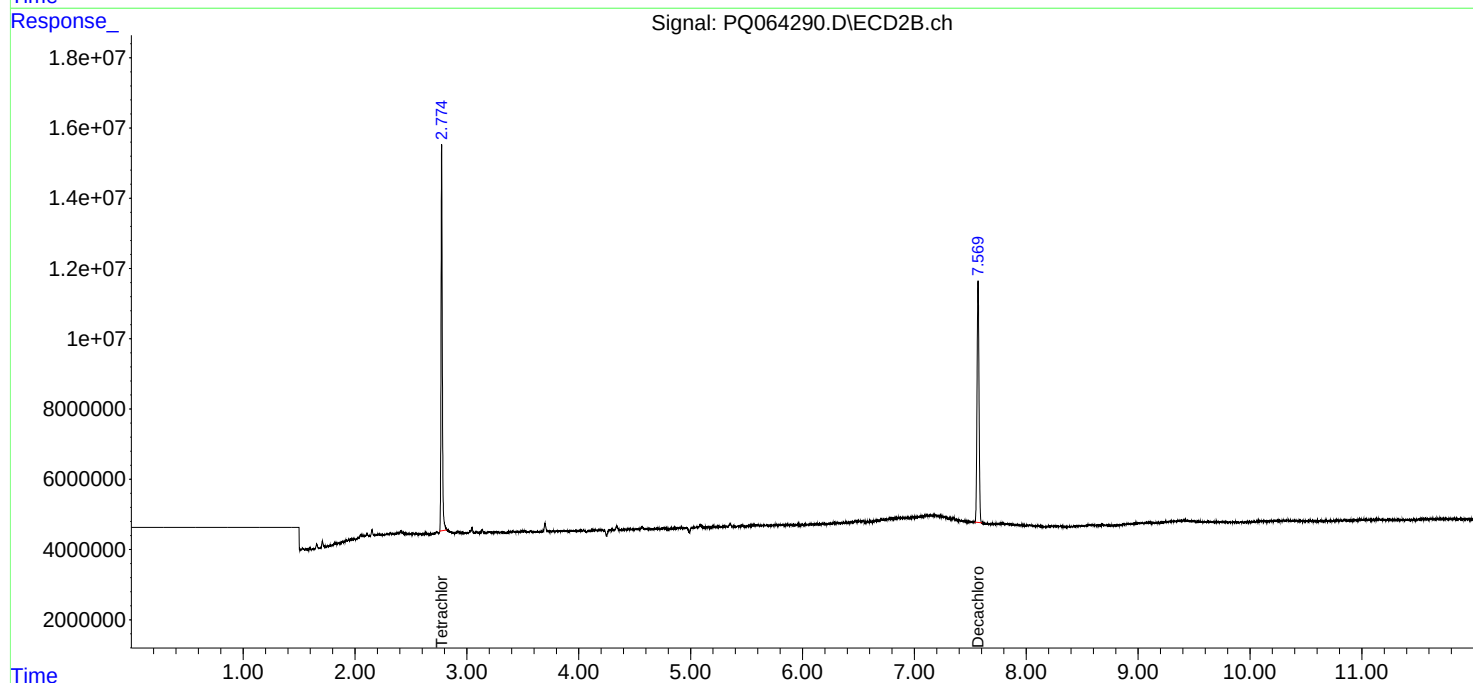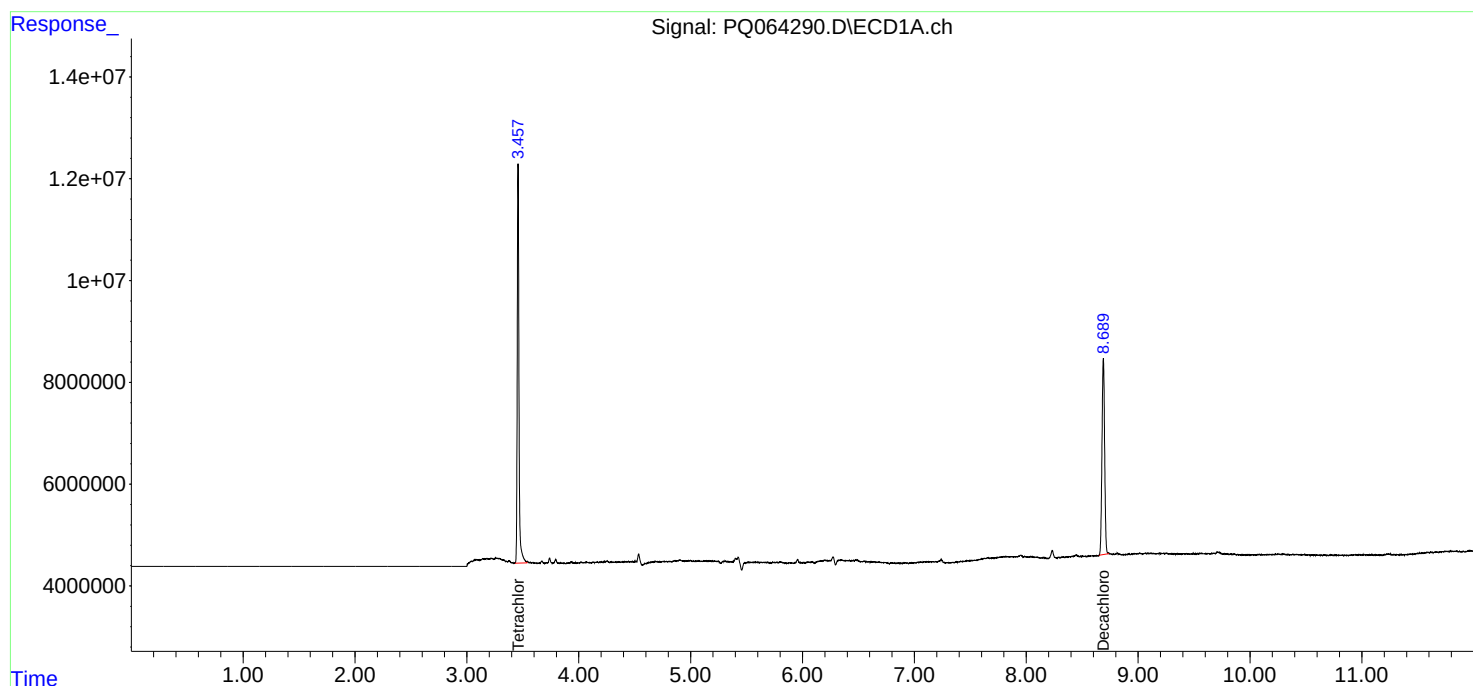

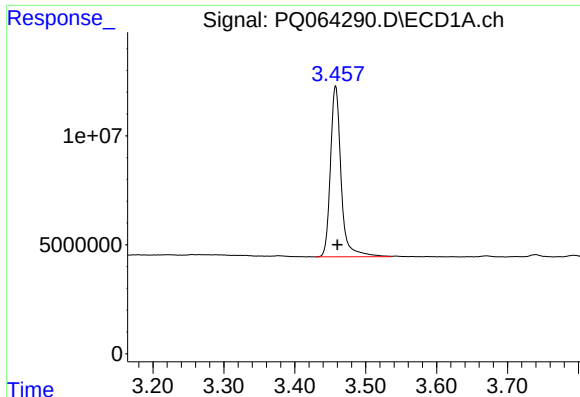


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: -0.002 min
Response: 81931065
Conc: 19.22 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/22/2023
Supervised By :Ankita Jodhani 11/22/2023

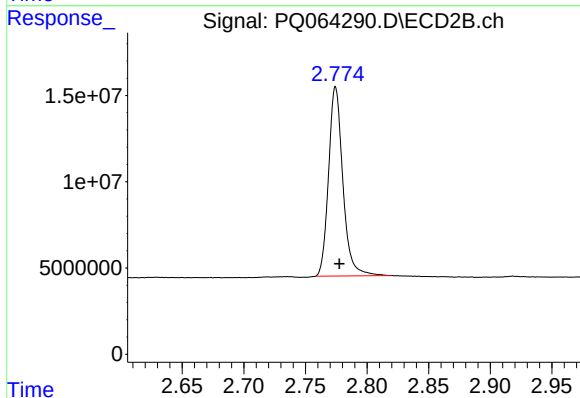


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: -0.003 min
Response: 88619421
Conc: 24.10 ng/ml

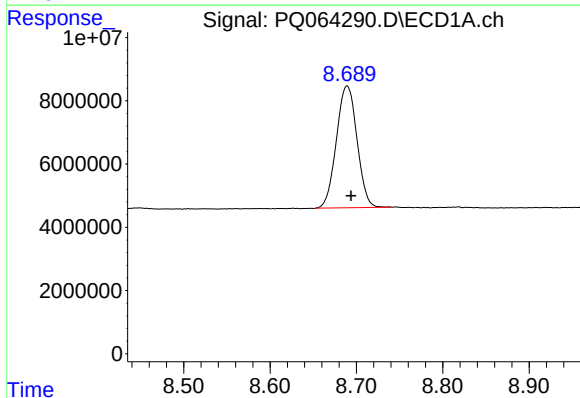

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.005 min
Response: 63967208
Conc: 19.81 ng/ml

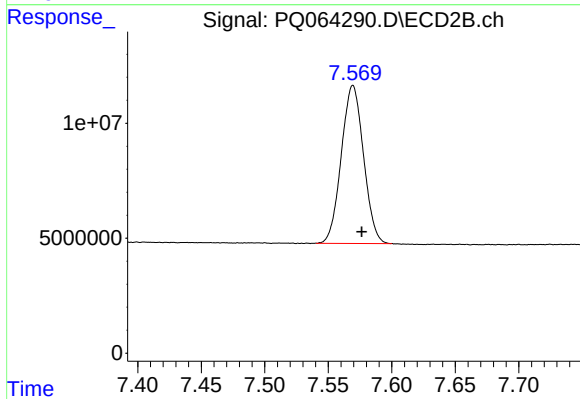

#2 Decachlorobiphenyl

R.T.: 7.569 min
Delta R.T.: -0.007 min
Response: 83711159
Conc: 17.87 ng/ml m