

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112219\
 Data File : PQ045341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 17:26
 Operator : SM\AJ
 Sample : K5985-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 C0B06

Manual Integrations
 APPROVED

Ankita

11/25/2019 11:49:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 17:45:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110719CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 03:35:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.092	4.300	98243473	63199890	12.377	13.403
2) SA Decachlor...	11.152	9.716	167.9E6	164.8E6	24.247	24.282m
Target Compounds						
26) L6 AR-1254-1	7.317	6.462	19489.3E6	17187.5E6	60234.543	47246.955
27) L6 AR-1254-2	7.546	6.621	31268.8E6	18232.7E6	62978.260	56609.310
28) L6 AR-1254-3	7.930	7.048	34697.9E6	32089.0E6	65189.685	57849.933
29) L6 AR-1254-4	8.219	7.288	29789.7E6	24150.2E6	77117.280m	67567.446
30) L6 AR-1254-5	8.651	7.721	33699.0E6	36415.8E6	78010.251	72828.243

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112219\
Data File : PQ045341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 17:26
Operator : SM\AJ
Sample : K5985-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
C0B06



Manual Integrations
APPROVED

Ankita

11/25/2019 11:49:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 17:45:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110719CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 03:35:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

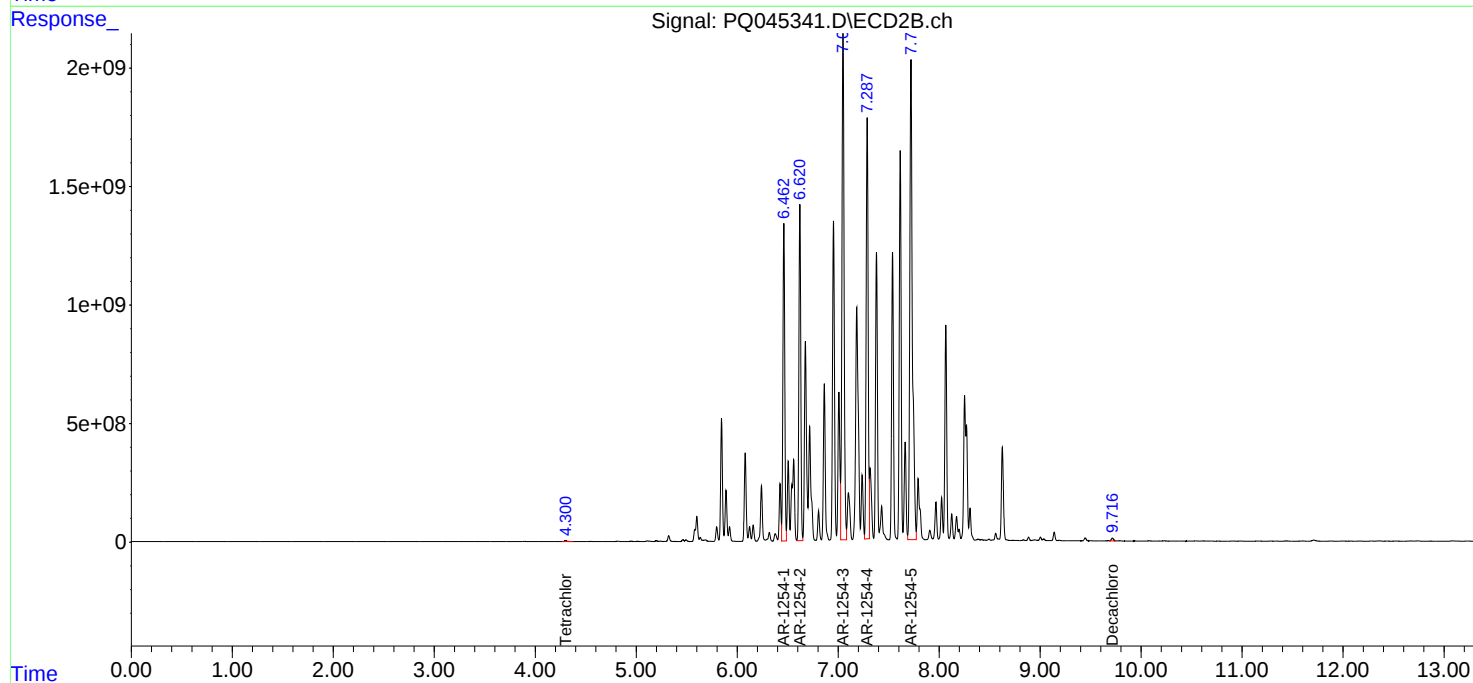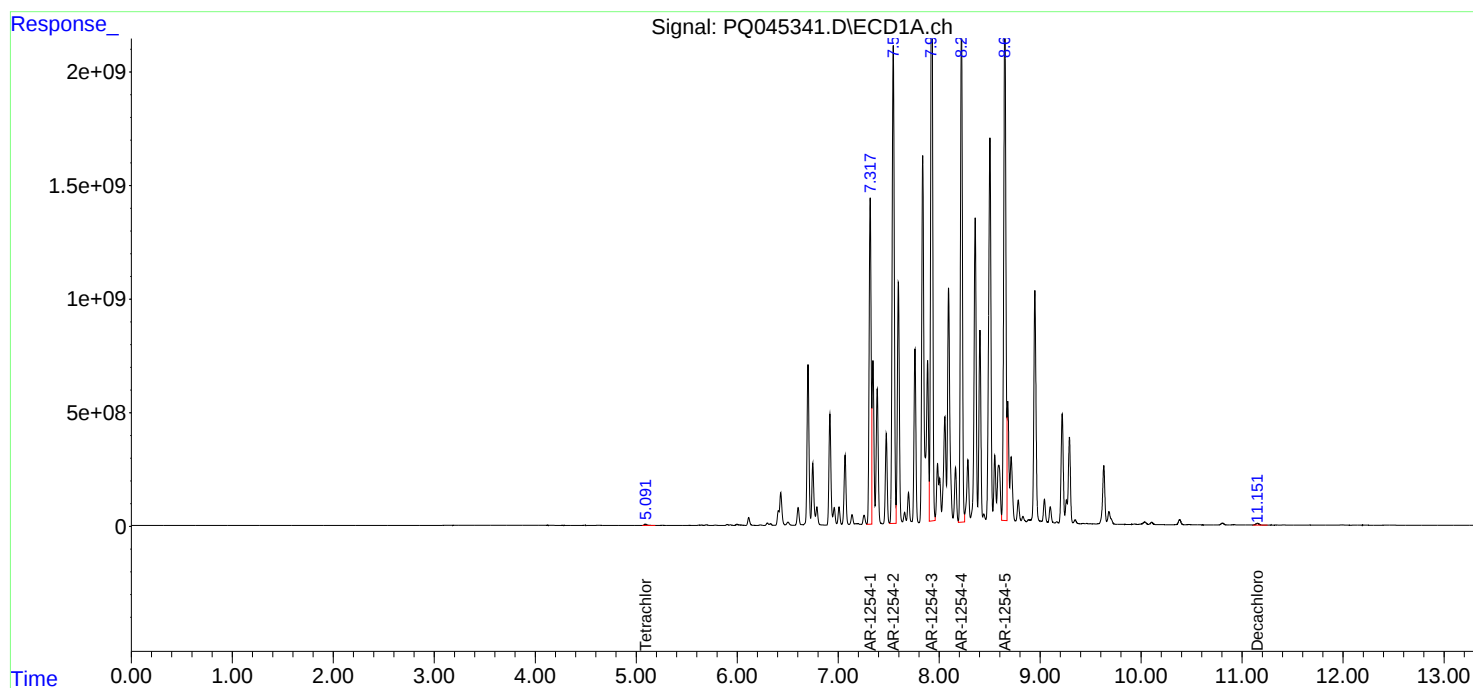

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112219\
Data File : PQ045341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 17:26
Operator : SM\AJ
Sample : K5985-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
C0B06


Manual Integrations
APPROVED

Ankita

11/25/2019 11:49:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 17:45:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110719CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 03:35:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

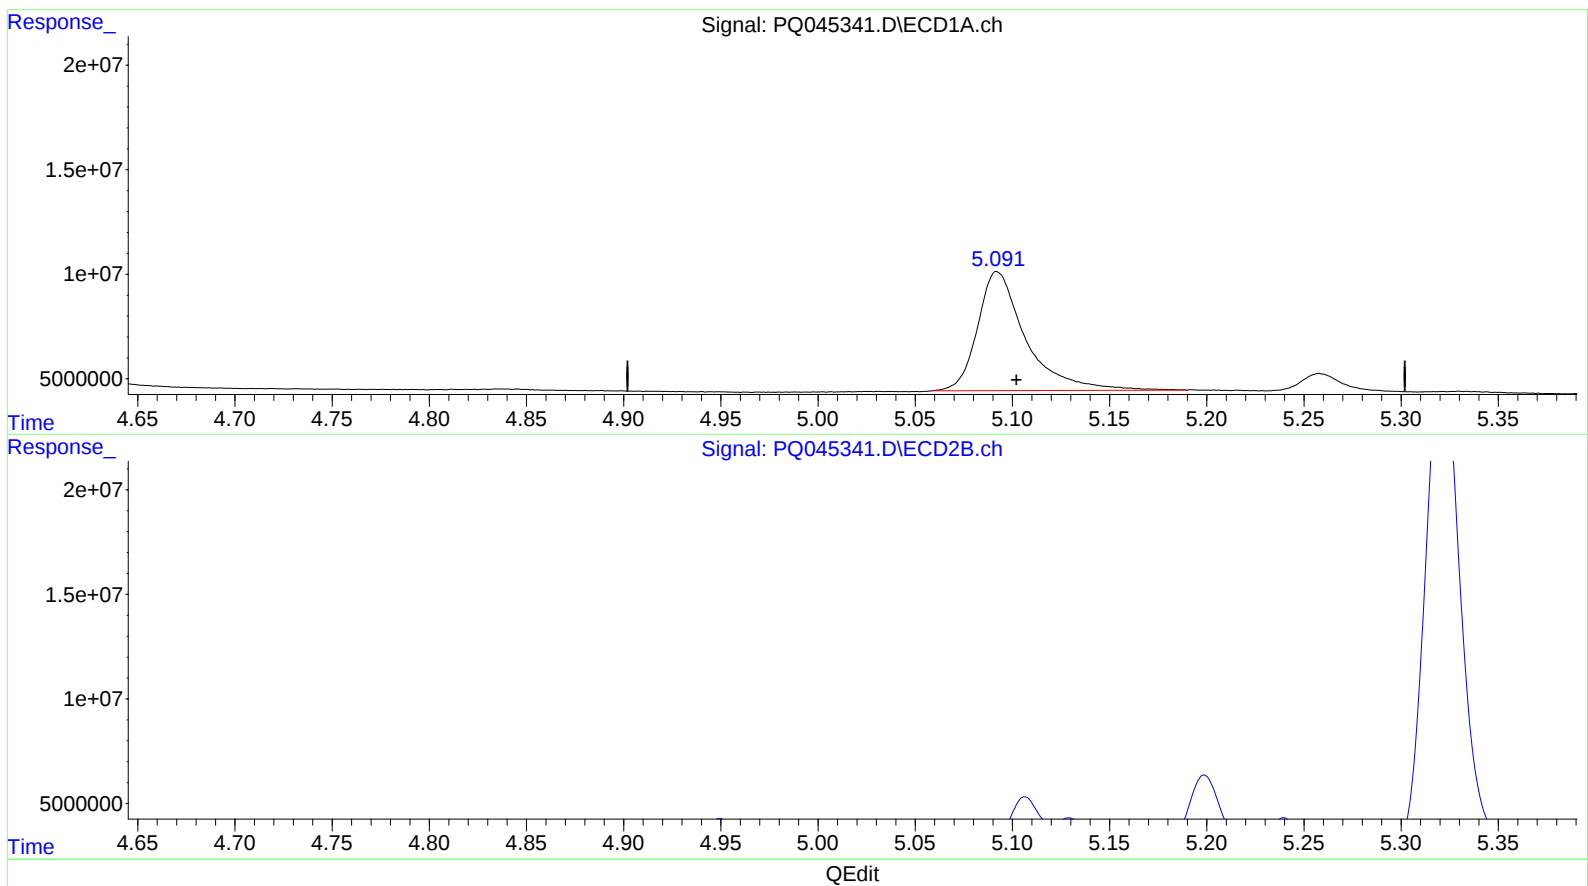

(1) Tetrachloro-m-xylene (SA)

5.092min 12.377 ng/ml

response 98243473

(1) Tetrachloro-m-xylene #2 (SA)

4.300min 13.403 ng/ml

response 63199890

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112219\
Data File : PQ045341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 17:26
Operator : SM\AJ
Sample : K5985-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
C0B06



Manual Integrations
APPROVED

Ankita

11/25/2019 11:49:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 17:45:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110719CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 03:35:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

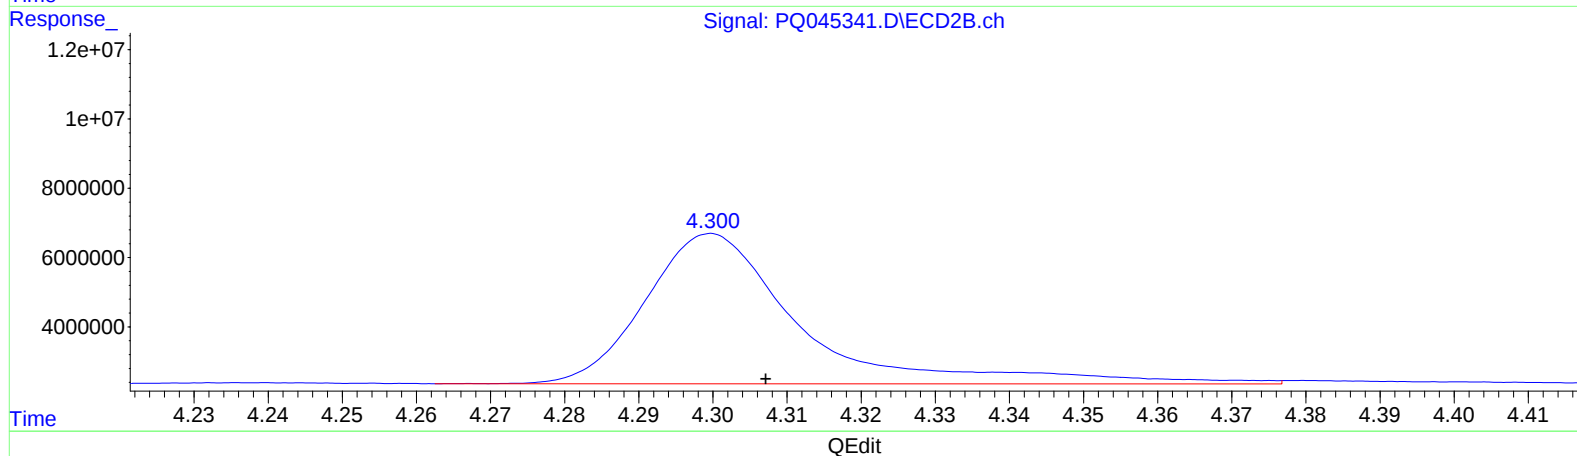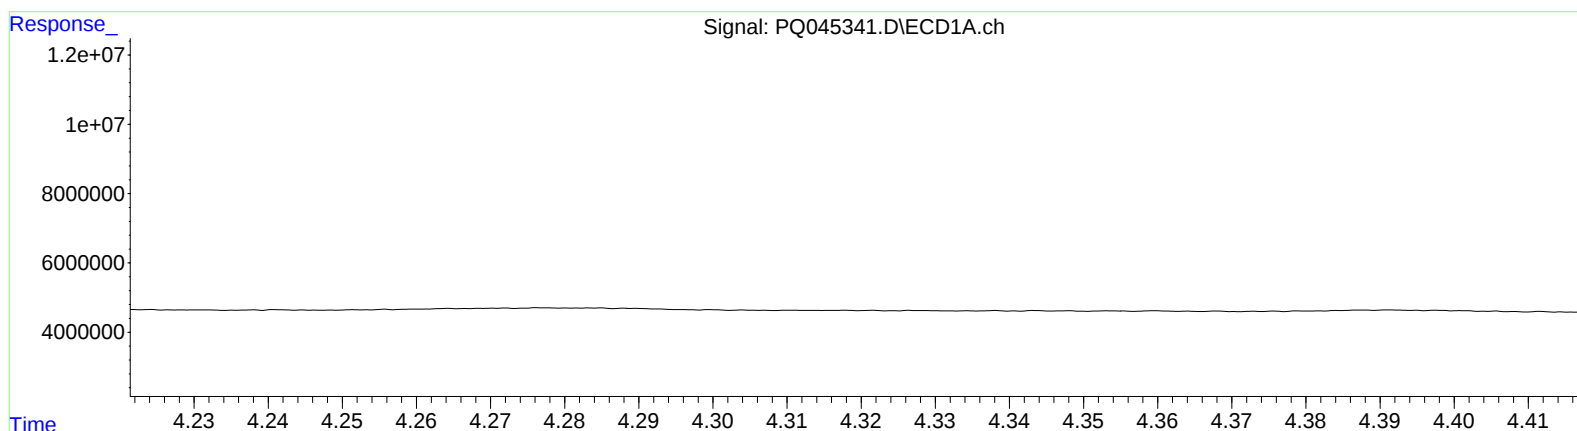

(1) Tetrachloro-m-xylene (SA)

5.092min 12.377 ng/ml

response 98243473

(1) Tetrachloro-m-xylene #2 (SA)

4.300min 13.403 ng/ml

response 63199890

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112219\
Data File : PQ045341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 17:26
Operator : SM\AJ
Sample : K5985-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
C0B06



Manual Integrations
APPROVED

Ankita

11/25/2019 11:49:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 17:45:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110719CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 03:35:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

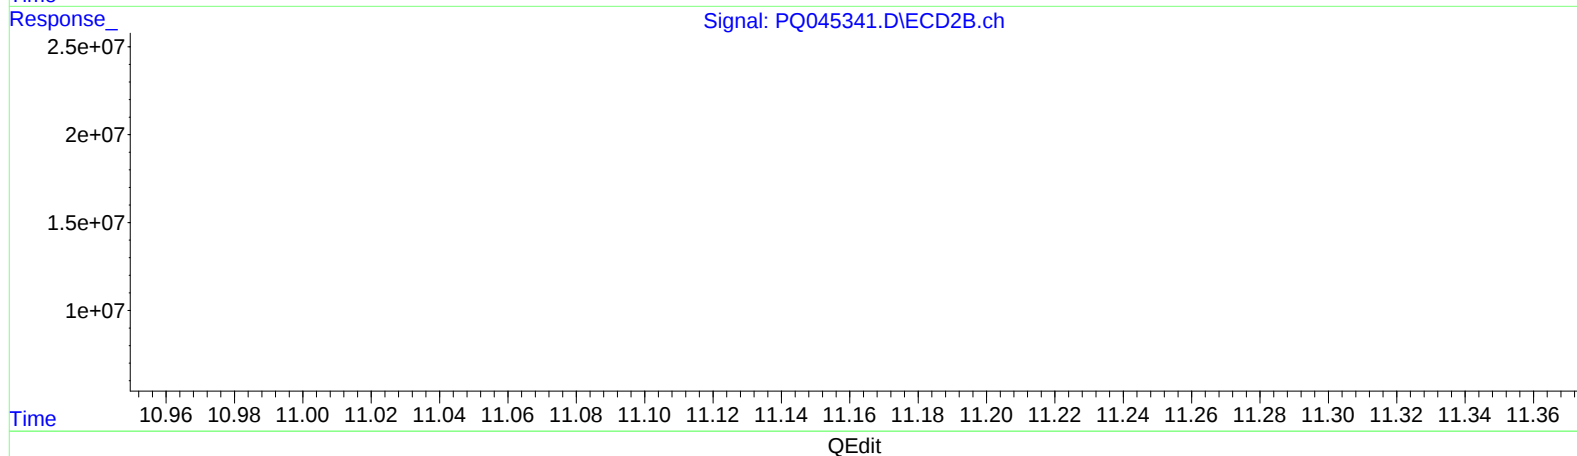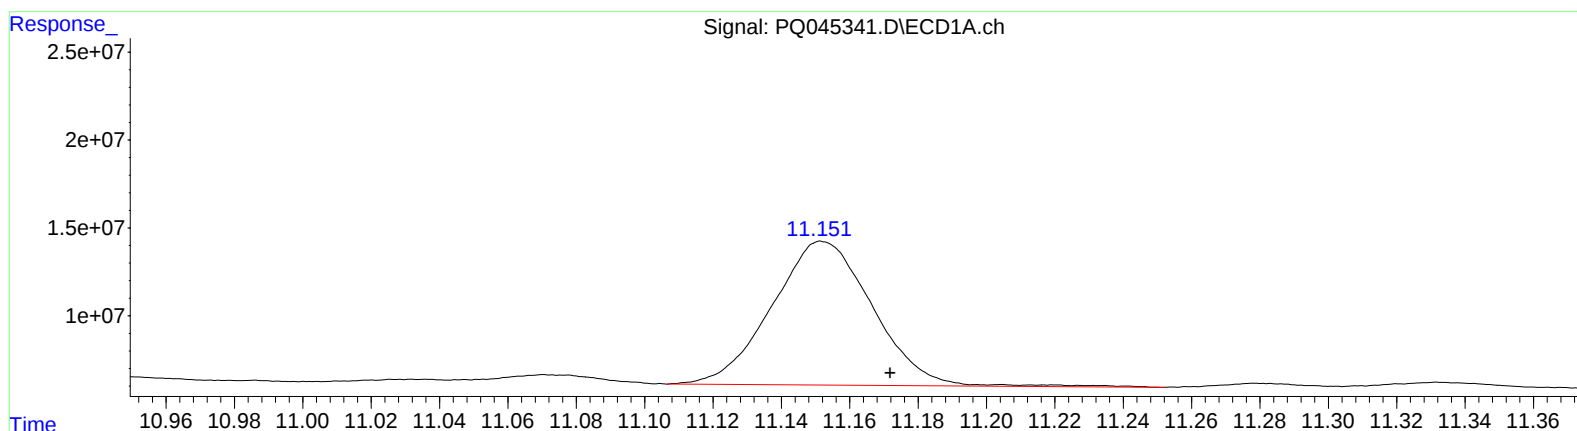

(2) Decachlorobiphenyl (SA)

11.152min 24.247 ng/ml

response 167933001

(2) Decachlorobiphenyl #2 (SA)

9.716min 24.282 ng/ml m

response 164757243

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112219\
Data File : PQ045341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 17:26
Operator : SM\AJ
Sample : K5985-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
C0B06



Manual Integrations
APPROVED

Ankita

11/25/2019 11:49:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 17:45:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ110719CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 03:35:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

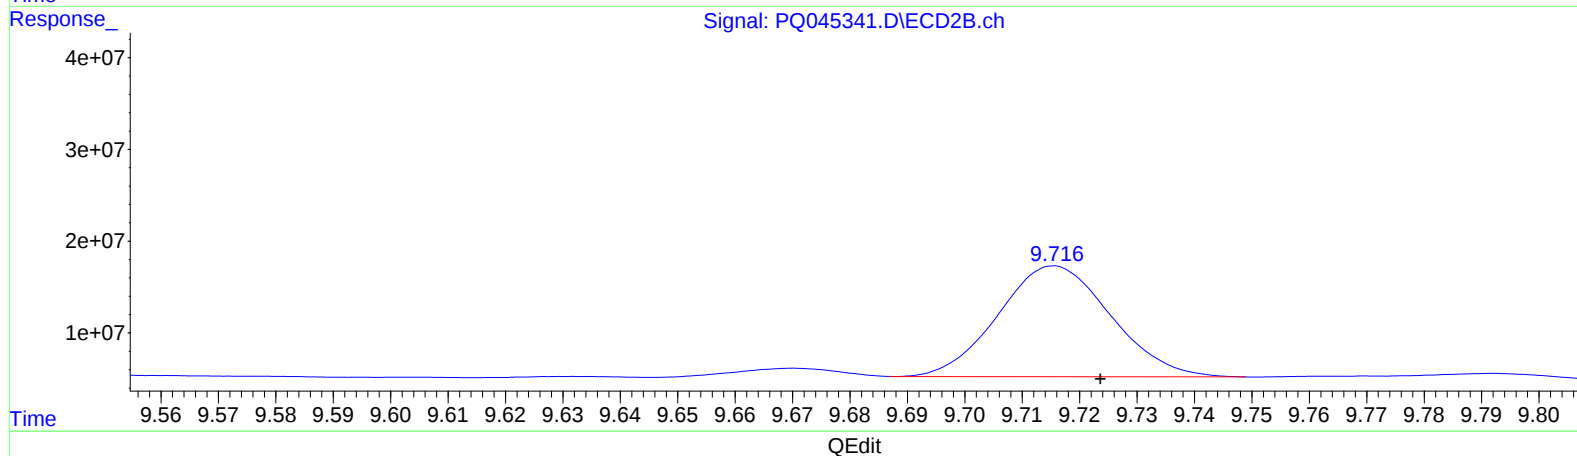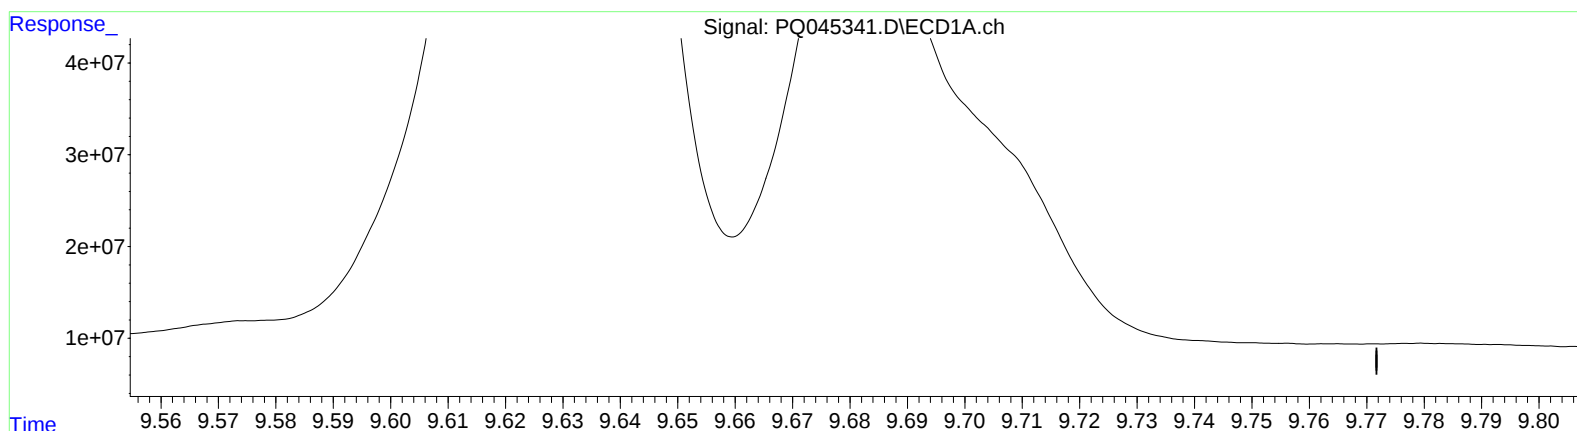

(2) Decachlorobiphenyl (SA)

11.152min 24.247 ng/ml

response 167933001

(2) Decachlorobiphenyl #2 (SA)

9.716min 24.282 ng/ml m

response 164757243