

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112525\
 Data File : PQ071528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 18:13
 Operator : YP\AJ
 Sample : Q3697-04 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MOO-25-0329

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/26/2025
 Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 05:11:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 19 04:02:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.409	2.853	15866548	22515600	1.823m	2.412 #
2) SA Decachlor...	8.535	7.651	6594395	9304104	1.053	1.018

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112525\
Data File : PQ071528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 18:13
Operator : YP\AJ
Sample : Q3697-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
MOO-25-0329


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 05:11:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 19 04:02:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

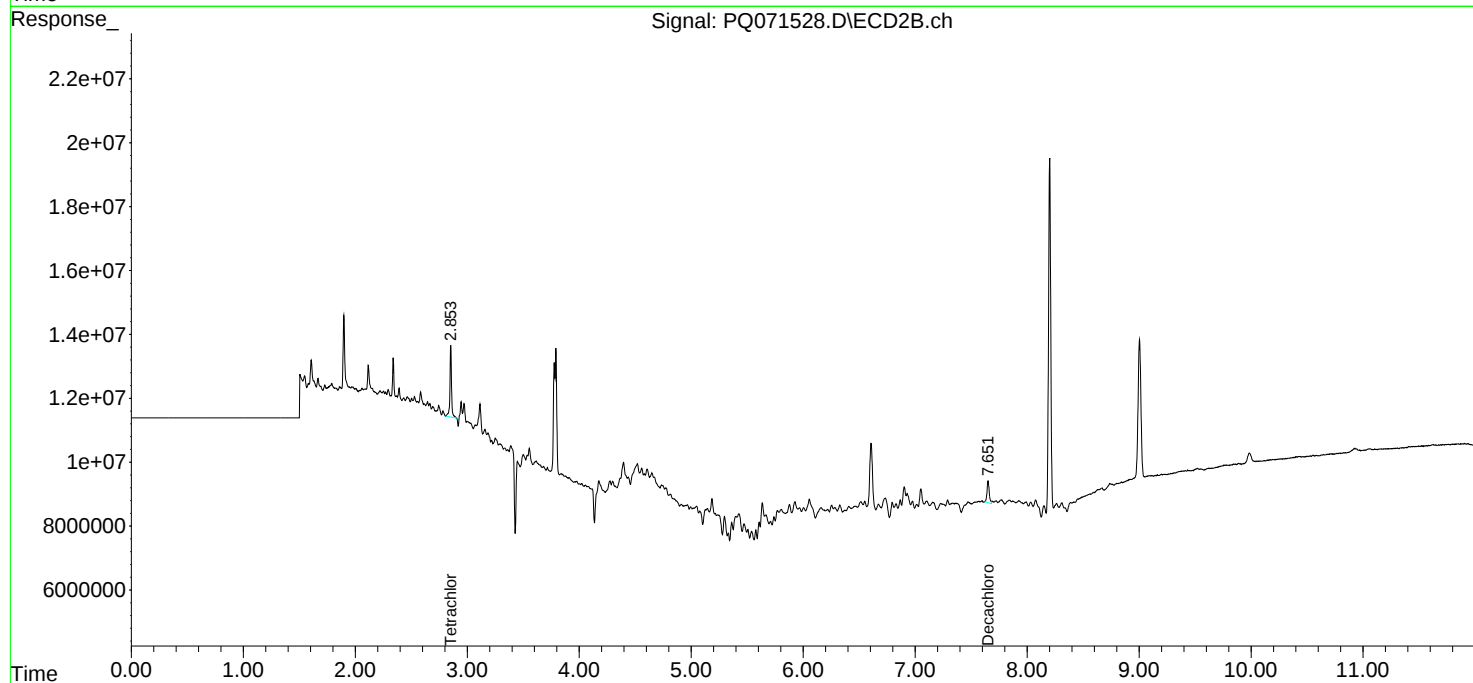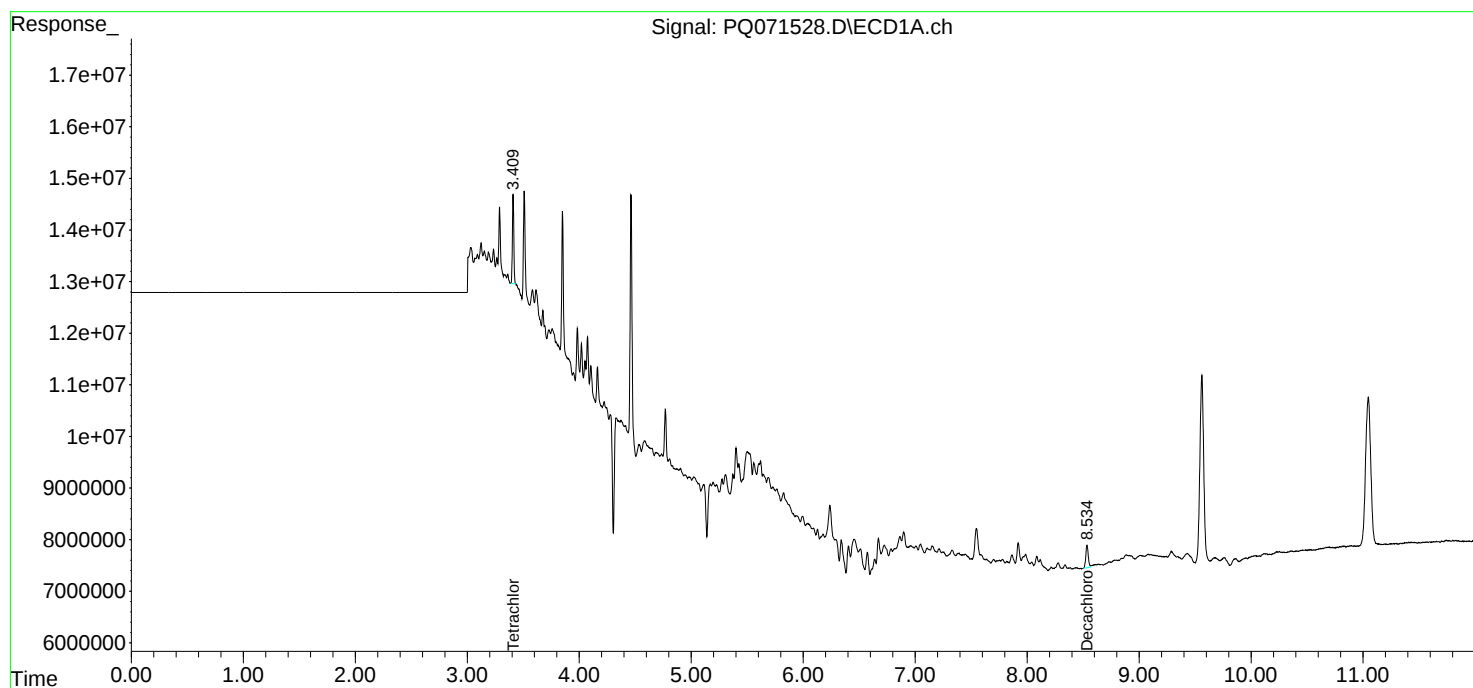

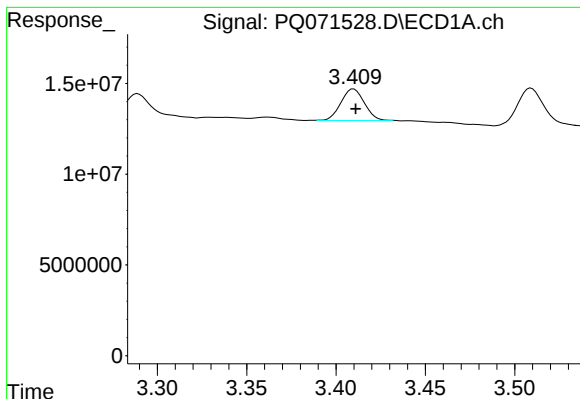


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: -0.002 min
Response: 15866548
Conc: 1.82 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MOO-25-0329


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

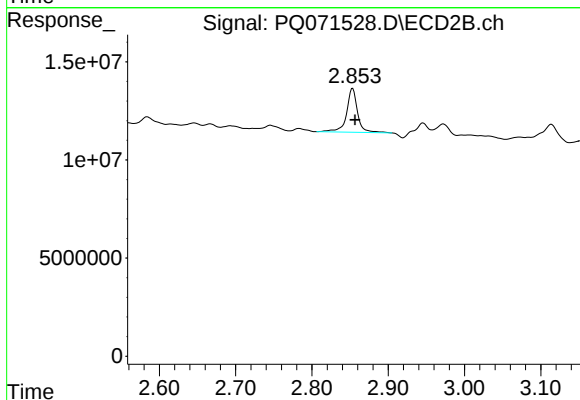


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: -0.003 min
Response: 22515600
Conc: 2.41 ng/ml

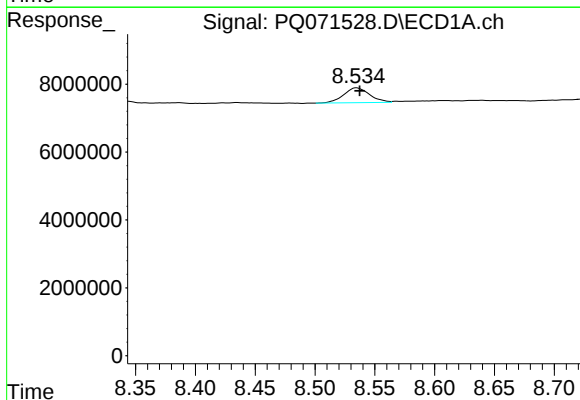

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.003 min
Response: 6594395
Conc: 1.05 ng/ml

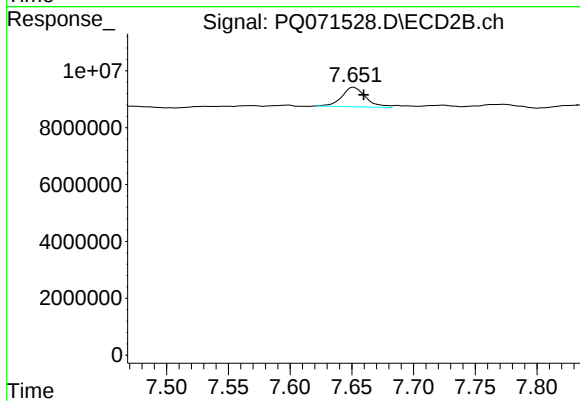

#2 Decachlorobiphenyl

R.T.: 7.651 min
Delta R.T.: -0.008 min
Response: 9304104
Conc: 1.02 ng/ml