

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ112618\  
Data File : PQ034988.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 26 Nov 2018 19:07  
Operator : SM\SJ  
Sample : J6039-09  
Misc :  
ALS Vial : 18 Sample Multiplier: 1


Instrument :  
ECD\_Q  
ClientSampleId :  
CB4N5

Manual Integrations  
APPROVED

mohammad  
11/29/2018 8:24:59 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 27 00:09:12 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ111718CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Nov 16 03:52:57 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

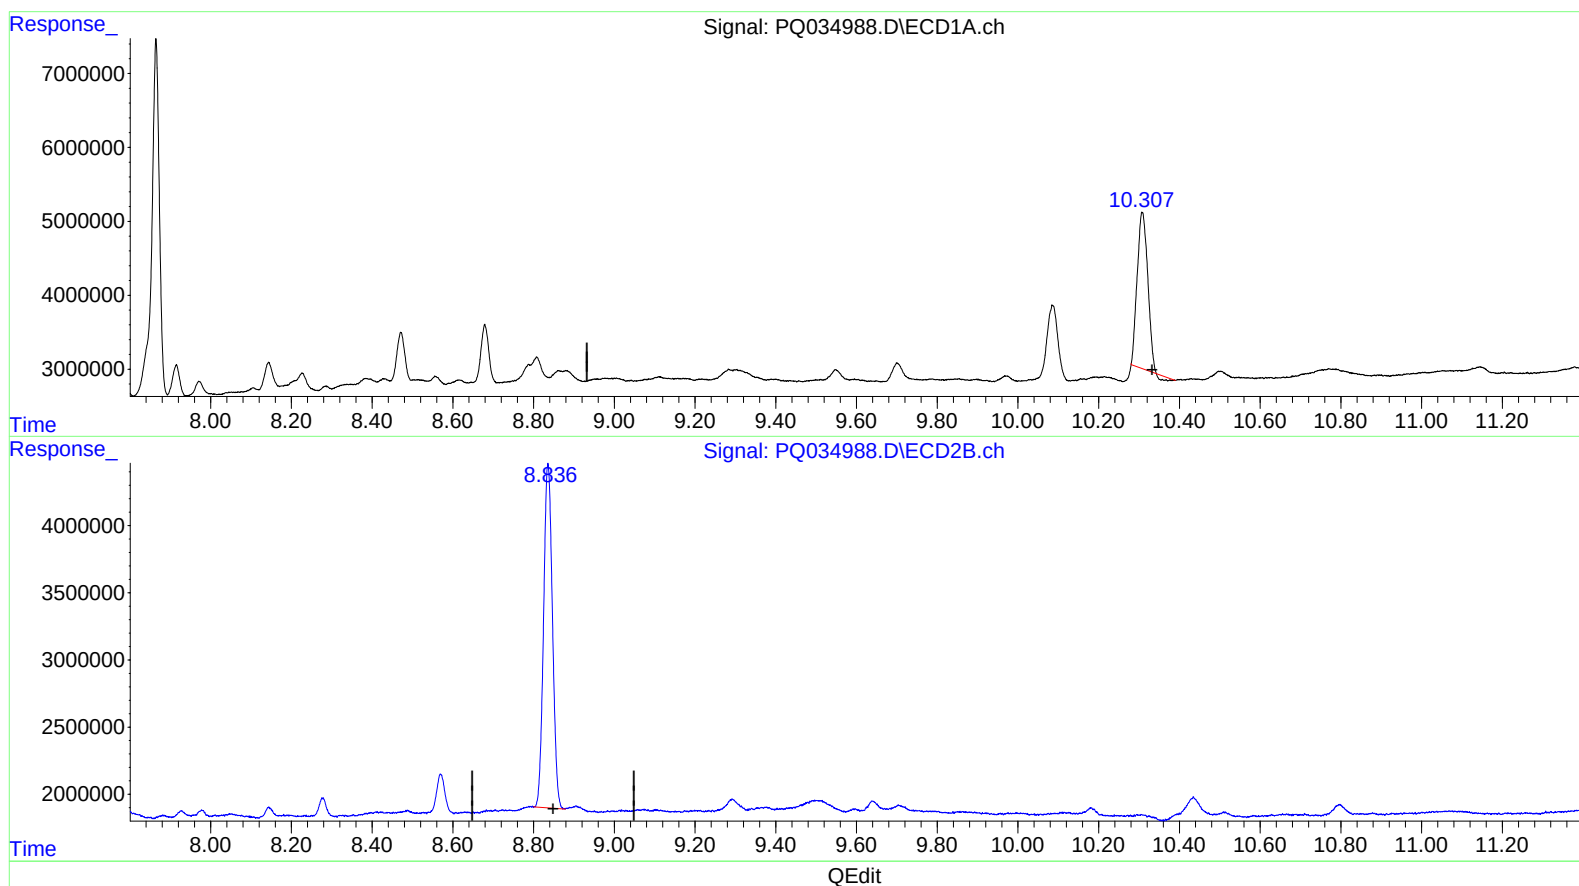

(2) Decachlorobiphenyl (SA)

10.308min 13.634 ng/ml

response 37561094

(2) Decachlorobiphenyl #2 (SA)

8.836min 19.970 ng/ml

response 38923329

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ112618\  
Data File : PQ034988.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 26 Nov 2018 19:07  
Operator : SM\SJ  
Sample : J6039-09  
Misc :  
ALS Vial : 18 Sample Multiplier: 1


Instrument :  
ECD\_Q  
ClientSampleId :  
CB4N5

Manual Integrations  
APPROVED

mohammad  
11/29/2018 8:24:59 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 27 09:22:08 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ111718CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Nov 16 03:52:57 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

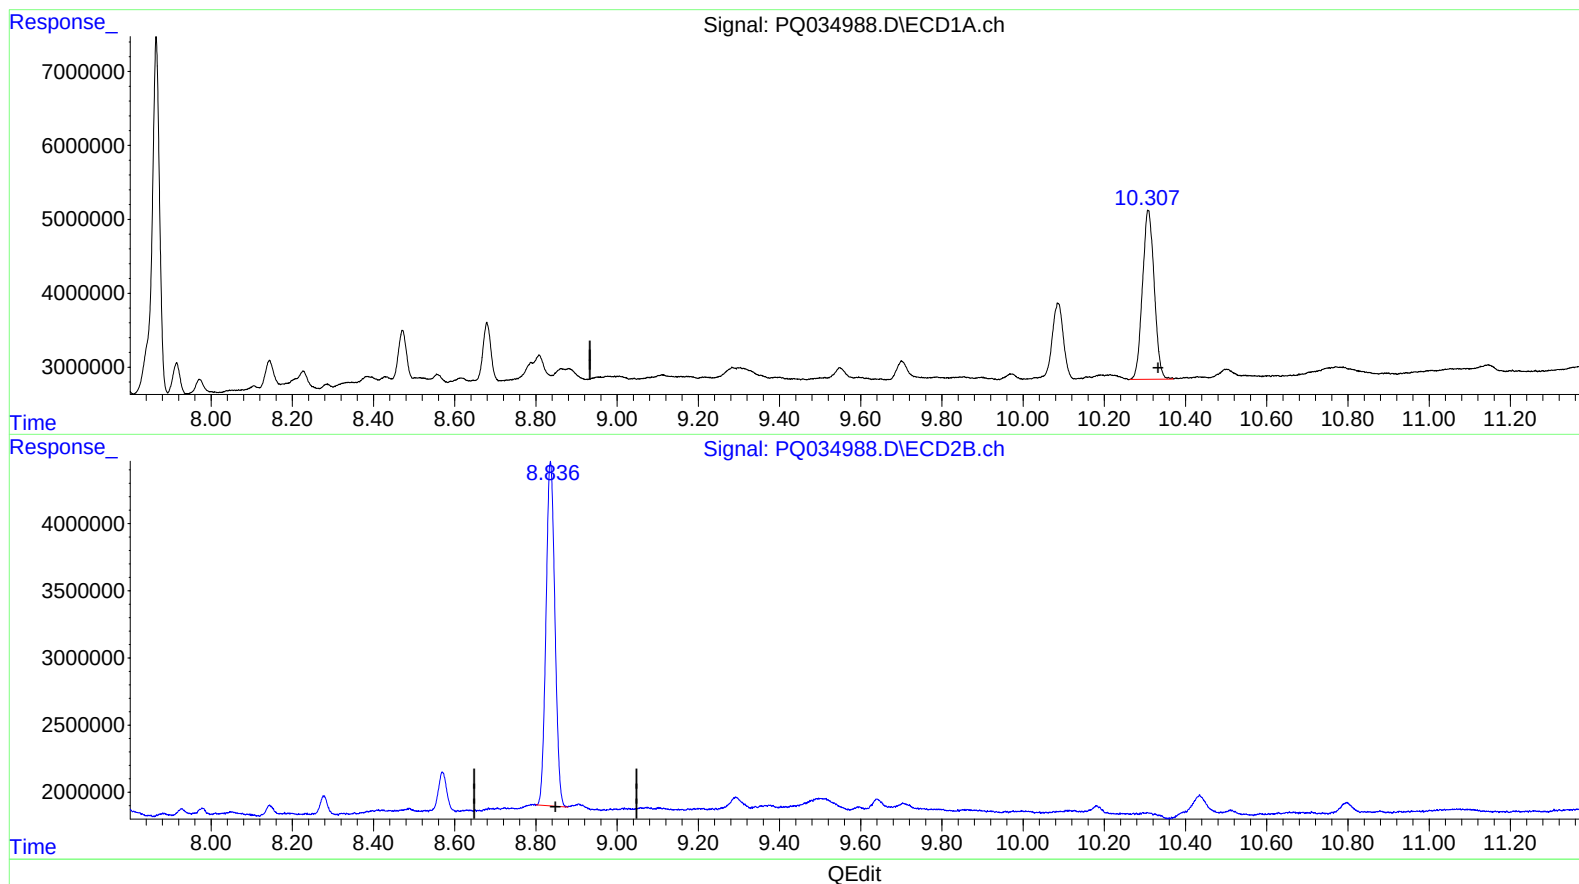

(2) Decachlorobiphenyl (SA)

10.307min 16.690 ng/ml m

response 45980251

(2) Decachlorobiphenyl #2 (SA)

8.836min 19.970 ng/ml

response 38923329

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ112618\  
 Data File : PQ034988.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 26 Nov 2018 19:07  
 Operator : SM\SJ  
 Sample : J6039-09  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_Q  
 ClientSampleId :  
 CB4N5

Manual Integrations  
 APPROVED

mohammad  
 11/29/2018 8:24:59 AM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 27 09:22:08 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ111718CLP.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Nov 16 03:52:57 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------|-------|----------|----------|---------|----------|
| -----                       |        |       |          |          |         |          |
| System Monitoring Compounds |        |       |          |          |         |          |
| 1) SA Tetrachlo...          | 4.527  | 3.815 | 48154551 | 30033655 | 17.483  | 17.719   |
| 2) SA Decachlor...          | 10.307 | 8.836 | 45980251 | 38923329 | 16.690m | 19.970   |
| Target Compounds            |        |       |          |          |         |          |
| 31) L7 AR-1260-1            | 7.300  | 6.379 | 6262677  | 4254976  | 45.115  | 39.685   |
| 32) L7 AR-1260-2            | 7.554  | 6.566 | 53281711 | 5435491  | 311.655 | 40.473 # |
| 33) L7 AR-1260-3            | 7.915  | 6.719 | 5028421  | 4490420  | 47.182  | 36.577   |
| 34) L7 AR-1260-4            | 8.144  | 7.188 | 6322572  | 3234149  | 47.737  | 37.497   |
| 35) L7 AR-1260-5            | 8.471  | 7.430 | 8972173  | 8418819  | 33.068  | 38.299   |
| -----                       |        |       |          |          |         |          |

) SJ 11/28/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.