

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112625\
 Data File : PQ071546.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2025 17:09
 Operator : YP\AJ
 Sample : Q3719-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SB-1125-16A

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/01/2025
 Supervised By :mohammad ahmed 12/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:34:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 19 04:02:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.409	2.853	195.0E6	204.4E6	22.396m	21.890m
2) SA Decachlor...	8.538	7.652	98509263	129.6E6	15.732	14.182m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112625\
Data File : PQ071546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2025 17:09
Operator : YP\AJ
Sample : Q3719-11
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SB-1125-16A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/01/2025
Supervised By :mohammad ahmed 12/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:34:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 19 04:02:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

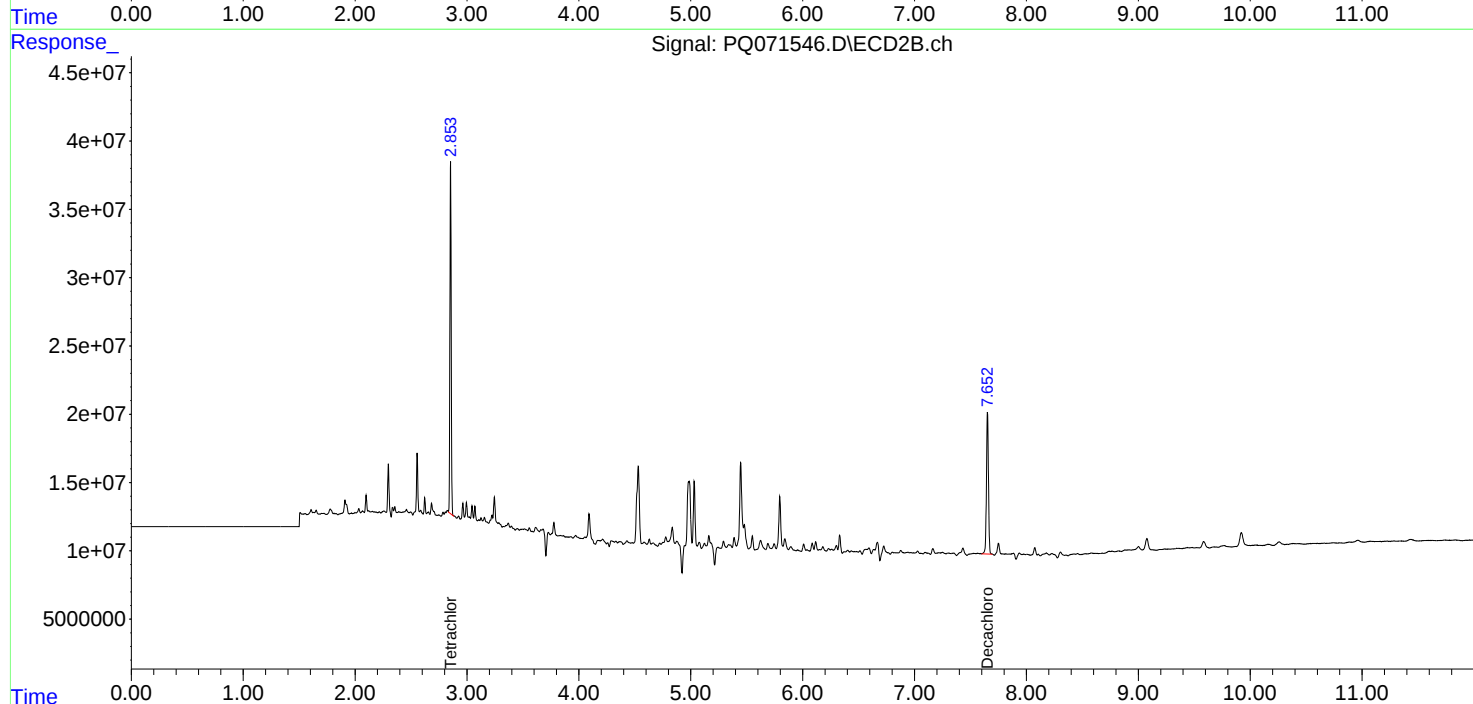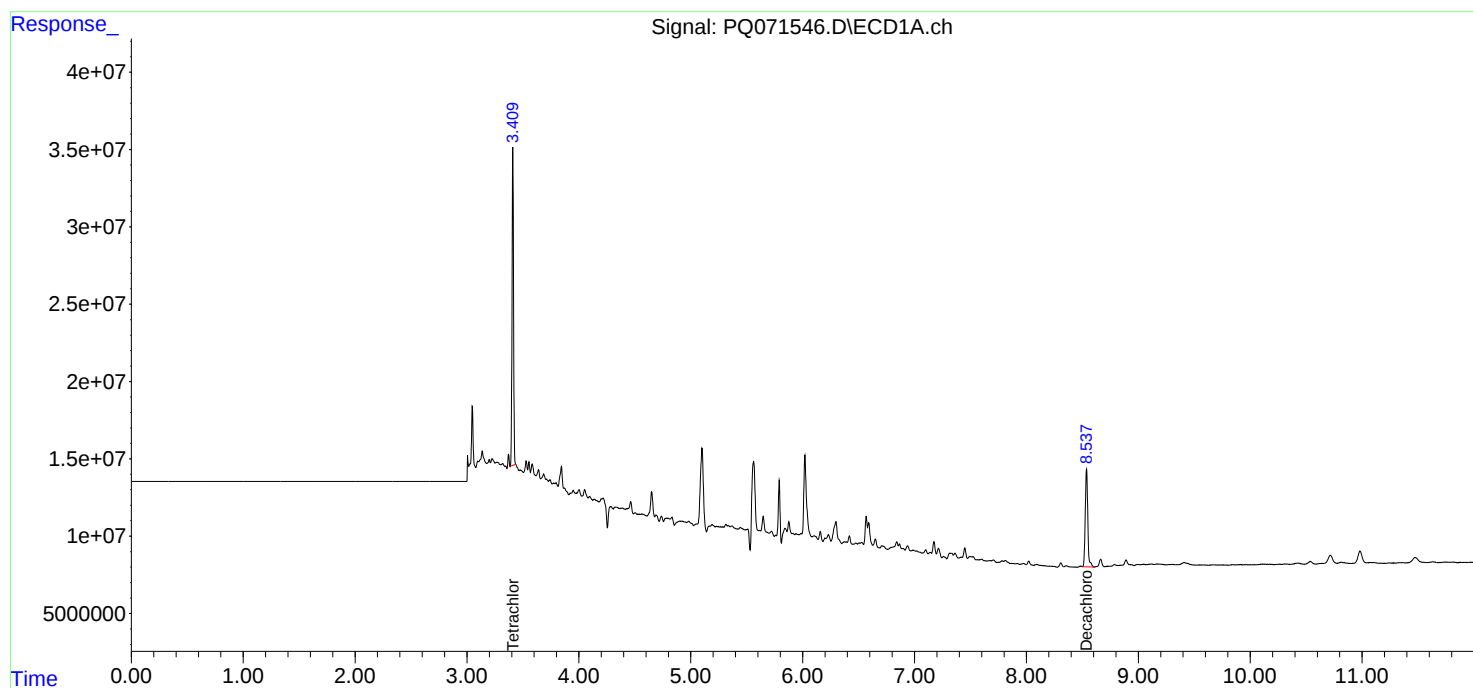

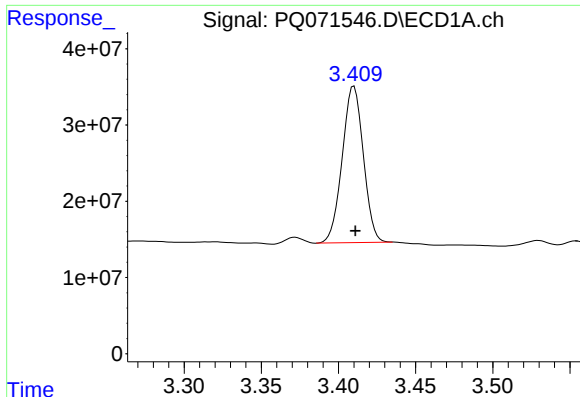


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: -0.002 min
Response: 194961279
Conc: 22.40 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB-1125-16A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/01/2025
Supervised By :mohammad ahmed 12/02/2025

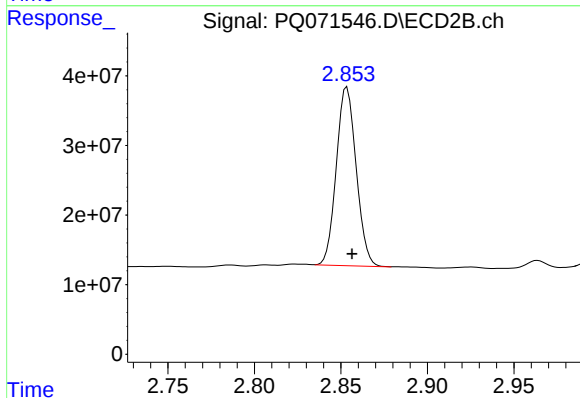


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: -0.004 min
Response: 204384531
Conc: 21.89 ng/ml m

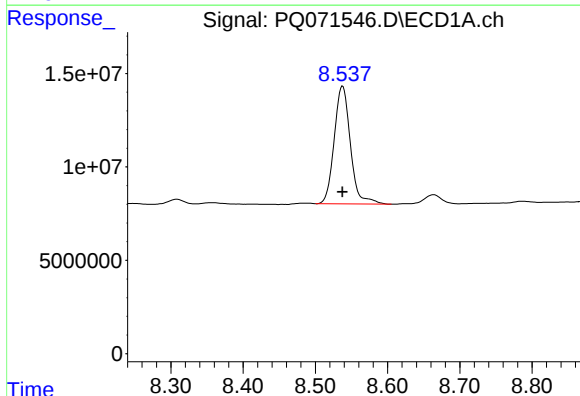

#2 Decachlorobiphenyl

R.T.: 8.538 min
Delta R.T.: 0.000 min
Response: 98509263
Conc: 15.73 ng/ml

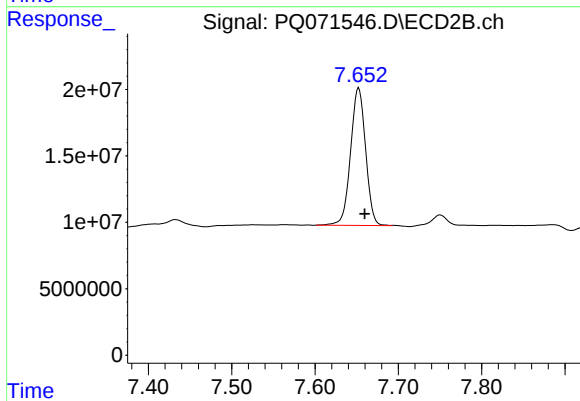

#2 Decachlorobiphenyl

R.T.: 7.652 min
Delta R.T.: -0.008 min
Response: 129590695
Conc: 14.18 ng/ml m