

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121123\
 Data File : PQ064371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 13:56
 Operator : YP\AJ
 Sample : 05718-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 WC-LIQUID-20231206

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 14:14:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.456	2.773	89075547	98485462	21.471	23.458
2) SA Decachlor...	8.693	7.571	54050224	85285275	18.438	21.130

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121123\
Data File : PQ064371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 13:56
Operator : YP\AJ
Sample : 05718-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
WC-LIQUID-20231206

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 14:14:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

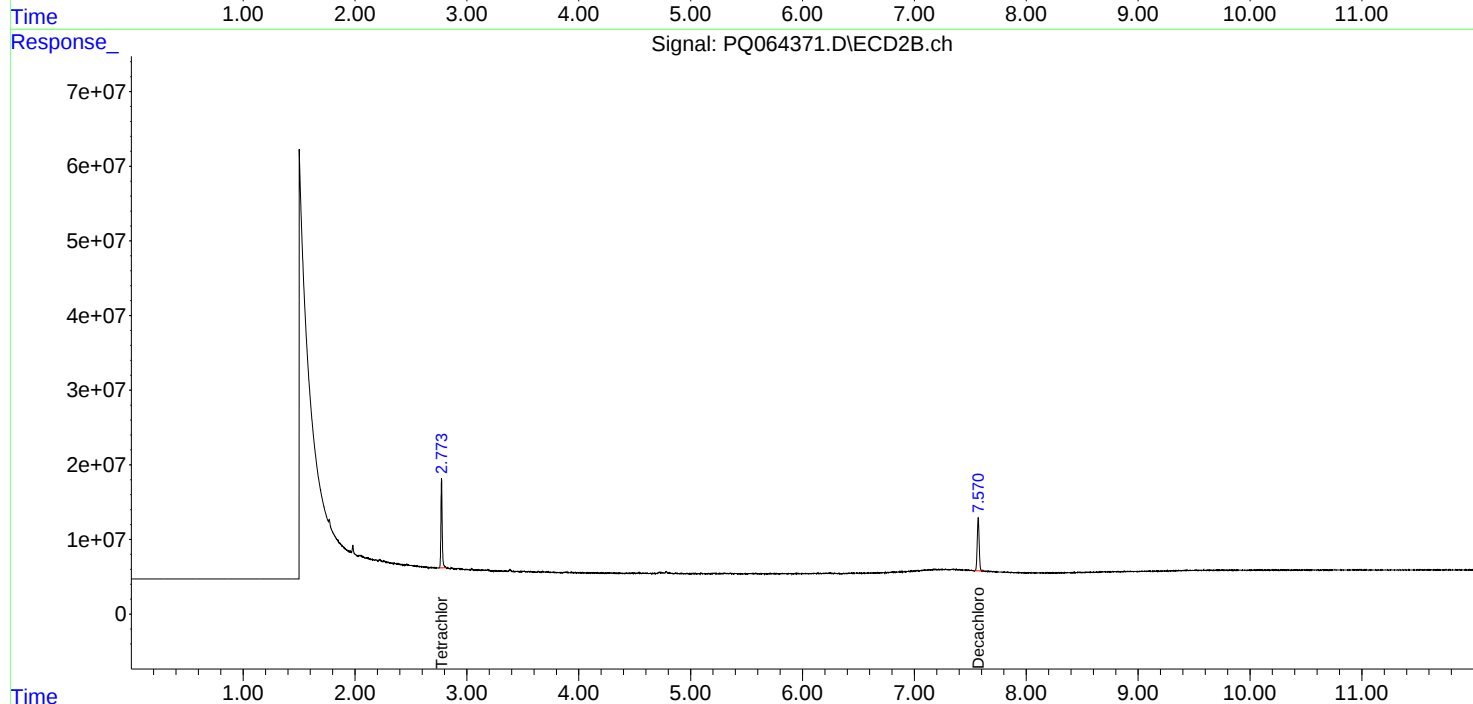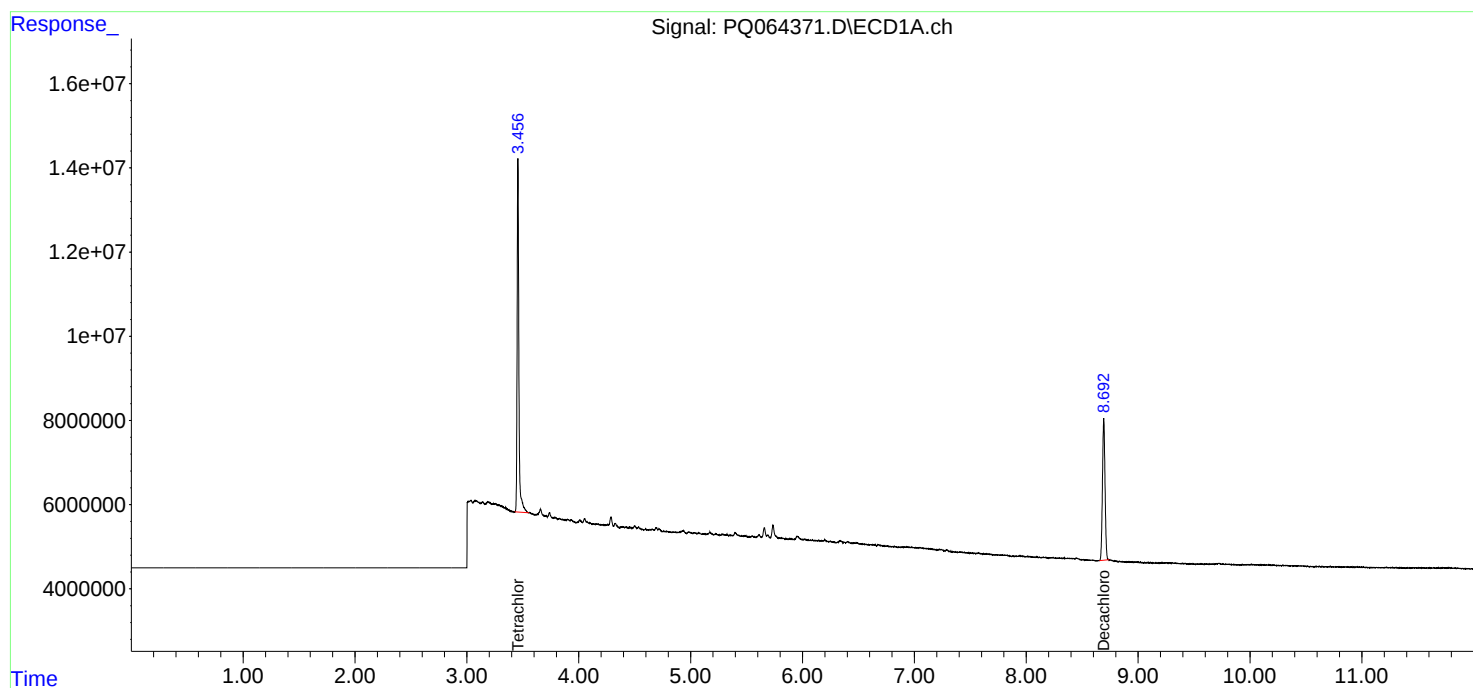


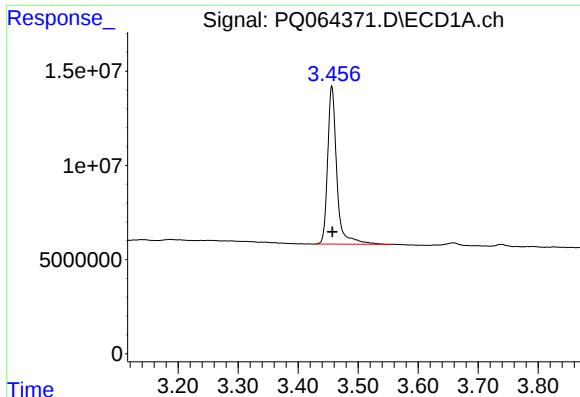

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 89075547
Conc: 21.47 ng/ml

Instrument :
ECD_Q
ClientSampleId :
WC-LIQUID-20231206

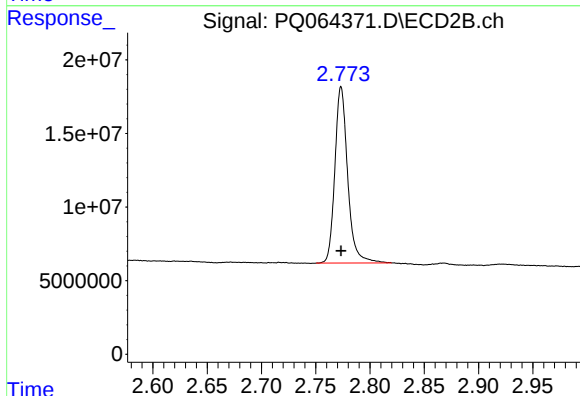


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 98485462
Conc: 23.46 ng/ml

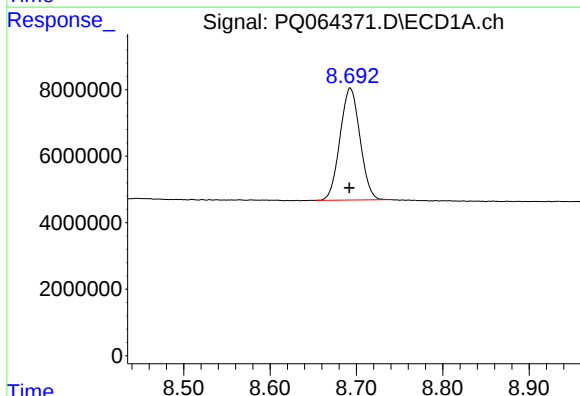

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 54050224
Conc: 18.44 ng/ml

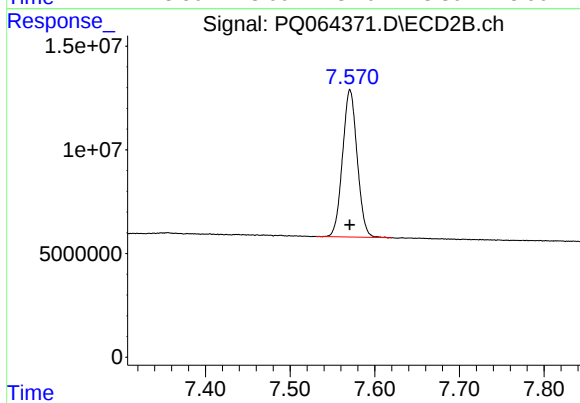

#2 Decachlorobiphenyl

R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 85285275
Conc: 21.13 ng/ml