

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121323\
 Data File : PQ064502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 00:55
 Operator : YP\AJ
 Sample : 05791-11 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MW-1B-EE-NN

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/14/2023
 Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 03:23:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.471	2.773	9362140	11773338	2.257m	2.804m
2) SA Decachlor...	8.718f	7.576	3645022	3687292	1.243m	0.914m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121323\
Data File : PQ064502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 00:55
Operator : YP\AJ
Sample : 05791-11 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
MW-1B-EE-NN


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 03:23:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

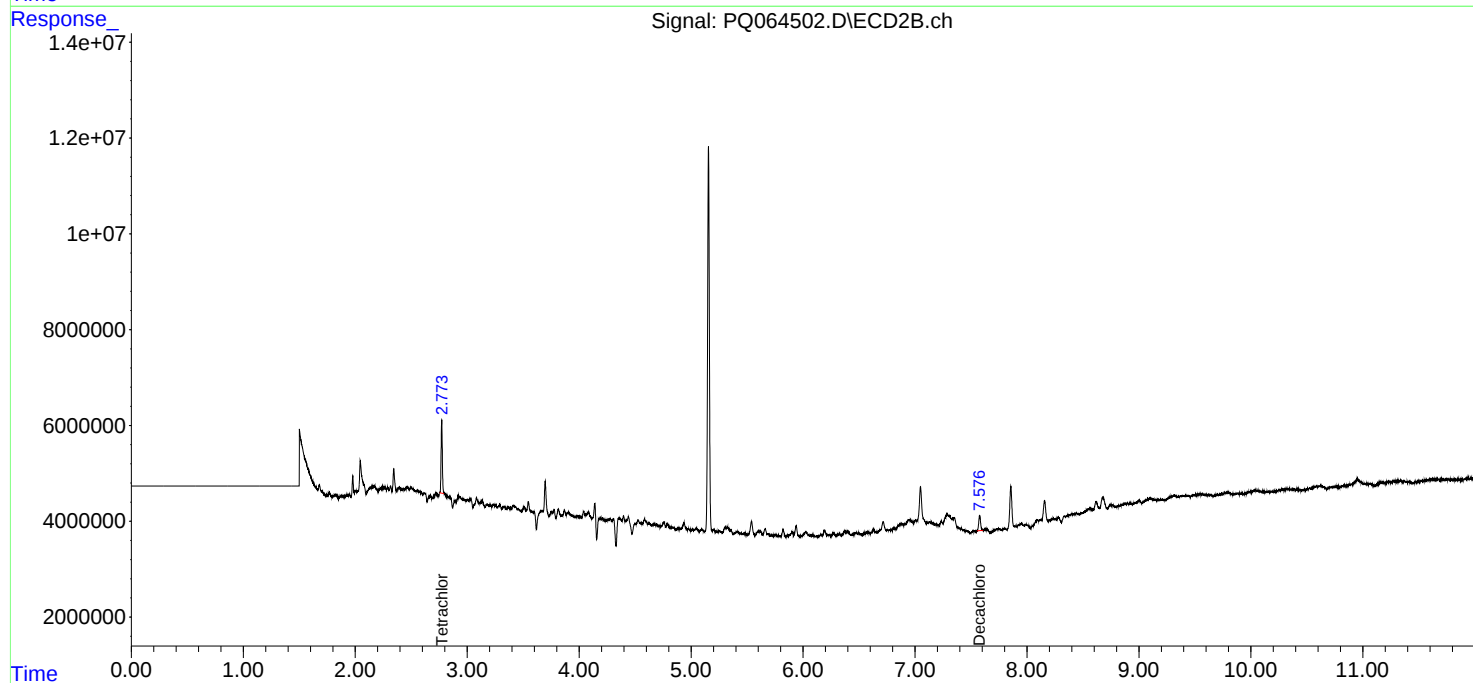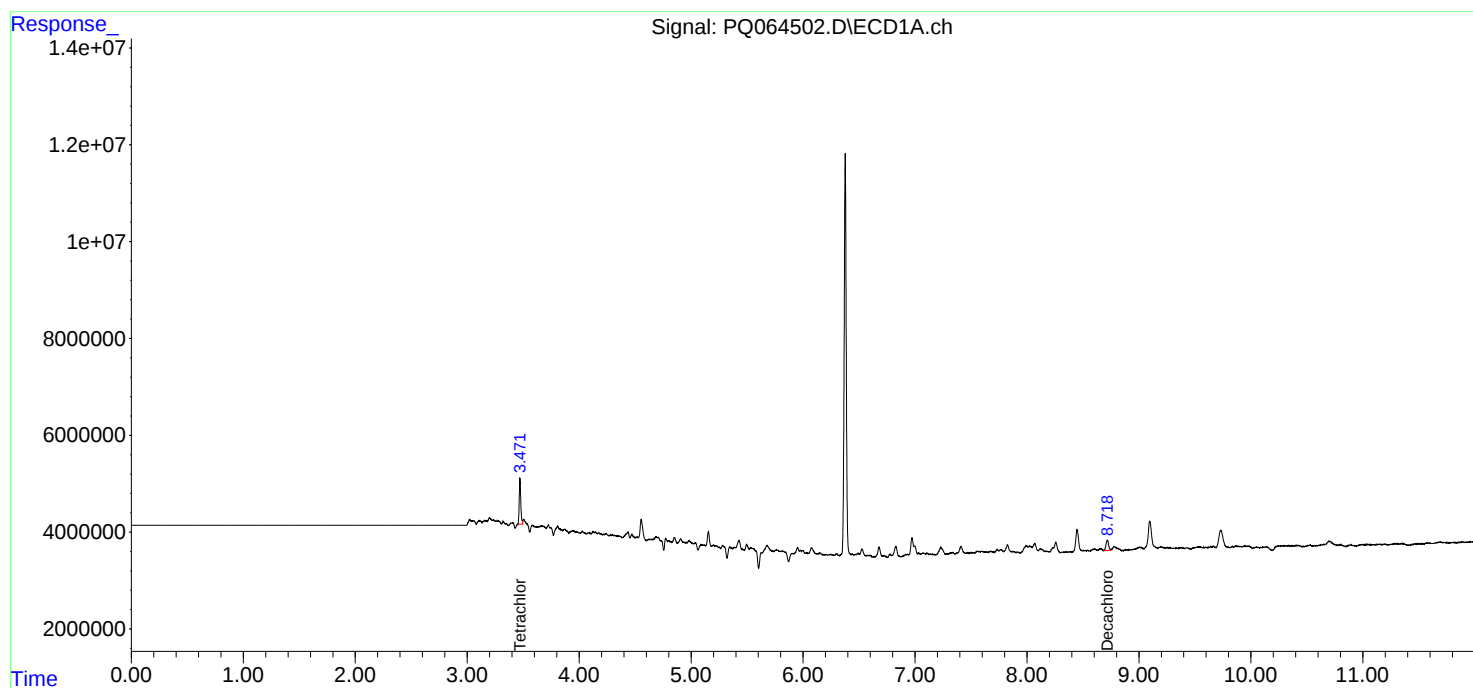

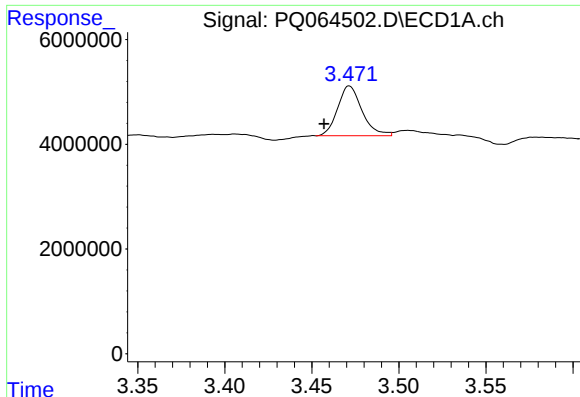


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.014 min
Response: 9362140
Conc: 2.26 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MW-1B-EE-NN


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

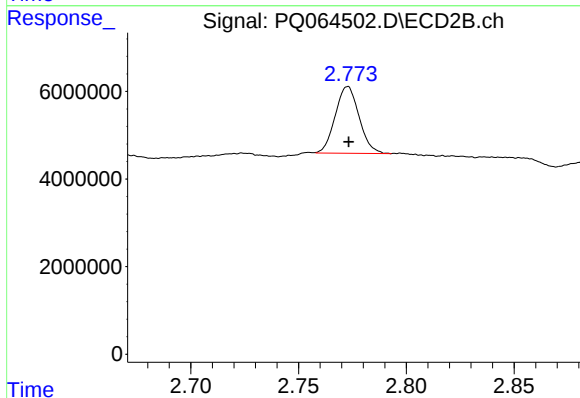


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 11773338
Conc: 2.80 ng/ml m

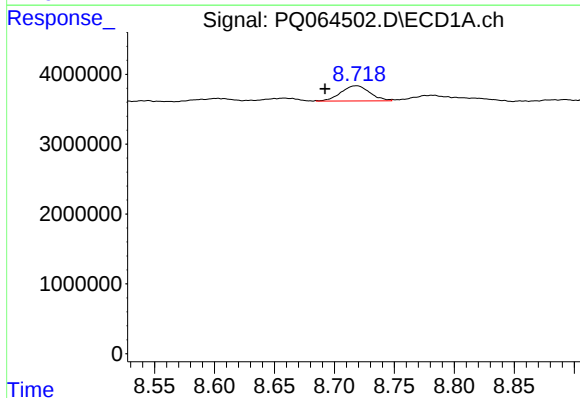

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: 0.026 min
Response: 3645022
Conc: 1.24 ng/ml m

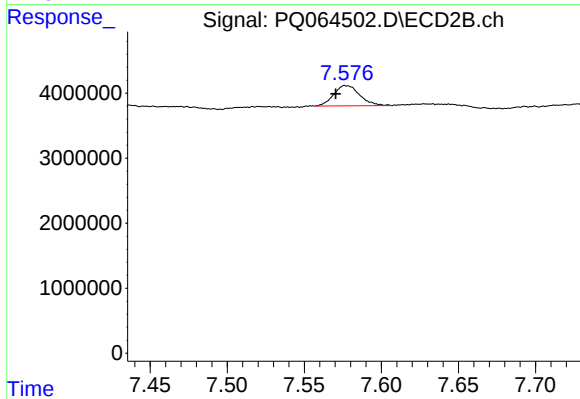

#2 Decachlorobiphenyl

R.T.: 7.576 min
Delta R.T.: 0.005 min
Response: 3687292
Conc: 0.91 ng/ml m