

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121323\
 Data File : PQ064504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 01:26
 Operator : YP\AJ
 Sample : 05768-02 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ELZ-23-00118

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/14/2023
 Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 03:24:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.460	2.772	4172557	5505493	1.006m	1.311 #
2) SA Decachlor...	8.697	7.570	3867294	5920574	1.319m	1.467

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121323\
Data File : PQ064504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 01:26
Operator : YP\AJ
Sample : 05768-02 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ELZ-23-00118


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 03:24:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

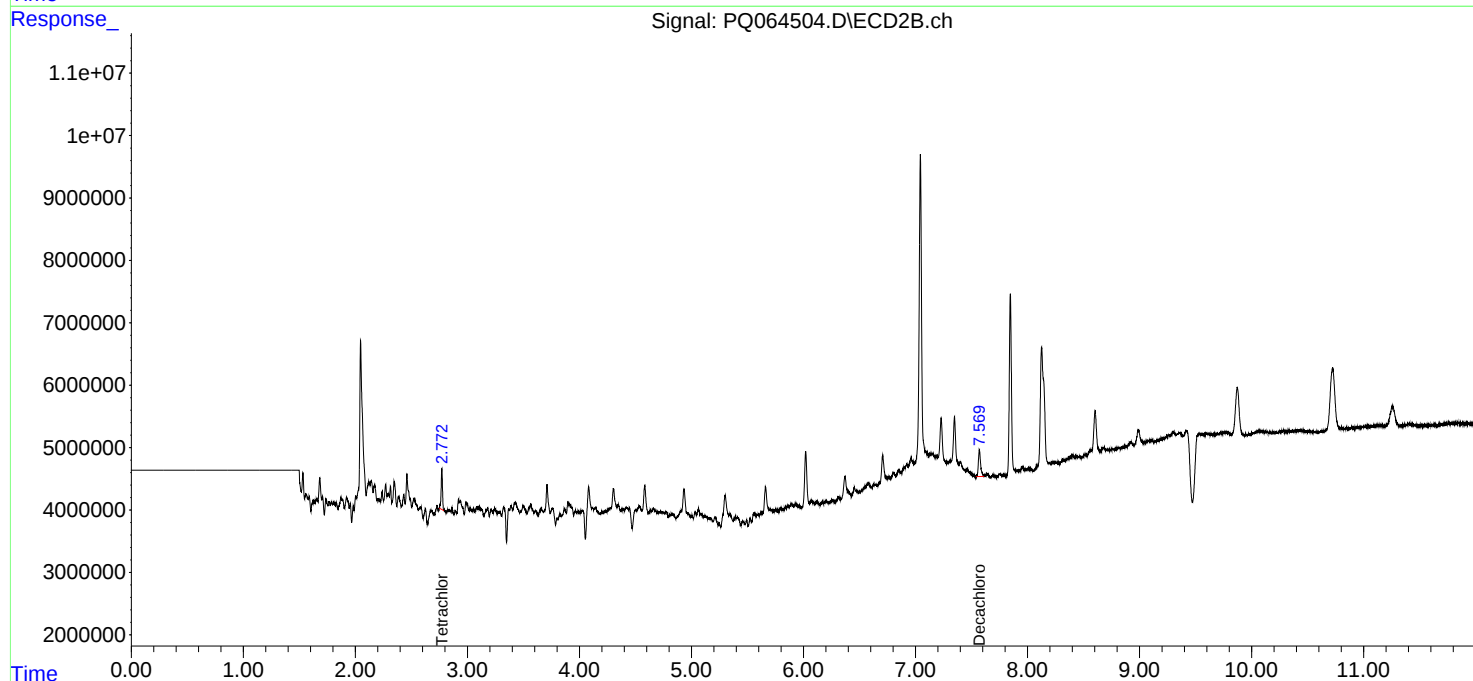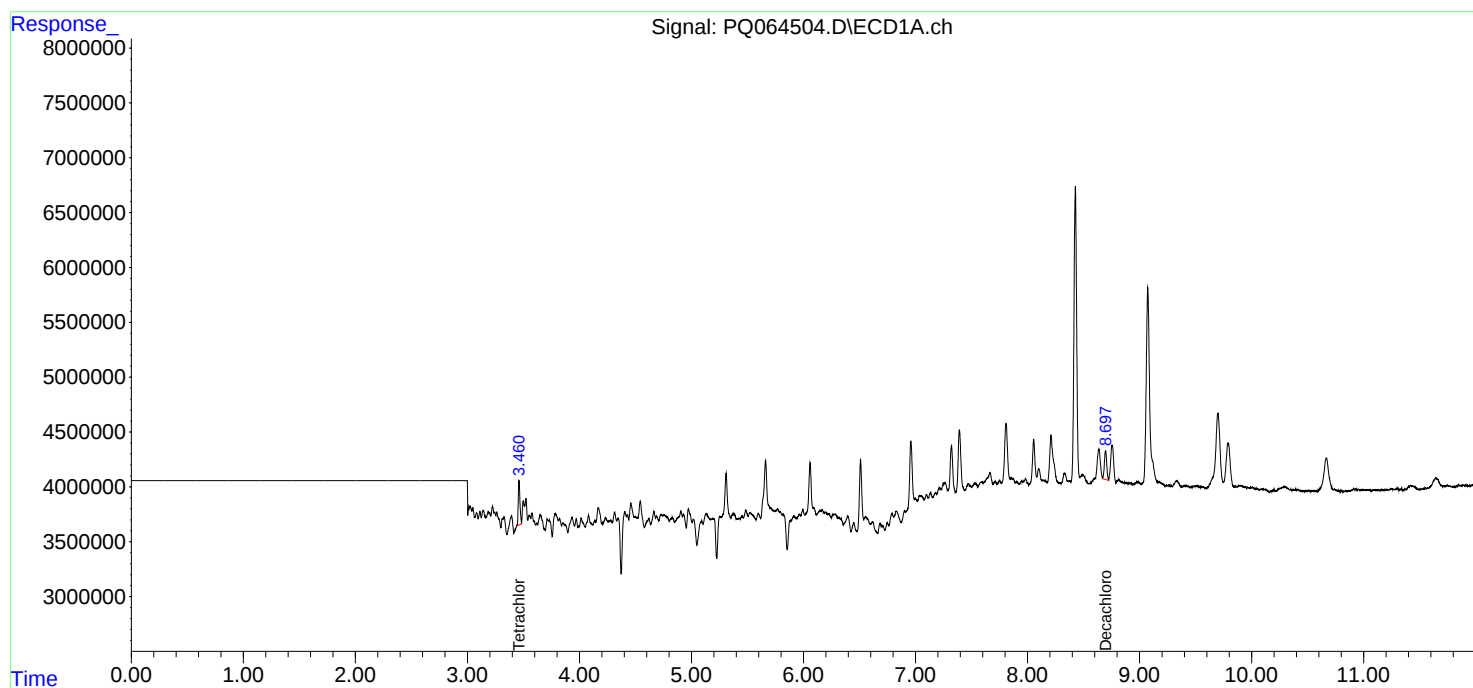

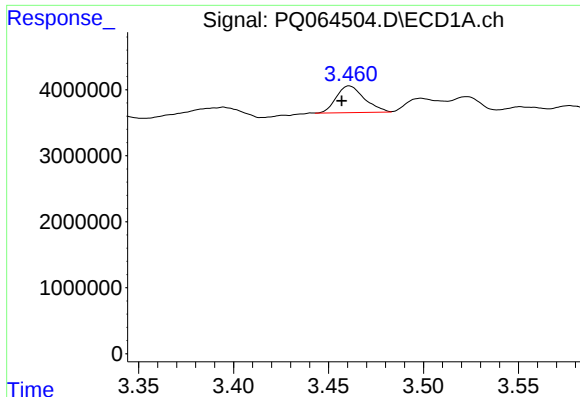

#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.003 min
Response: 4172557
Conc: 1.01 ng/ml

Instrument :

ECD_Q

ClientSampleId :


ELZ-23-00118

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 12/14/2023

Supervised By :Ankita Jodhani 12/14/2023

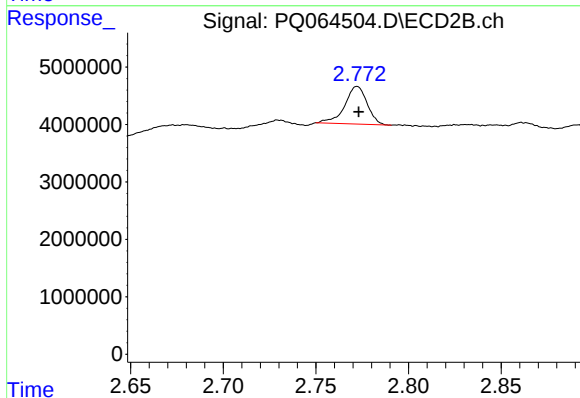


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 5505493
Conc: 1.31 ng/ml

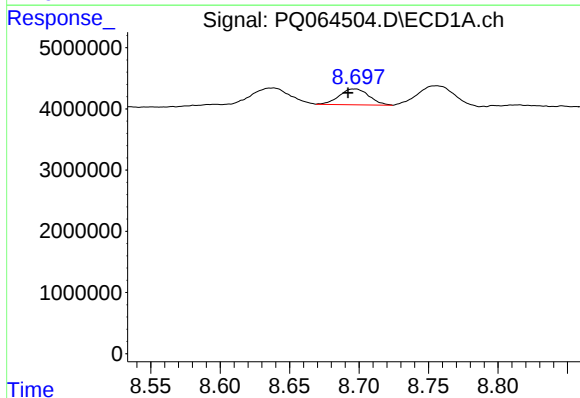

#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: 0.005 min
Response: 3867294
Conc: 1.32 ng/ml m

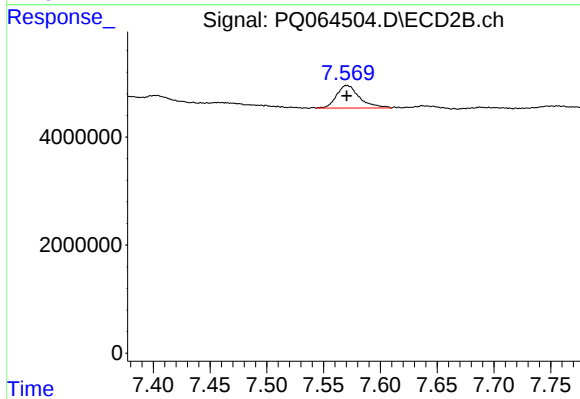

#2 Decachlorobiphenyl

R.T.: 7.570 min
Delta R.T.: 0.000 min
Response: 5920574
Conc: 1.47 ng/ml