

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121323\
 Data File : PQ064505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 01:41
 Operator : YP\AJ
 Sample : 05768-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ELZ-23-00109

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/14/2023
 Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 03:25:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.475	2.770	255.3E6	158.1E6	61.541m	37.656 #
2) SA Decachlor...	8.699	7.575	39624274	37648176	13.517m	9.328m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121323\
Data File : PQ064505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 01:41
Operator : YP\AJ
Sample : 05768-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ELZ-23-00109


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 03:25:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

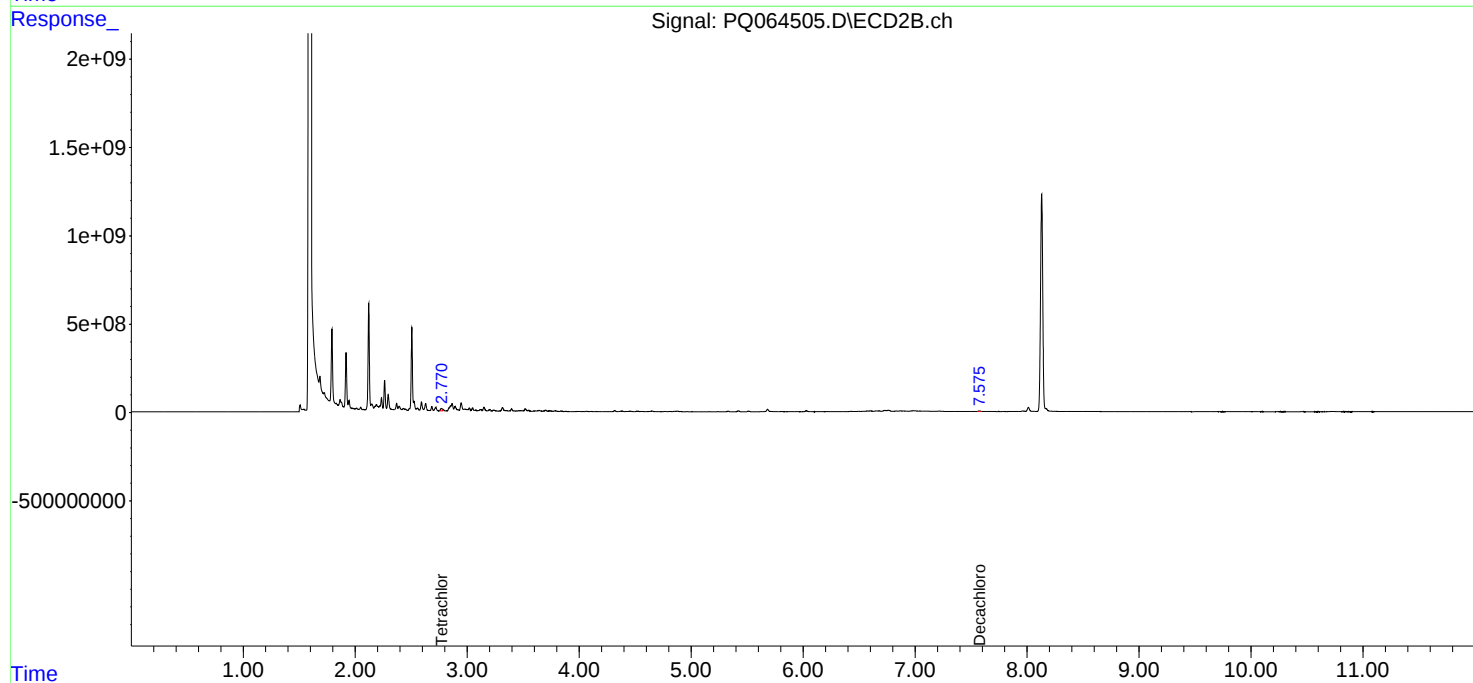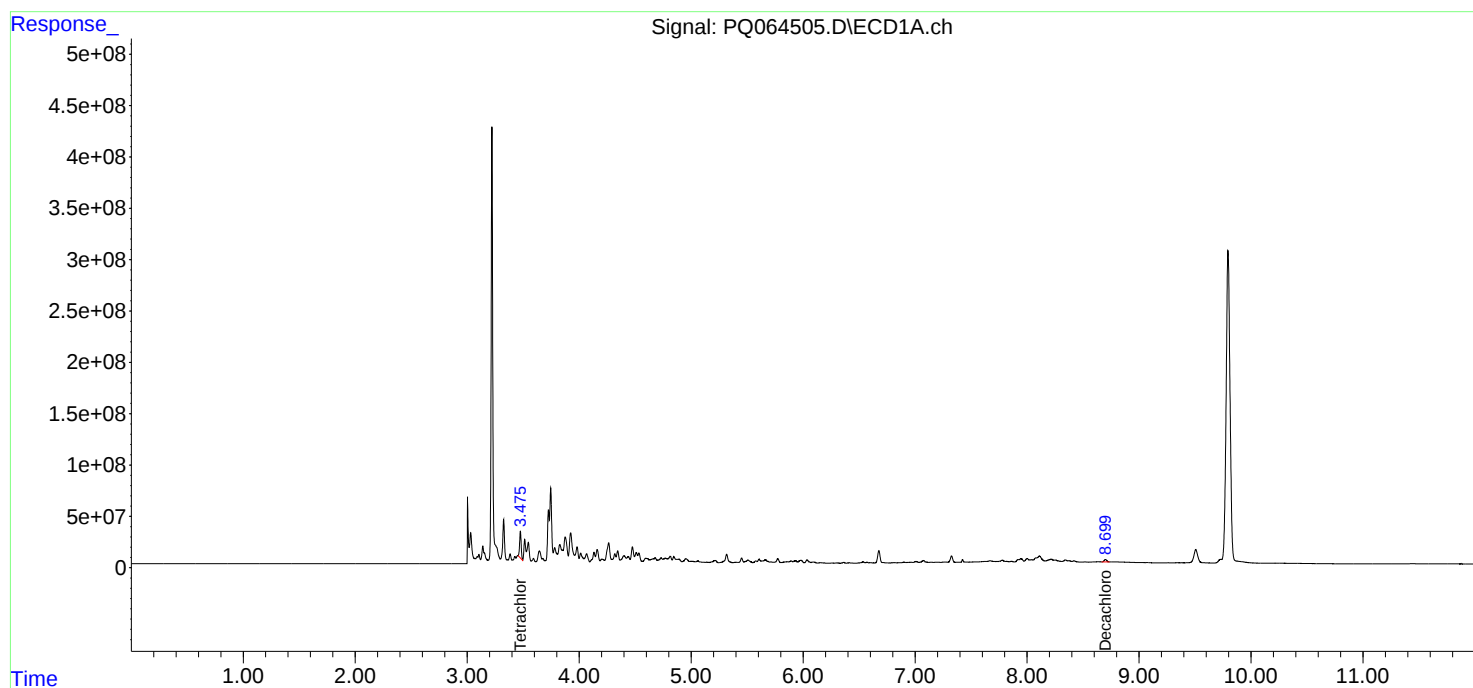

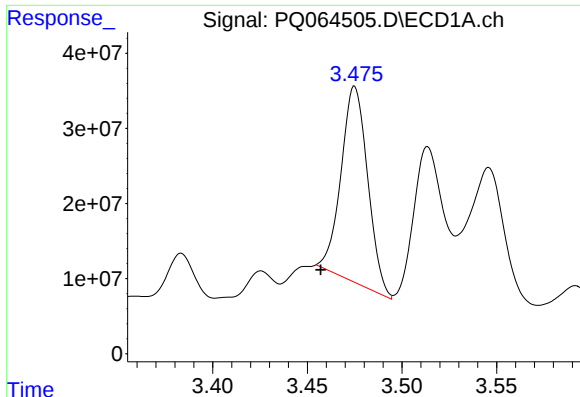


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: 0.018 min
Response: 255310361
Conc: 61.54 ng/ml

Instrument :
ECD_Q
ClientSampleId :
ELZ-23-00109


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :Ankita Jodhani 12/14/2023

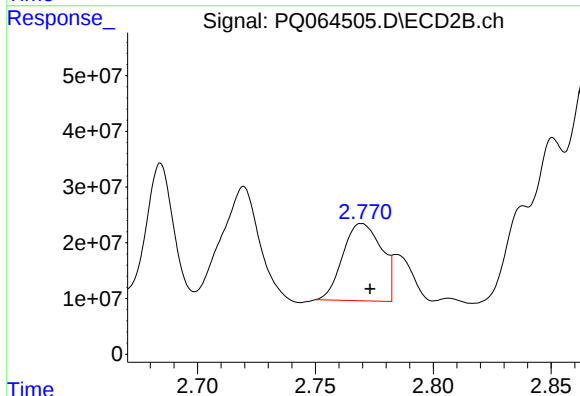


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.003 min
Response: 158096217
Conc: 37.66 ng/ml

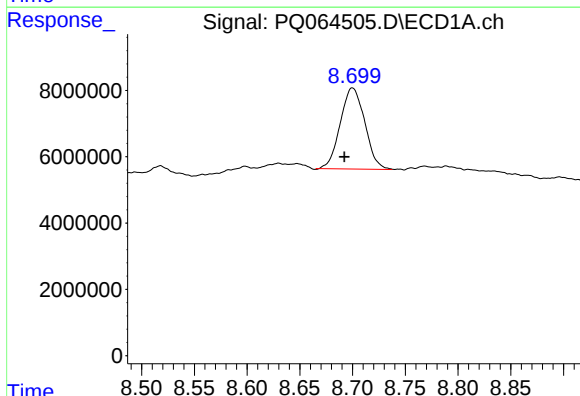

#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: 0.007 min
Response: 39624274
Conc: 13.52 ng/ml m

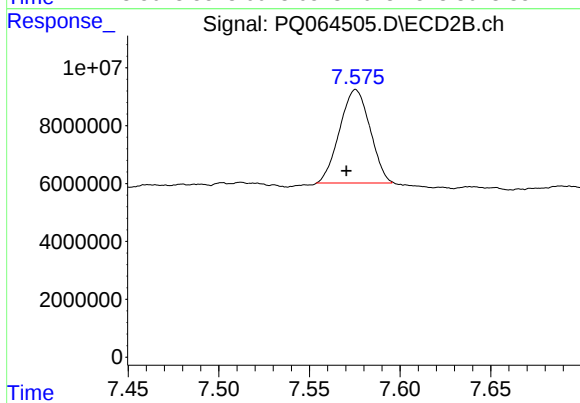

#2 Decachlorobiphenyl

R.T.: 7.575 min
Delta R.T.: 0.005 min
Response: 37648176
Conc: 9.33 ng/ml m