

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ121418\  
Data File : PQ035529.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Dec 2018 22:09  
Operator : SM\SJ  
Sample : J6376-07  
Misc :  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
ECD\_Q  
ClientSampleId :  
TEST-PIT-1-WATER

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 15 01:02:24 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ121318.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Dec 12 22:07:58 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml  |
|-----------------------------|--------|-------|----------|----------|---------|--------|
| -----                       |        |       |          |          |         |        |
| System Monitoring Compounds |        |       |          |          |         |        |
| 1) SA Tetrachlo...          | 4.435  | 3.746 | 93594011 | 53010408 | 23.921  | 23.725 |
| 2) SA Decachlor...          | 10.138 | 8.725 | 58218678 | 35135887 | 19.751m | 19.879 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ121418\  
Data File : PQ035529.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Dec 2018 22:09  
Operator : SM\SJ  
Sample : J6376-07  
Misc :  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
ECD\_Q  
ClientSampleId :  
TEST-PIT-1-WATER

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 15 01:02:24 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ121318.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Dec 12 22:07:58 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

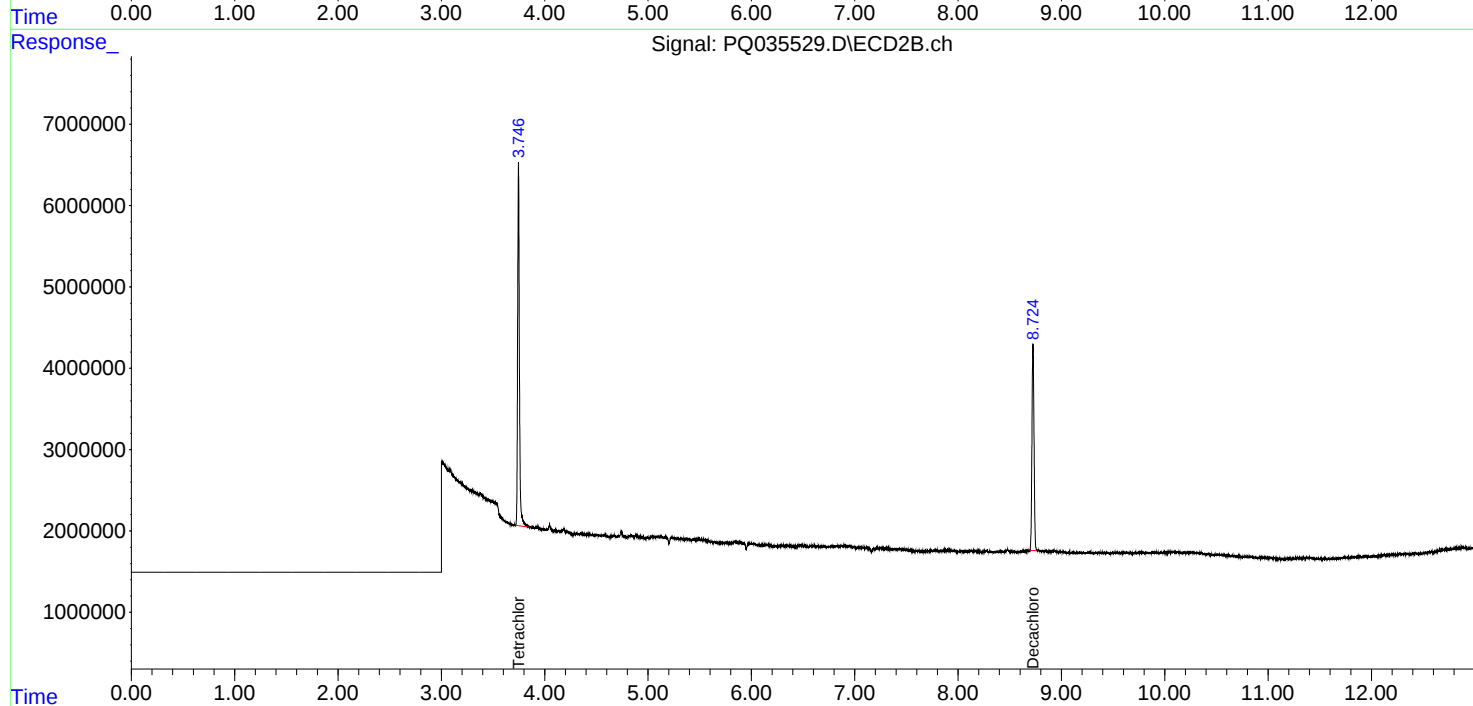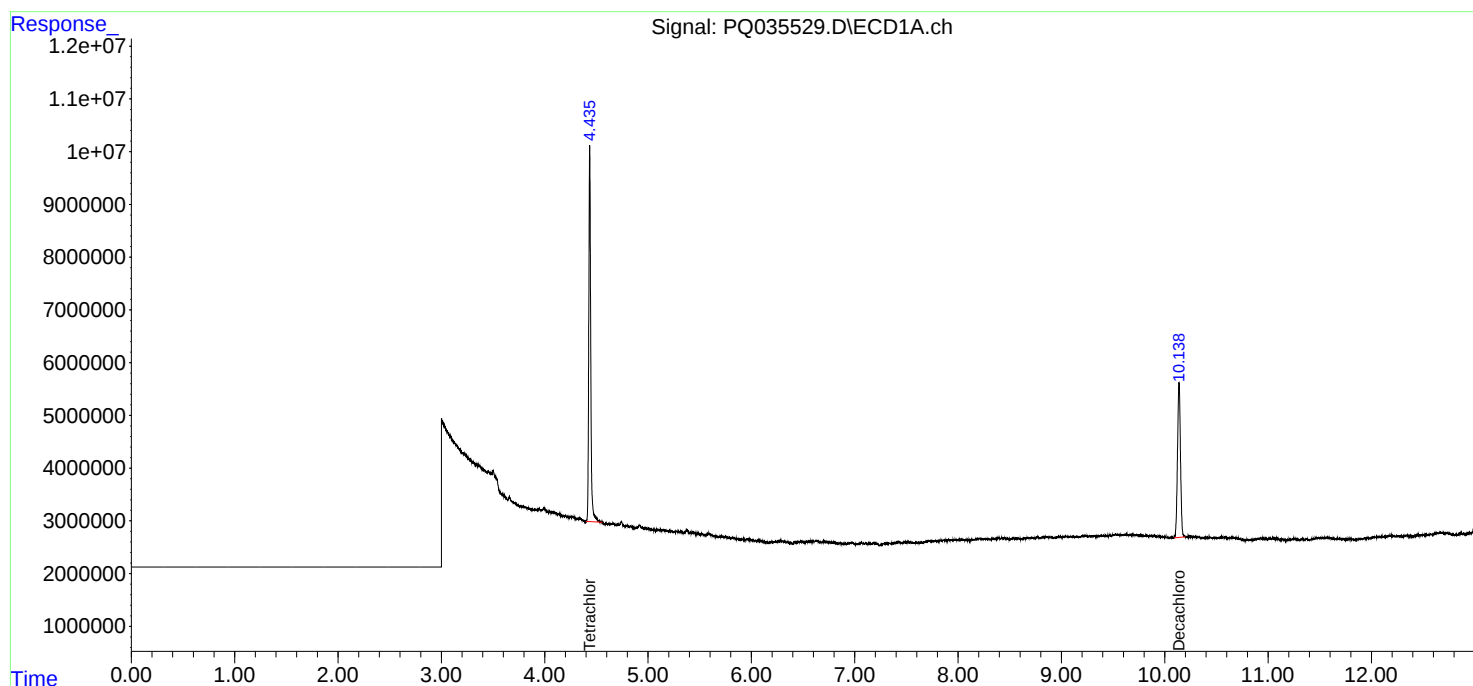


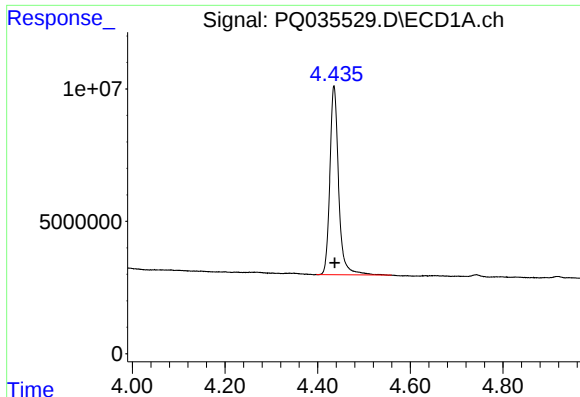

#1 Tetrachloro-m-xylene


R.T.: 4.435 min  
Delta R.T.: -0.002 min  
Response: 93594011  
Conc: 23.92 ng/ml

Instrument :  
ECD\_Q  
ClientSampleId :  
TEST-PIT-1-WATER

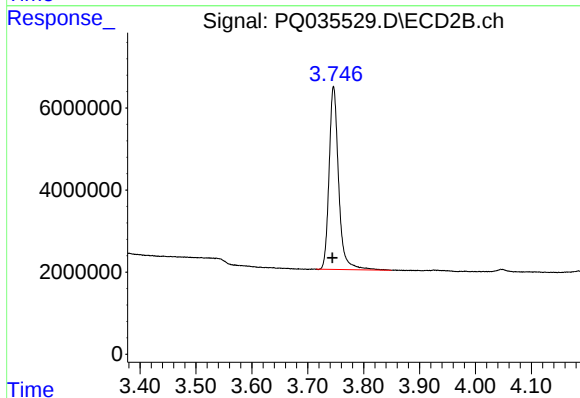


#1 Tetrachloro-m-xylene

R.T.: 3.746 min  
Delta R.T.: 0.002 min  
Response: 53010408  
Conc: 23.72 ng/ml

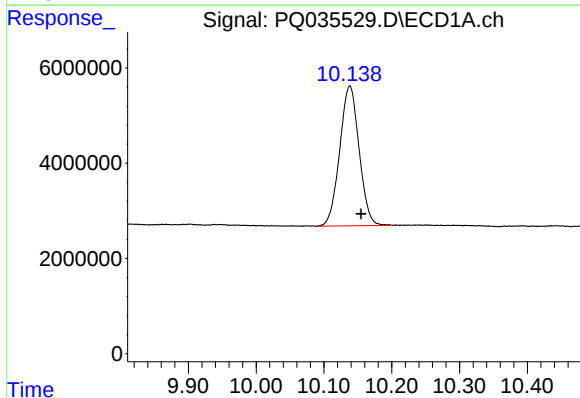

#2 Decachlorobiphenyl

R.T.: 10.138 min  
Delta R.T.: -0.017 min  
Response: 58218678  
Conc: 19.75 ng/ml m

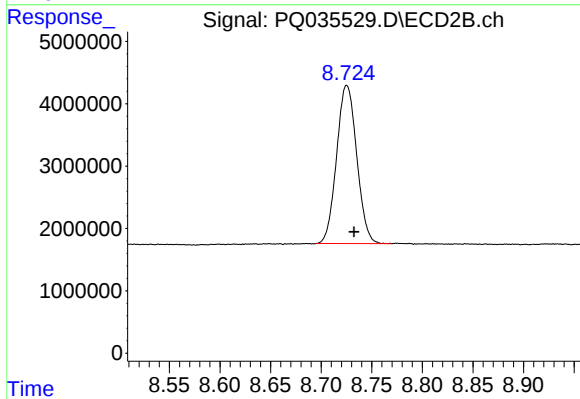

#2 Decachlorobiphenyl

R.T.: 8.725 min  
Delta R.T.: -0.007 min  
Response: 35135887  
Conc: 19.88 ng/ml