

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121523\
 Data File : PQ064569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 16:59
 Operator : YP\AJ
 Sample : 05853-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SOUTH-WALL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/18/2023
 Supervised By :Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 22:34:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.456	2.773	80580584	103.6E6	19.423	24.680 #
2) SA Decachlor...	8.688	7.567	97482223	125.1E6	33.254m	30.999

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121523\
Data File : PQ064569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 16:59
Operator : YP\AJ
Sample : 05853-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SOUTH-WALL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/18/2023
Supervised By :Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 22:34:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

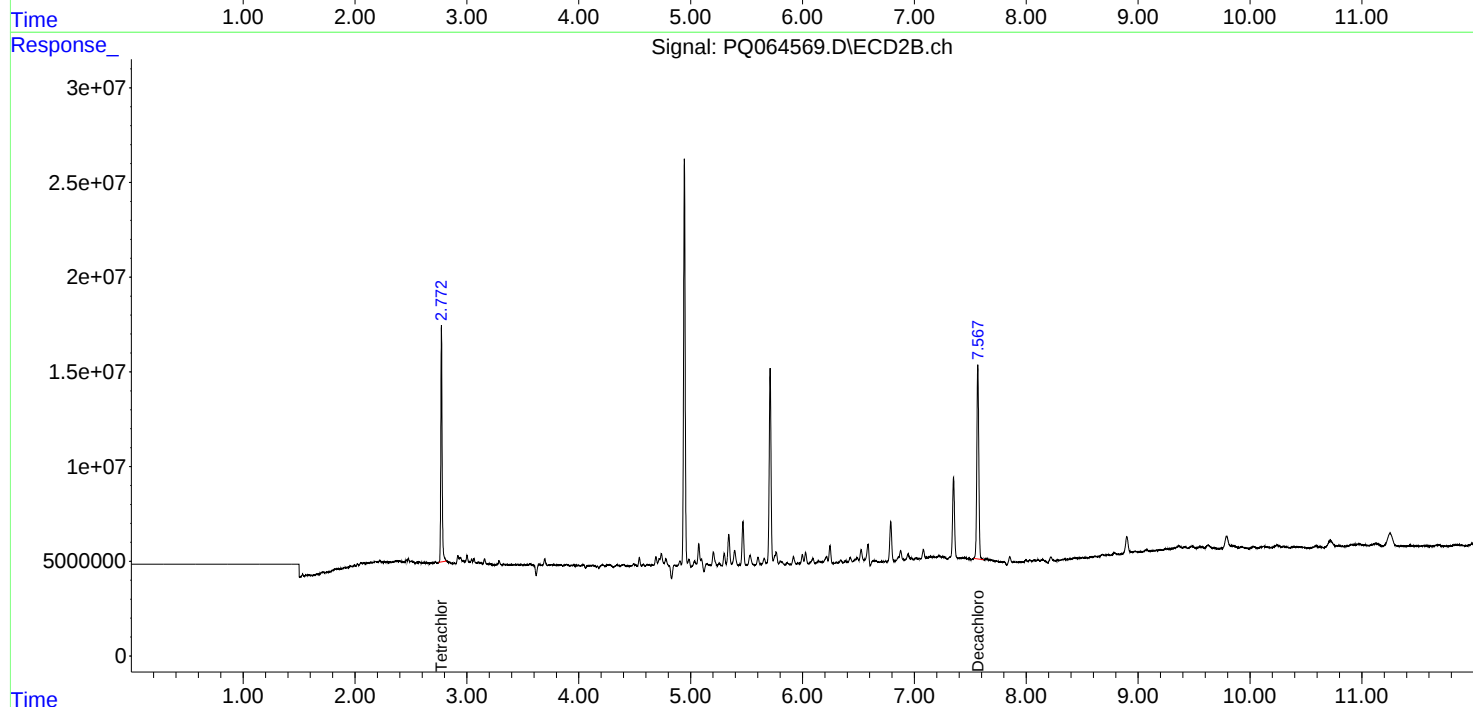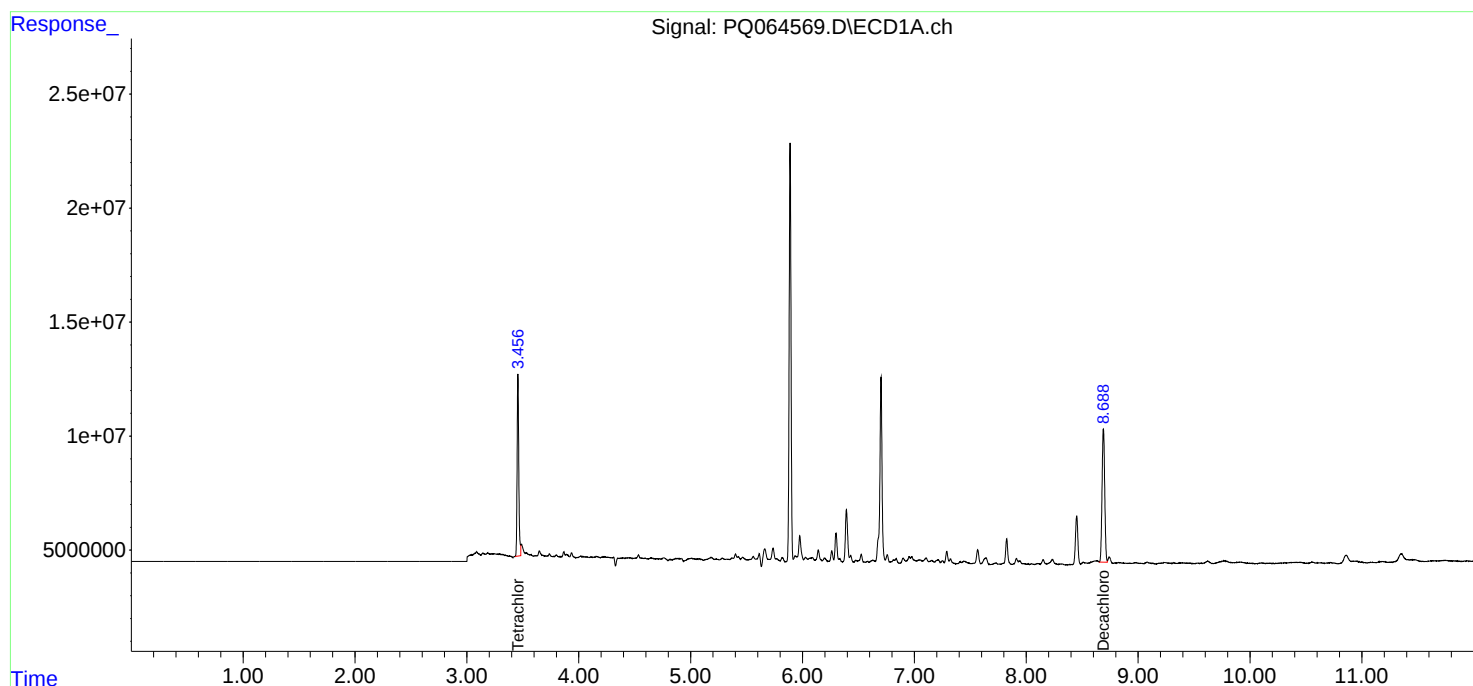

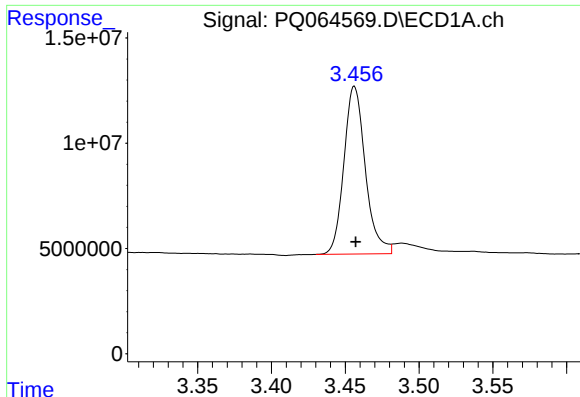


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 80580584
Conc: 19.42 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SOUTH-WALL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/18/2023
Supervised By :Ankita Jodhani 12/18/2023

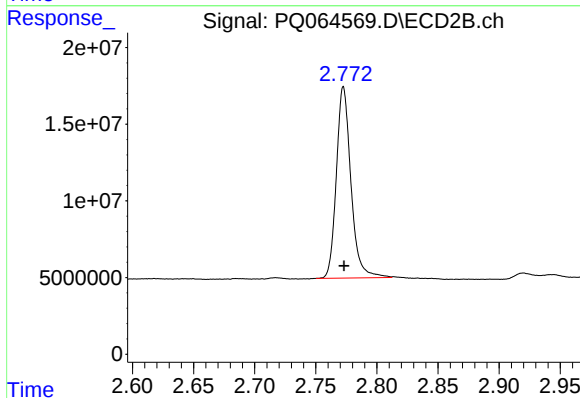


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 103614982
Conc: 24.68 ng/ml

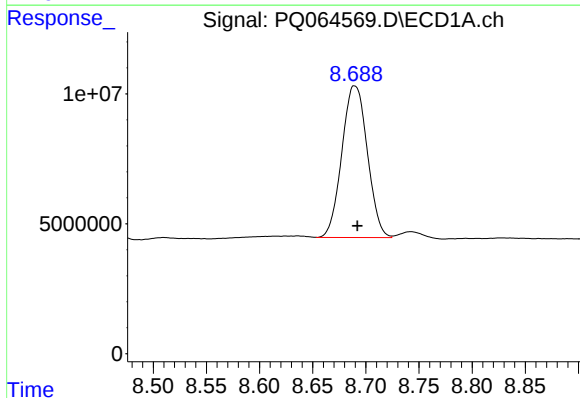

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: -0.004 min
Response: 97482223
Conc: 33.25 ng/ml m

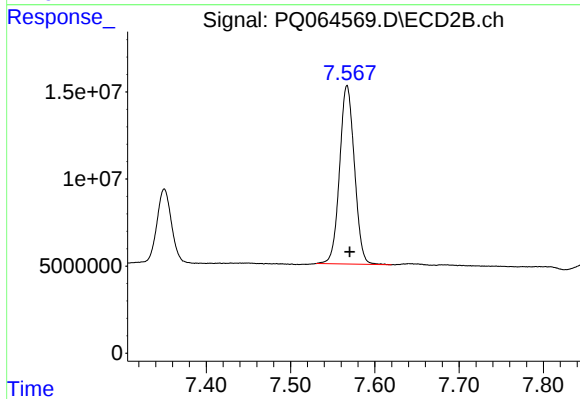

#2 Decachlorobiphenyl

R.T.: 7.567 min
Delta R.T.: -0.003 min
Response: 125117266
Conc: 31.00 ng/ml