

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ122023\
 Data File : PQ064652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2023 20:35
 Operator : YP\AJ
 Sample : 05897-18 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 GHL-SS-22

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/21/2023
 Supervised By :Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 00:27:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.455	2.772	9325551	12945897	2.248	3.084 #
2) SA Decachlor...	8.689	7.567	7414404	13280038	2.529m	3.290 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ122023\
Data File : PQ064652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2023 20:35
Operator : YP\AJ
Sample : 05897-18 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
GHL-SS-22


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2023
Supervised By :Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 00:27:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

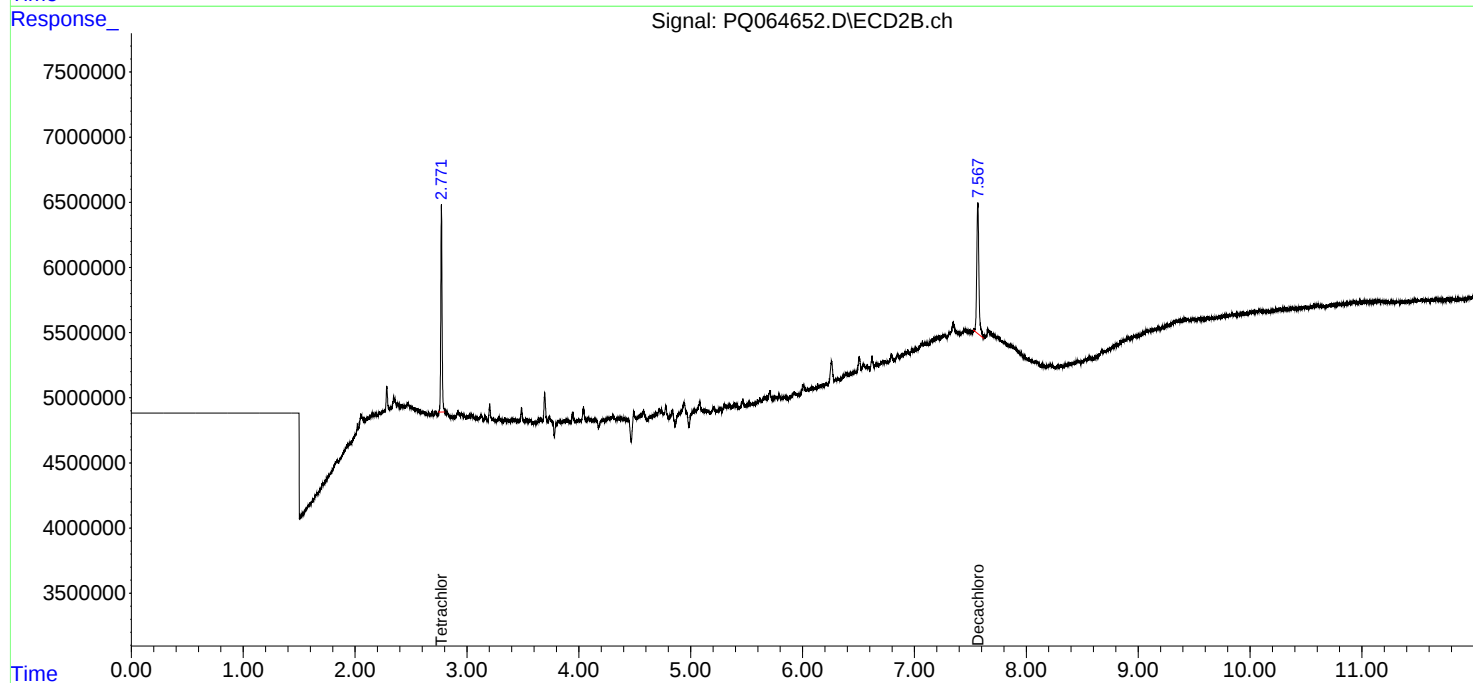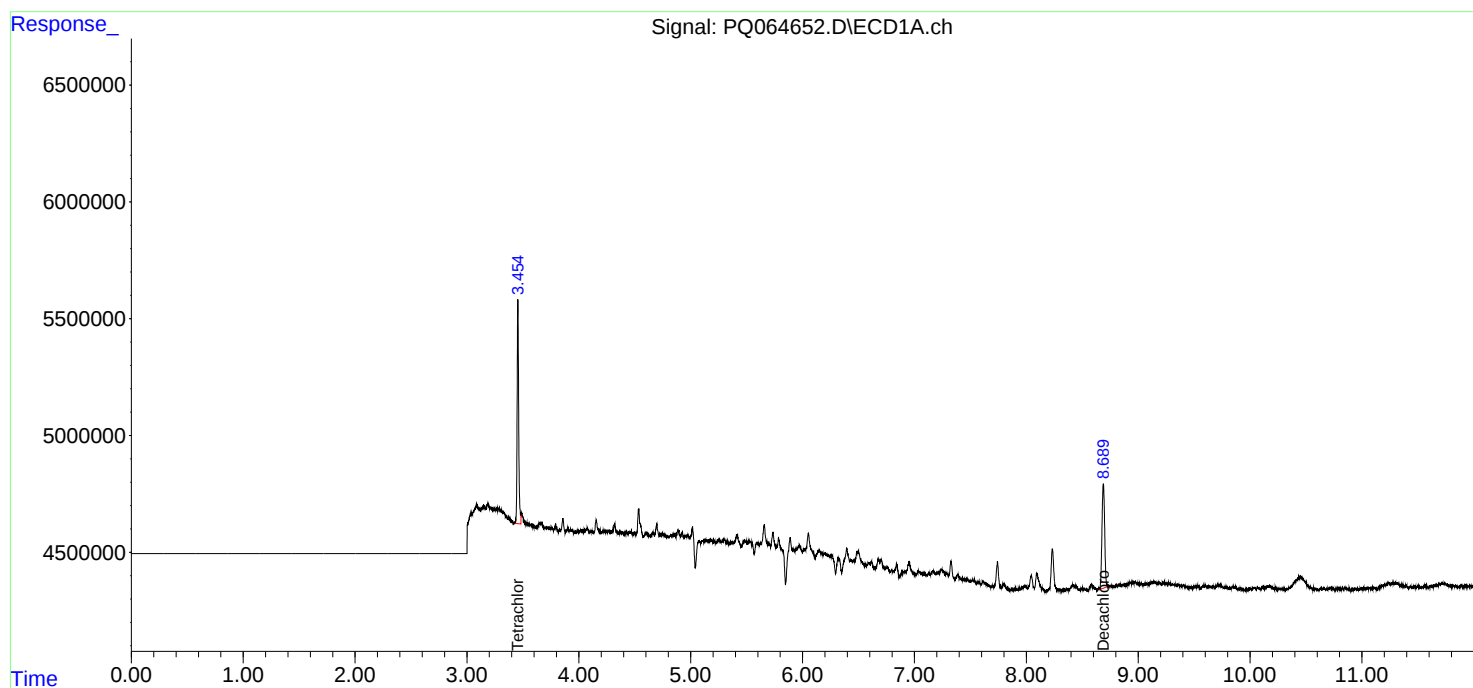

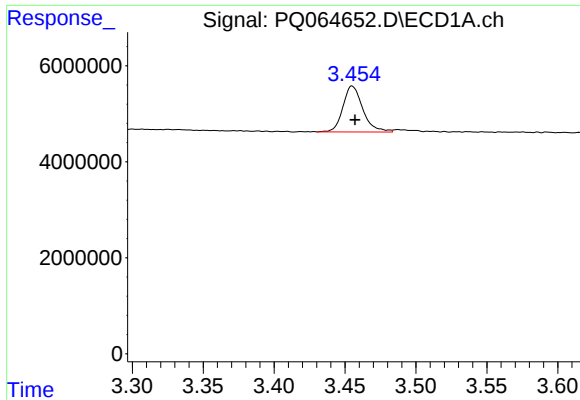


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: -0.002 min
Response: 9325551
Conc: 2.25 ng/ml

Instrument :
ECD_Q
ClientSampleId :
GHL-SS-22


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2023
Supervised By :Ankita Jodhani 12/21/2023

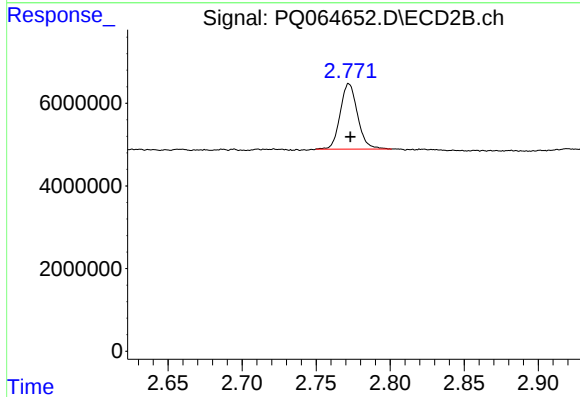


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.001 min
Response: 12945897
Conc: 3.08 ng/ml

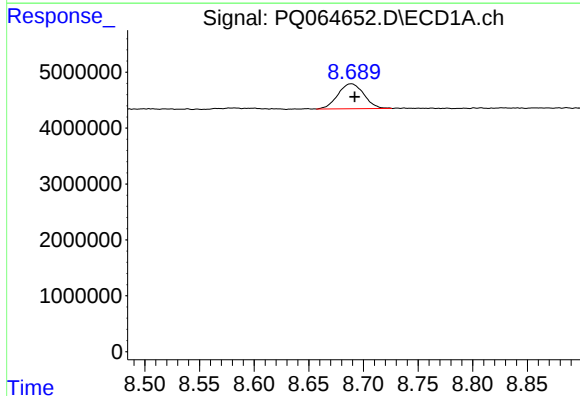

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.003 min
Response: 7414404
Conc: 2.53 ng/ml m

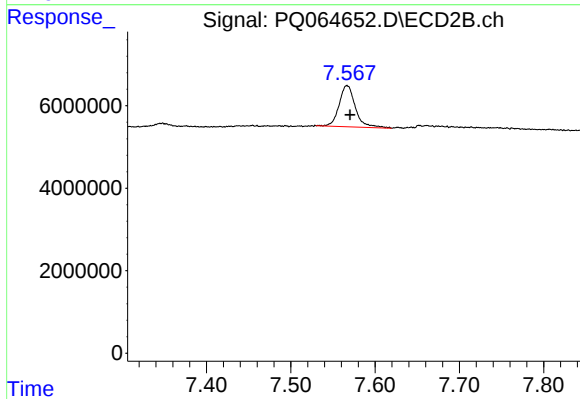

#2 Decachlorobiphenyl

R.T.: 7.567 min
Delta R.T.: -0.004 min
Response: 13280038
Conc: 3.29 ng/ml