

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ122023\
 Data File : PQ064680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 04:39
 Operator : YP\AJ
 Sample : 05929-09
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 CONCRETE-PAD-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 05:22:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 09 05:18:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.456	2.772	85472436	111.6E6	20.603	26.577 #
2) SA Decachlor...	8.688	7.566	59275636	91513385	20.221	22.673

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ122023\
Data File : PQ064680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 04:39
Operator : YP\AJ
Sample : 05929-09
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
CONCRETE-PAD-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 05:22:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 09 05:18:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

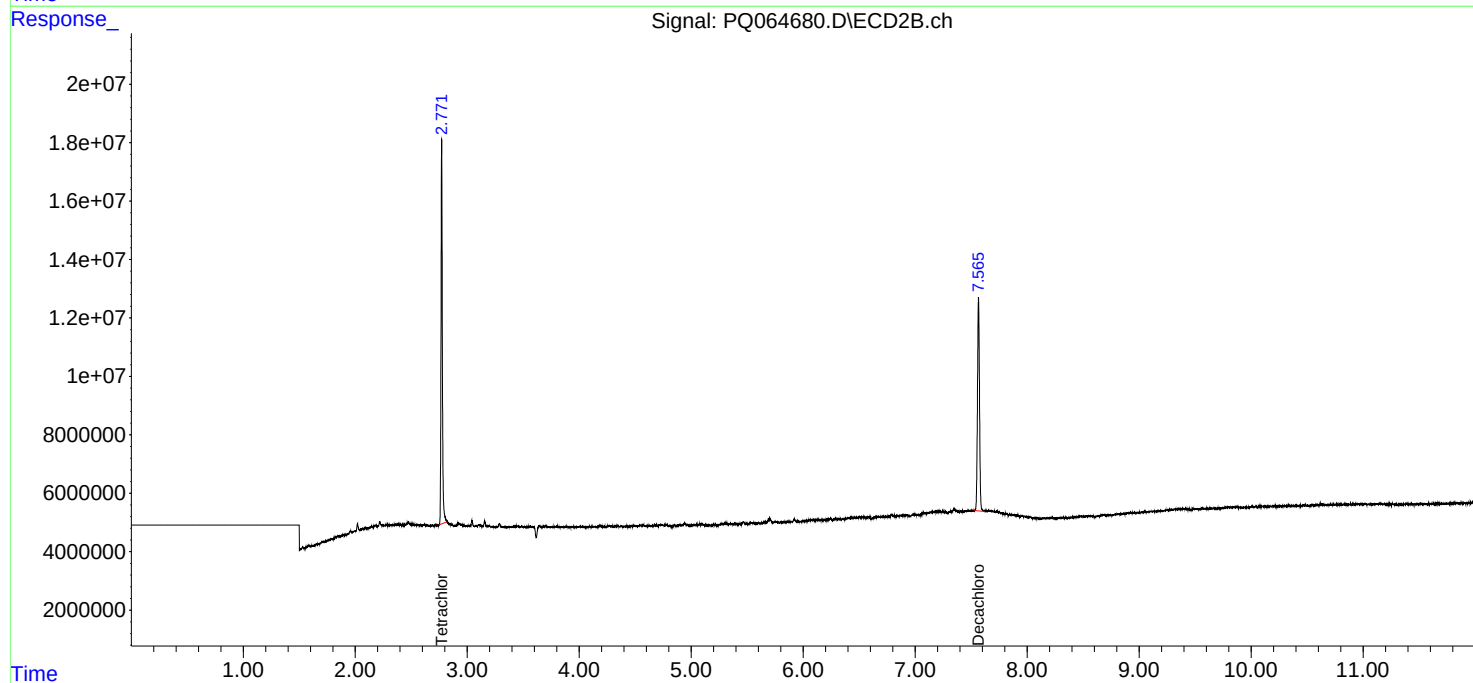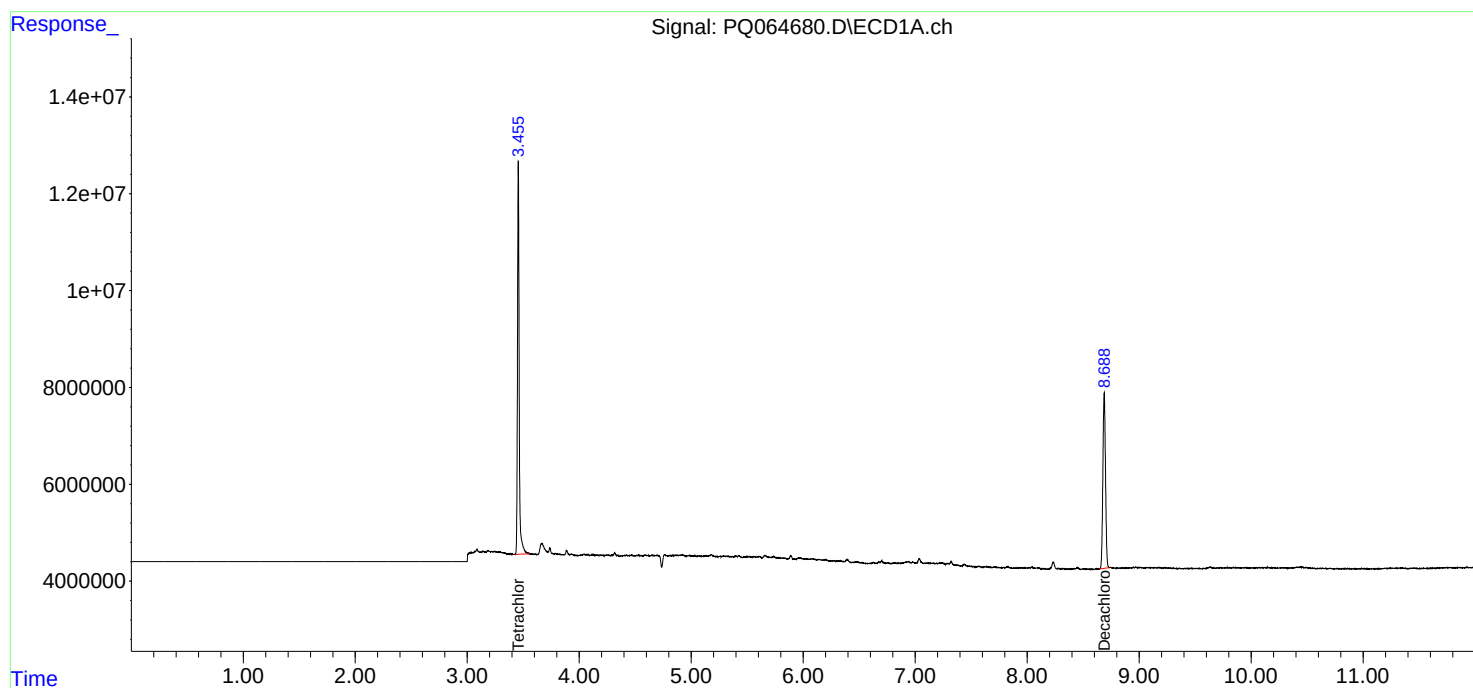


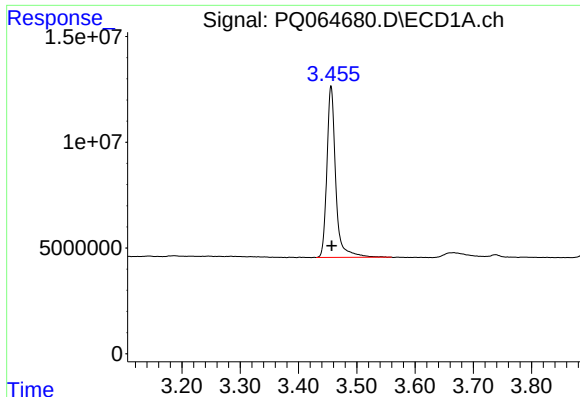

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.001 min
Response: 85472436
Conc: 20.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CONCRETE-PAD-5

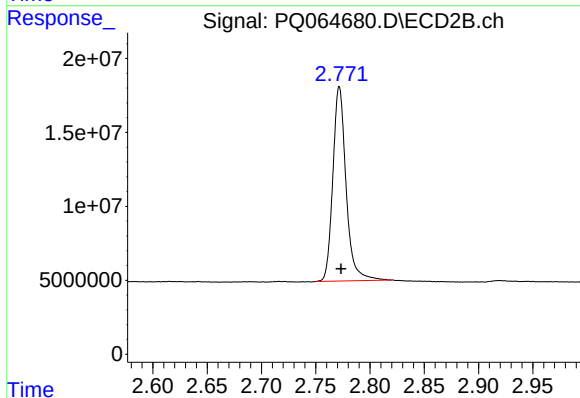


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.001 min
Response: 111580568
Conc: 26.58 ng/ml

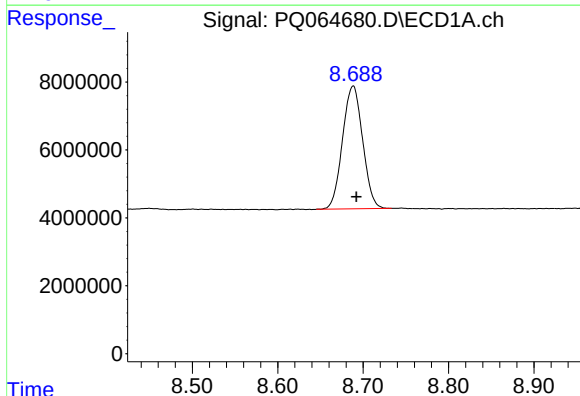

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: -0.004 min
Response: 59275636
Conc: 20.22 ng/ml

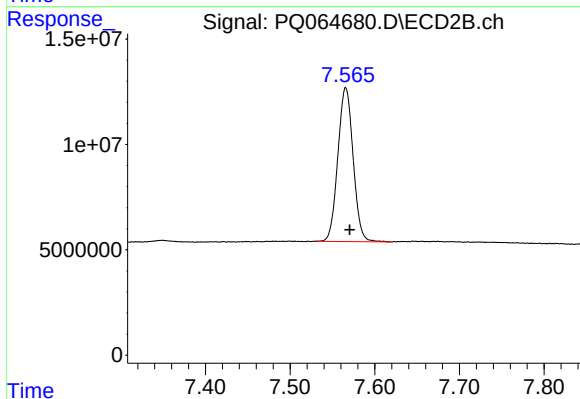

#2 Decachlorobiphenyl

R.T.: 7.566 min
Delta R.T.: -0.005 min
Response: 91513385
Conc: 22.67 ng/ml